

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
 Data File : BM043824.D
 Acq On : 12 Jan 2024 09:35
 Operator : MA/JU
 Sample : PB158339BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK339

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043824.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.351	24	28	38	rVB	66922	105075	1.31%	0.132%
2	3.781	97	101	125	rBV	798732	1553081	19.30%	1.947%
3	4.093	151	154	159	rVB4	12261	14347	0.18%	0.018%
4	7.045	650	656	659	rBV3	10724	17341	0.22%	0.022%
5	7.116	661	668	681	rBV	1070920	1846154	22.94%	2.314%
6	7.286	691	697	710	rBV	919987	1494783	18.57%	1.874%
7	7.475	722	729	741	rBV	1093026	1792555	22.28%	2.247%
8	7.945	802	809	818	rBV	800038	1299030	16.14%	1.628%
9	8.004	818	819	827	rVB8	6075	9741	0.12%	0.012%
10	8.669	923	932	948	rBV	1355177	2329597	28.95%	2.920%
11	9.122	1001	1009	1024	rBV	1106959	1943294	24.15%	2.436%
12	9.486	1066	1071	1077	rBV8	6866	15230	0.19%	0.019%
13	9.845	1125	1132	1143	rBV	964060	1664337	20.68%	2.086%
14	10.386	1216	1224	1245	rBV	1216127	2353905	29.25%	2.951%
15	10.757	1279	1287	1299	rVB	1213340	2058849	25.58%	2.581%
16	10.910	1305	1313	1331	rBV	1268763	2631732	32.70%	3.299%
17	11.980	1492	1495	1500	rVB7	5914	8345	0.10%	0.010%
18	12.363	1555	1560	1569	rVB3	17191	36241	0.45%	0.045%
19	13.486	1747	1751	1757	rBV3	14636	24774	0.31%	0.031%
20	14.010	1834	1840	1853	rVV	2886438	4283235	53.23%	5.369%
21	14.286	1879	1887	1903	rBV	3373566	4952613	61.54%	6.208%
22	14.592	1932	1939	1946	rBV	2095812	3095647	38.47%	3.881%
23	14.821	1969	1978	2002	rBV	1129161	2232645	27.74%	2.799%
24	15.586	2101	2108	2117	rBV	4464599	6300220	78.29%	7.898%
25	15.721	2125	2131	2144	rBV	1380542	2055102	25.54%	2.576%
26	15.827	2146	2149	2156	rVB2	20544	31545	0.39%	0.040%
27	16.080	2189	2192	2198	rVB7	4696	8122	0.10%	0.010%
28	16.368	2234	2241	2247	rVB5	17901	28492	0.35%	0.036%
29	17.015	2347	2351	2356	rVB7	9324	14127	0.18%	0.018%
30	17.345	2400	2407	2416	rBV	2591812	3785351	47.04%	4.745%
31	17.445	2417	2424	2439	rVV	4766136	7056603	87.69%	8.846%
32	17.868	2491	2496	2499	rBV5	5034	10227	0.13%	0.013%
33	18.015	2516	2521	2522	rBV5	6230	8527	0.11%	0.011%
34	18.245	2555	2560	2566	rBV8	20556	39048	0.49%	0.049%
35	19.297	2735	2739	2747	rBV2	56324	77167	0.96%	0.097%
36	19.374	2747	2752	2756	rBV	47363	71489	0.89%	0.090%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
Data File : BM043824.D
Acq On : 12 Jan 2024 09:35
Operator : MA/JU
Sample : PB158339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK339

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Title : SVOA CALIBRATION

37	19.515	2773	2776	2784	rBV9	15865	33907	0.42%	0.043%
38	19.733	2807	2813	2829	rBV	6021158	8047337	100.00%	10.088%
39	21.527	3113	3118	3131	rBV	2877735	4064217	50.50%	5.095%
40	22.091	3211	3214	3221	rVB2	122357	146993	1.83%	0.184%
41	22.709	3316	3319	3325	rVB	185375	265071	3.29%	0.332%
42	23.797	3496	3504	3511	rBV	4007028	7877407	97.89%	9.875%
43	23.950	3523	3530	3544	rVB	1948258	4089840	50.82%	5.127%




Sum of corrected areas: 79773343

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
Data File : BM043824.D
Acq On : 12 Jan 2024 09:35
Operator : MA/JU
Sample : PB158339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK339

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

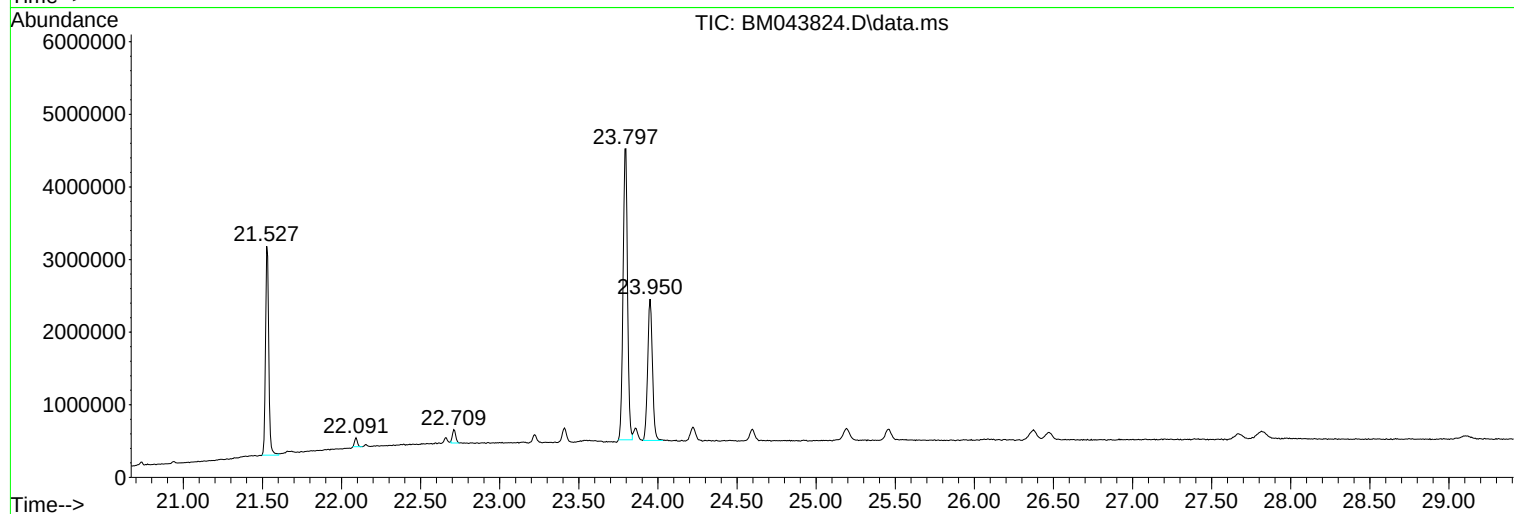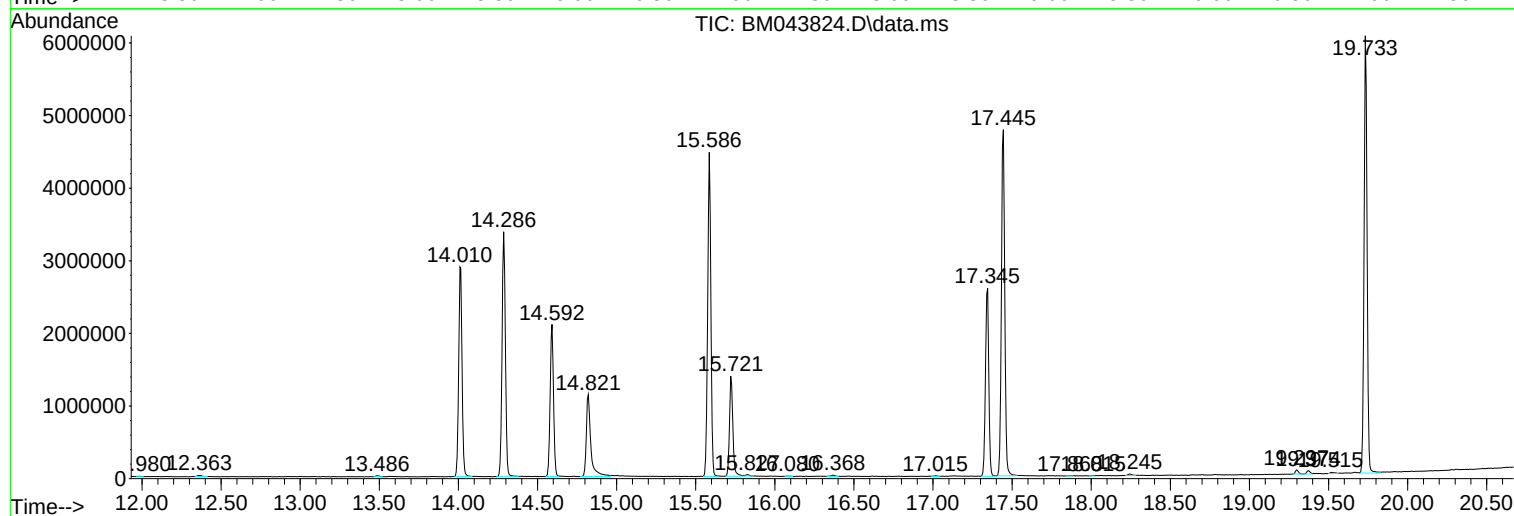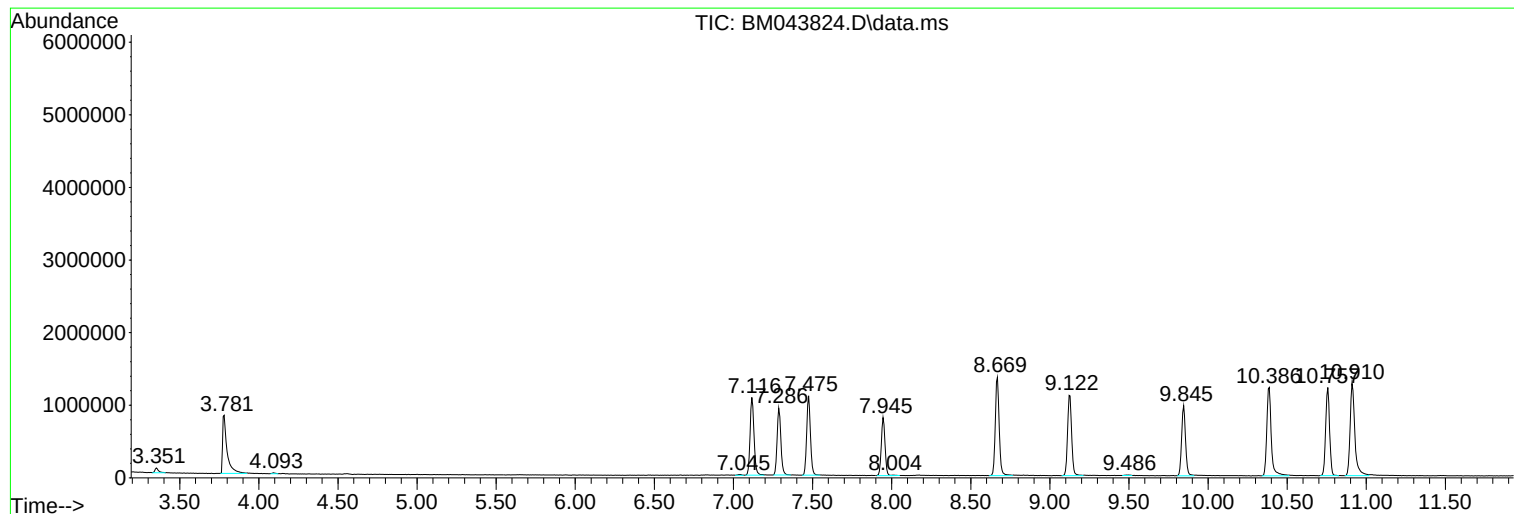

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
Data File : BM043824.D
Acq On : 12 Jan 2024 09:35
Operator : MA/JU
Sample : PB158339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK339

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
Data File : BM043824.D
Acq On : 12 Jan 2024 09:35
Operator : MA/JU
Sample : PB158339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK339

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc