

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
 Data File : BM043828.D
 Acq On : 12 Jan 2024 14:55
 Operator : MA/JU
 Sample : PB158340BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK340

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043828.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.351	24	28	39	rVB	74279	118029	1.74%	0.158%
2	3.775	97	100	122	rBV	828374	1587405	23.44%	2.119%
3	4.093	151	154	162	rVB3	17849	26366	0.39%	0.035%
4	7.116	660	668	687	rBV	1047018	1860073	27.46%	2.483%
5	7.286	690	697	705	rBV	891726	1491665	22.02%	1.991%
6	7.475	721	729	741	rBV	1060680	1827007	26.98%	2.439%
7	7.945	801	809	818	rBV	972221	1620621	23.93%	2.163%
8	8.663	924	931	947	rBV	1337033	2265982	33.46%	3.025%
9	9.122	1001	1009	1022	rBV	1107817	1879819	27.76%	2.509%
10	9.845	1124	1132	1144	rBV	909795	1595989	23.57%	2.130%
11	10.380	1215	1223	1241	rBV	1182685	2240377	33.08%	2.991%
12	10.751	1278	1286	1295	rBV	1419168	2449733	36.17%	3.270%
13	10.910	1305	1313	1334	rBV	1170093	2451365	36.20%	3.272%
14	12.369	1555	1561	1569	rVB3	18647	38975	0.58%	0.052%
15	13.492	1744	1752	1755	rBV6	8334	13710	0.20%	0.018%
16	13.568	1761	1765	1769	rVB5	7252	9348	0.14%	0.012%
17	13.957	1824	1831	1834	rBV6	8323	18489	0.27%	0.025%
18	14.010	1834	1840	1851	rVV	2585876	3756801	55.47%	5.015%
19	14.286	1879	1887	1902	rBV	3017231	4474629	66.07%	5.973%
20	14.592	1931	1939	1952	rBV	2271473	3474450	51.30%	4.638%
21	14.821	1971	1978	2006	rBV	923158	1888220	27.88%	2.521%
22	15.527	2095	2098	2101	rBV3	8590	13208	0.20%	0.018%
23	15.586	2101	2108	2118	rVV	3848611	5543523	81.85%	7.400%
24	15.727	2125	2132	2146	rBV	1088974	1748473	25.82%	2.334%
25	15.821	2146	2148	2157	rVB4	18097	35165	0.52%	0.047%
26	16.362	2236	2240	2245	rVB6	12027	18529	0.27%	0.025%
27	16.462	2251	2257	2261	rBV9	10741	16860	0.25%	0.023%
28	16.780	2305	2311	2316	rBV7	7884	16296	0.24%	0.022%
29	17.127	2358	2370	2375	rBV7	7464	22680	0.33%	0.030%
30	17.345	2400	2407	2417	rBV	2818827	4078503	60.22%	5.444%
31	17.445	2417	2424	2437	rBV	4023412	6053175	89.38%	8.080%
32	18.021	2518	2522	2525	rBV6	8693	13086	0.19%	0.017%
33	18.250	2555	2561	2566	rBV5	20381	37558	0.55%	0.050%
34	18.786	2648	2652	2653	rBV4	8027	8615	0.13%	0.012%
35	19.303	2735	2740	2745	rBV3	48369	71728	1.06%	0.096%
36	19.374	2748	2752	2755	rBV	34465	50966	0.75%	0.068%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
Data File : BM043828.D
Acq On : 12 Jan 2024 14:55
Operator : MA/JU
Sample : PB158340BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK340

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Title : SVOA CALIBRATION

37	19.521	2774	2777	2782	rBV6	13505	20477	0.30%	0.027%
38	19.739	2807	2814	2825	rBV	4881427	6772651	100.00%	9.041%
39	21.533	3114	3119	3129	rBV	3097952	4133501	61.03%	5.518%
40	23.797	3497	3504	3512	rBV2	3488207	6749722	99.66%	9.010%
41	23.956	3524	3531	3544	rVB	2131110	4418143	65.24%	5.898%




Sum of corrected areas: 74911912

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
Data File : BM043828.D
Acq On : 12 Jan 2024 14:55
Operator : MA/JU
Sample : PB158340BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK340

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

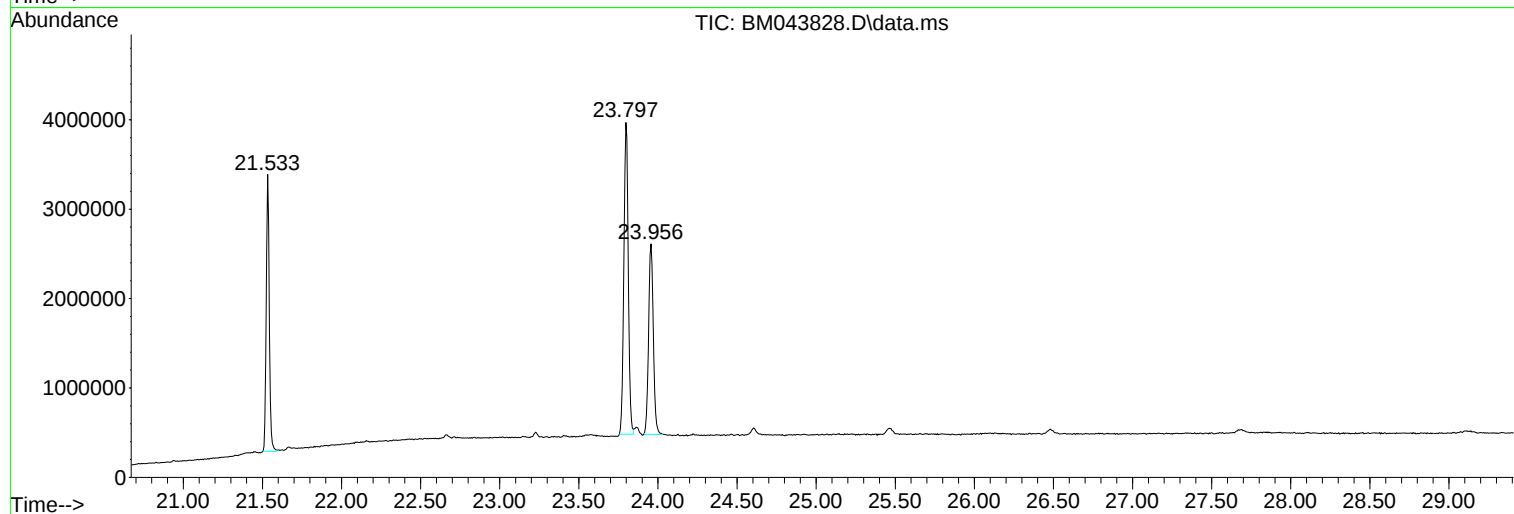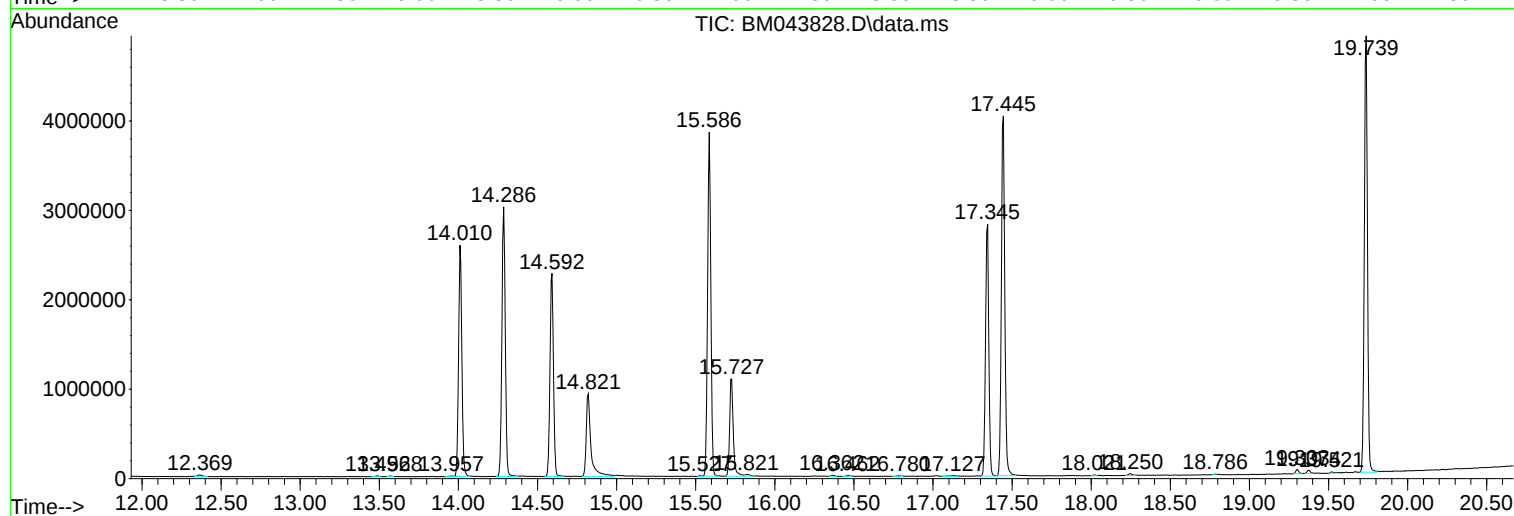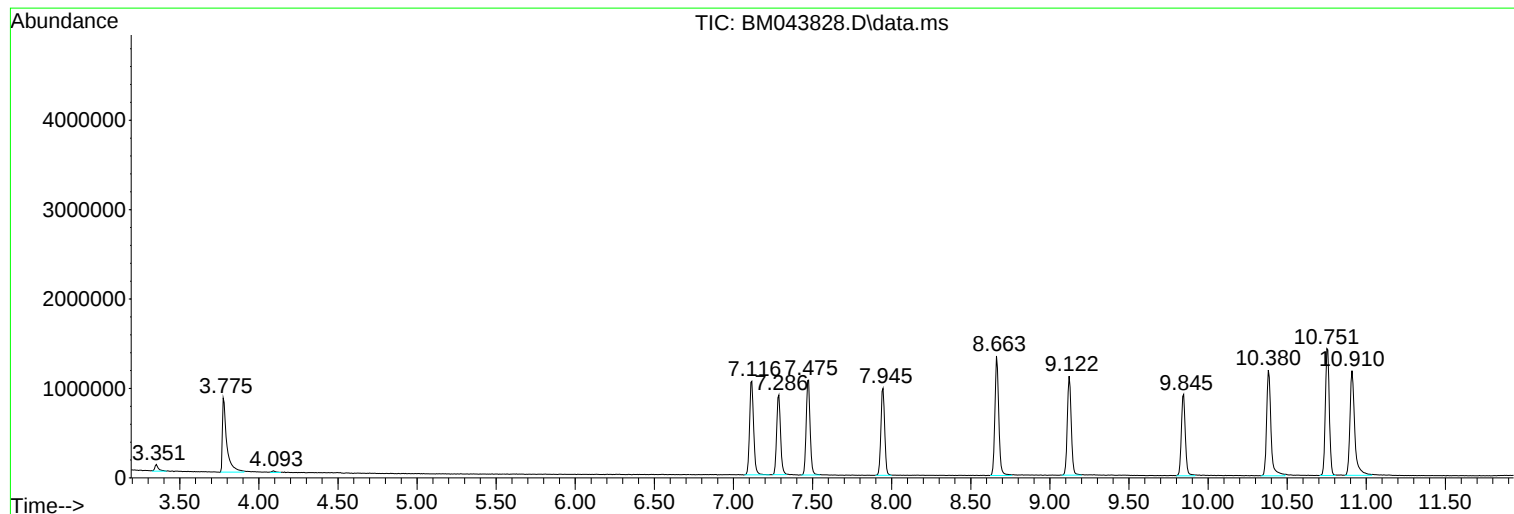

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
Data File : BM043828.D
Acq On : 12 Jan 2024 14:55
Operator : MA/JU
Sample : PB158340BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK340

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
Data File : BM043828.D
Acq On : 12 Jan 2024 14:55
Operator : MA/JU
Sample : PB158340BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK340

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc