

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
 Data File : BM043829.D
 Acq On : 12 Jan 2024 15:31
 Operator : MA/JU
 Sample : PB158341BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK341

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043829.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	39	rVB	92224	145081	1.63%	0.147%
2	3.775	97	100	129	rBV	1115856	2082944	23.36%	2.106%
3	4.093	151	154	161	rVB	20582	29417	0.33%	0.030%
4	7.116	661	668	687	rVB	1403487	2400353	26.92%	2.427%
5	7.287	690	697	708	rBV	1185187	1937095	21.73%	1.959%
6	7.475	721	729	740	rBV	1413146	2344558	26.30%	2.370%
7	7.945	801	809	818	rBV	1323392	2156322	24.19%	2.180%
8	8.663	924	931	945	rBV	1746636	2952846	33.12%	2.986%
9	9.122	1001	1009	1025	rBV	1459831	2466991	27.67%	2.494%
10	9.845	1122	1132	1148	rBV	1206860	2124043	23.82%	2.148%
11	10.381	1214	1223	1246	rBV	1625403	3003104	33.68%	3.036%
12	10.751	1278	1286	1301	rBV	1933074	3331215	37.36%	3.368%
13	10.910	1305	1313	1338	rBV	1576622	3291231	36.91%	3.328%
14	12.369	1554	1561	1569	rBV2	22166	44343	0.50%	0.045%
15	13.486	1742	1751	1758	rBV2	27430	52230	0.59%	0.053%
16	14.010	1833	1840	1855	rBV	3477080	4966451	55.70%	5.021%
17	14.286	1879	1887	1899	rBV	4048485	5917127	66.37%	5.983%
18	14.586	1931	1938	1951	rBV	3107622	4737966	53.14%	4.790%
19	14.816	1969	1977	2001	rBV	1404050	2535697	28.44%	2.564%
20	15.027	2012	2013	2019	rVB6	7693	9715	0.11%	0.010%
21	15.586	2101	2108	2119	rBV	5121394	7395439	82.95%	7.477%
22	15.721	2124	2131	2145	rBV	1565634	2385565	26.76%	2.412%
23	15.827	2145	2149	2153	rVB4	22491	36897	0.41%	0.037%
24	16.368	2235	2241	2246	rBV5	16574	27019	0.30%	0.027%
25	17.021	2348	2352	2355	rVB6	9018	11222	0.13%	0.011%
26	17.339	2399	2406	2416	rBV	3833304	5570201	62.47%	5.632%
27	17.439	2416	2423	2442	rVV	5475048	8056955	90.37%	8.146%
28	18.251	2558	2561	2565	rBV6	6838	11809	0.13%	0.012%
29	19.298	2735	2739	2746	rBV3	56171	79607	0.89%	0.080%
30	19.374	2747	2752	2756	rVV	48051	65696	0.74%	0.066%
31	19.733	2807	2813	2826	rBV	6494516	8915934	100.00%	9.015%
32	21.533	3113	3119	3132	rBV	3949790	5583847	62.63%	5.646%
33	23.797	3496	3504	3512	rBV	4470209	8484129	95.16%	8.578%
34	23.950	3523	3530	3545	rVB	2758403	5752656	64.52%	5.816%

Sum of corrected areas: 98905705

Instrument :

BNA_M

ClientSampleId :




SBLK341

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
Data File : BM043829.D
Acq On : 12 Jan 2024 15:31
Operator : MA/JU
Sample : PB158341BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK341

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

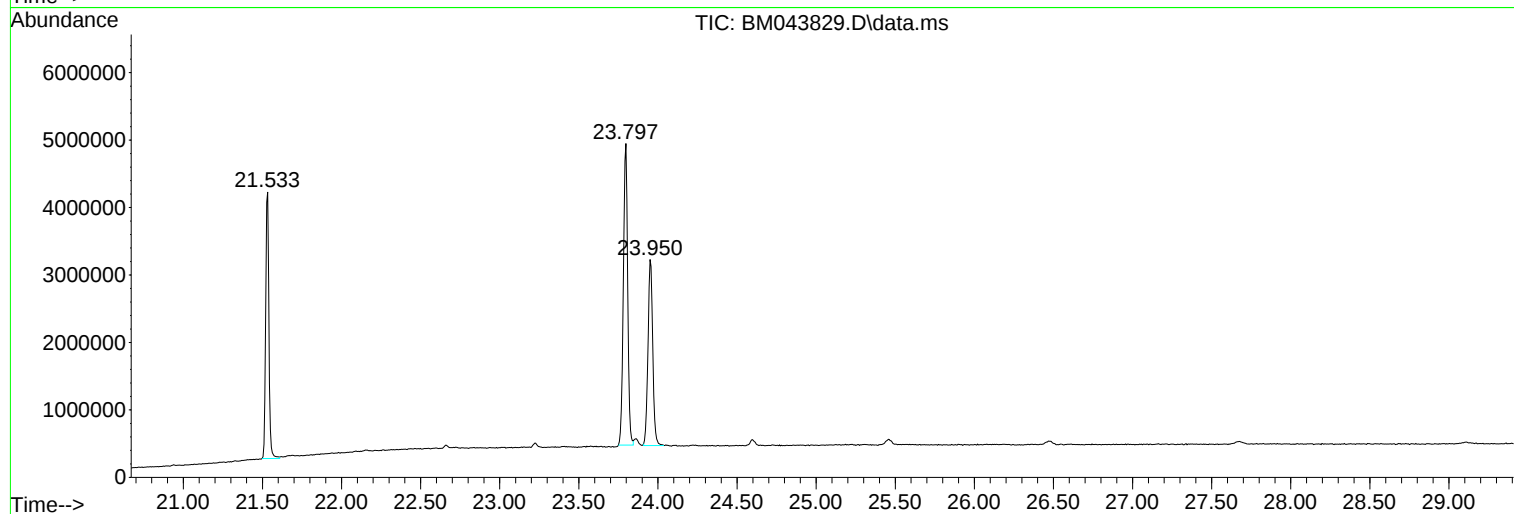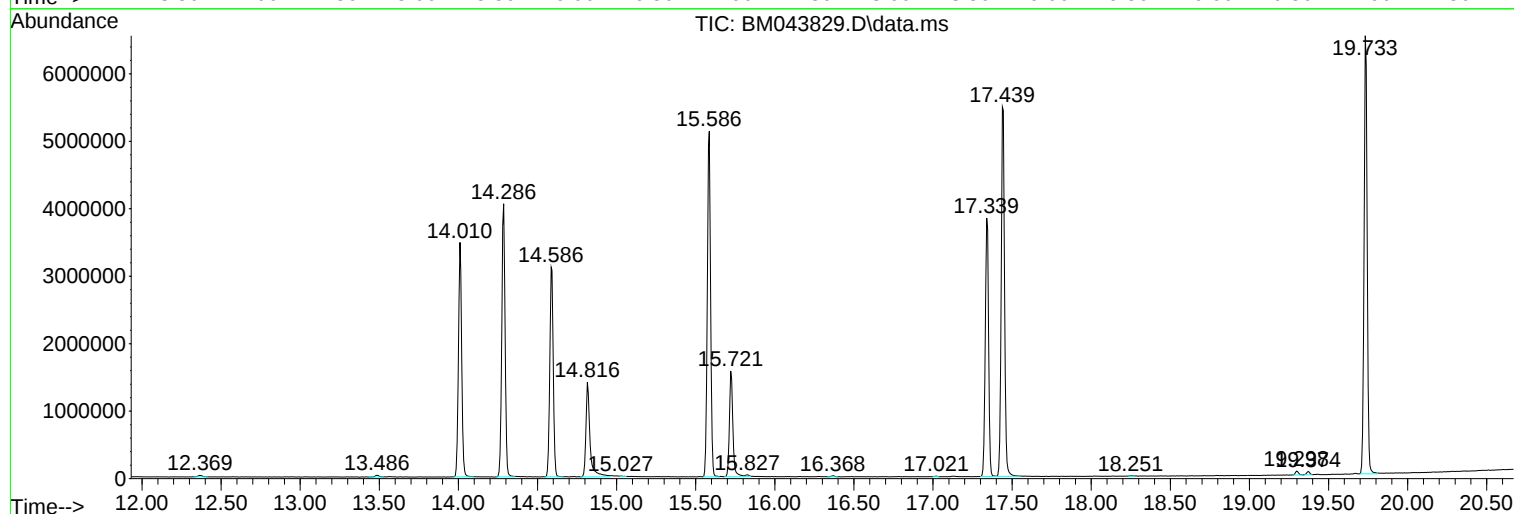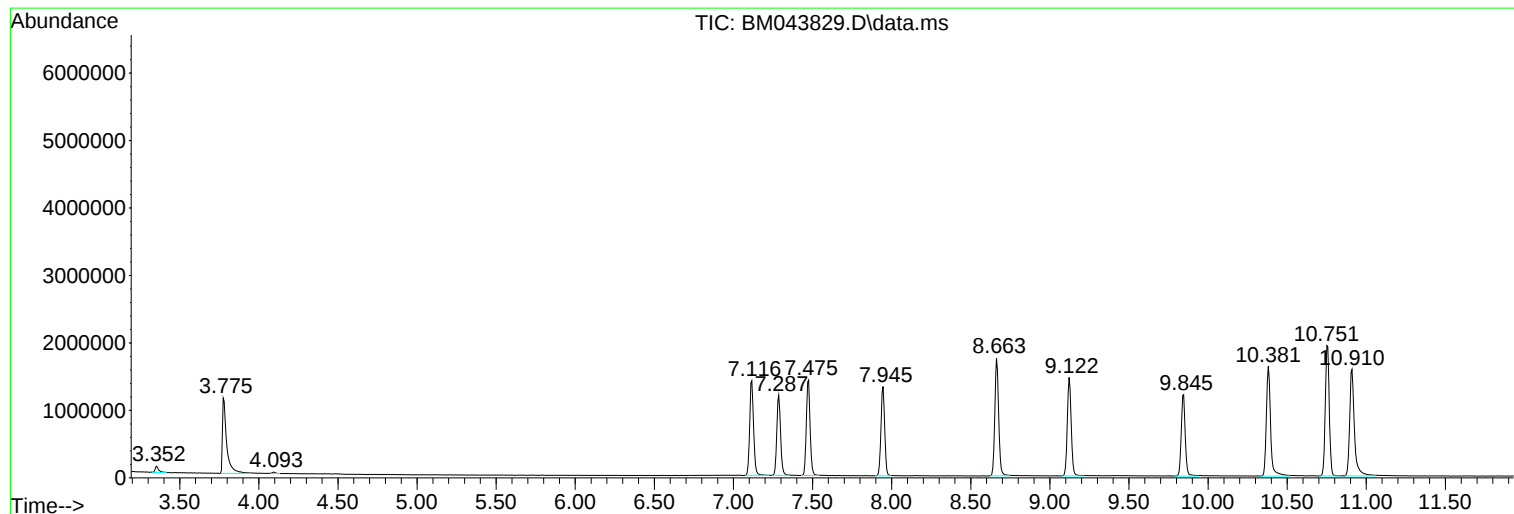

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
Data File : BM043829.D
Acq On : 12 Jan 2024 15:31
Operator : MA/JU
Sample : PB158341BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK341

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011224\
Data File : BM043829.D
Acq On : 12 Jan 2024 15:31
Operator : MA/JU
Sample : PB158341BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK341

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc