

Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM011315\
 Data File : BM000185.D
 Acq On : 14 Jan 2015 01:20
 Operator : TP/IZ
 Sample : G1065-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAE3

Manual Integrations
 APPROVED

tejaskumar
 1/14/2015 5:23:52 PM

Quant Time: Jan 14 14:16:05 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 14 12:47:10 2015
 Response via : Initial Calibration

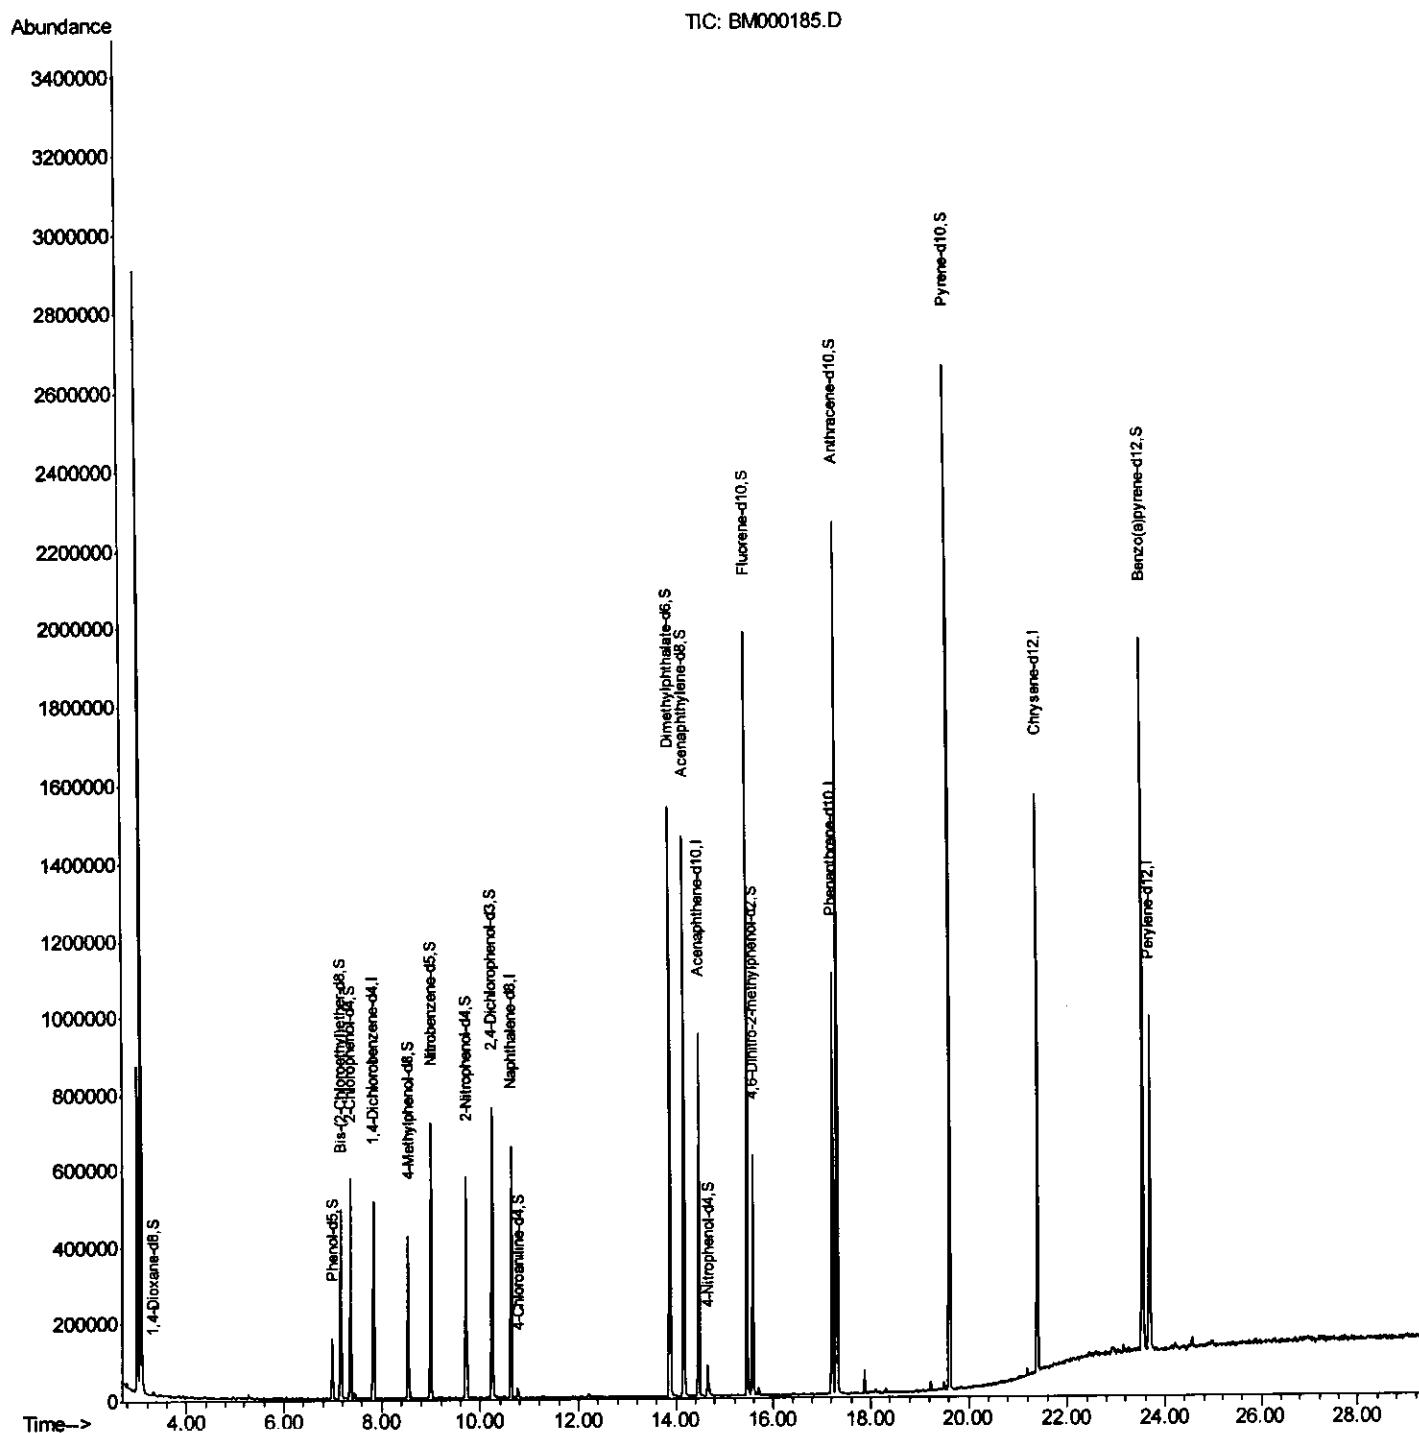

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM011315\
Data File : BM000185.D
Acq On : 14 Jan 2015 01:20
Operator : TP/IZ
Sample : G1065-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jan 14 14:14:02 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 14 12:47:10 2015
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
C0AE3

Manual Integrations
APPROVED

tejaskumar
1/14/2015 5:23:52 PM

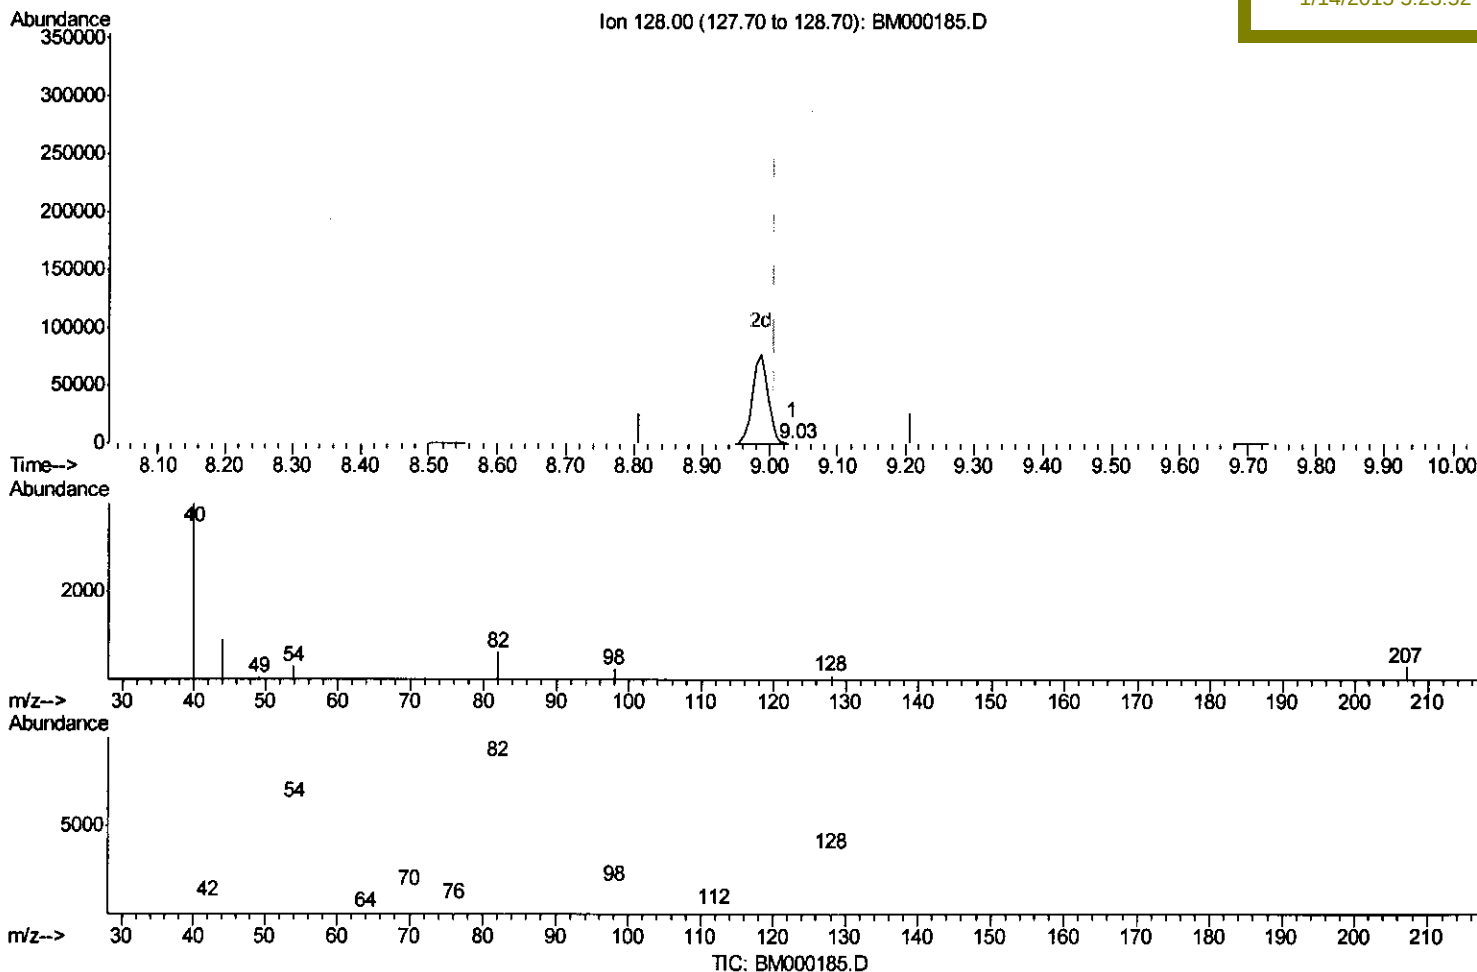

(19) Nitrobenzene-d5 (S)

9.034min (+0.026) 0.04ng/ul

response 132

Ion	Exp%	Act%
128.00	100	100
82.00	274.90	221.60
54.00	158.00	148.27
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM011315\
 Data File : BM000185.D
 Acq On : 14 Jan 2015 01:20
 Operator : TP/IZ
 Sample : G1065-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 C0AE3

Manual Integrations
 APPROVED

tejaskumar
 1/14/2015 5:23:52 PM

Quant Time: Jan 14 14:14:02 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 14 12:47:10 2015
 Response via : Initial Calibration

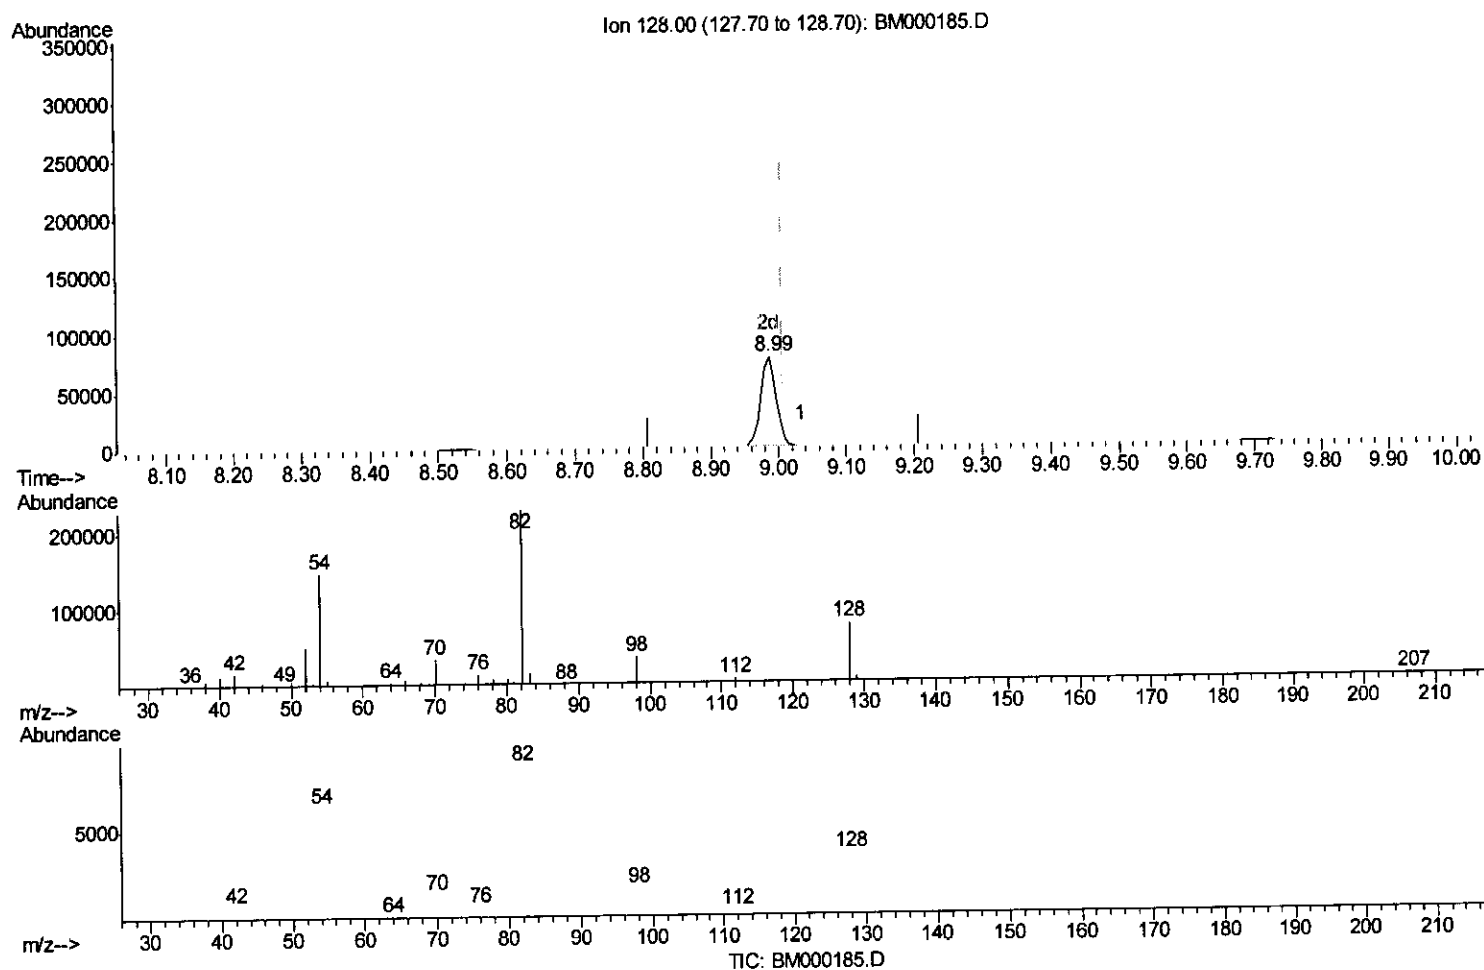

(19) Nitrobenzene-d5 (S)

8.986min (-0.021) 38.22ng/ul m

response 122981

Ion Exp% Act%

128.00 100 100

82.00 274.90 295.52

54.00 158.00 190.80#

0.00 0.00 0.00

T.P
 1/20/15

Data Path : Z:\HPCHEM1\BNA_M\Data\BM011315\
 Data File : BM000185.D
 Acq On : 14 Jan 2015 01:20
 Operator : TP/IZ
 Sample : G1065-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE3

Quant Time: Jan 14 14:16:05 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 14 12:47:10 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

tejaskumar
 1/14/2015 5:23:52 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	118236	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.62	136	465335	20.00	ng/ul	-0.02
35) Acenaphthene-d10	14.46	164	307434	20.00	ng/ul	-0.02
61) Phenanthrene-d10	17.21	188	620788	20.00	ng/ul	-0.02
75) Chrysene-d12	21.39	240	701547	20.00	ng/ul	-0.02
83) Perylene-d12	23.67	264	661583	20.00	ng/ul	-0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	3684	1.81	ng/uL	-0.01
5) Phenol-d5	6.99	99	75052	7.55	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	7.16	67	220898	35.14	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.36	132	205715	28.21	ng/ul	-0.01
13) 4-Methylphenol-d8	8.53	113	130914	16.55	ng/ul	-0.01
19) Nitrobenzene-d5	8.99	128	122981m	38.22	ng/ul	-0.02
22) 2-Nitrophenol-d4	9.70	143	129547	39.43	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.23	165	229271	31.59	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.76	131	12145	1.47	ng/ul	-0.02
43) Dimethylphthalate-d6	13.87	166	883371	38.96	ng/ul	-0.01
46) Acenaphthylene-d8	14.16	160	980628	36.10	ng/ul	-0.02
51) 4-Nitrophenol-d4	14.66	143	18804	5.10	ng/ul	0.00
57) Fluorene-d10	15.46	176	724793	37.22	ng/ul	-0.02
62) 4,6-Dinitro-2-methylphenol	15.57	200	107152	36.42	ng/ul	-0.02
70) Anthracene-d10	17.30	188	1205518	42.00	ng/ul	-0.01
76) Pyrene-d10	19.60	212	1314725	40.62	ng/ul	-0.02
87) Benzo(a)pyrene-d12	23.53	264	1271810	42.35	ng/ul	-0.04

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

T.P
 1/20/15