

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011315\
 Data File : BM000182.D
 Acq On : 13 Jan 2015 23:33
 Operator : TP/IZ
 Sample : G1063-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AQ2

Quant Time: Jan 14 12:59:49 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 14 12:47:10 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	127925	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.62	136	486880	20.00	ng/ul	-0.02
35) Acenaphthene-d10	14.46	164	302083	20.00	ng/ul	-0.02
61) Phenanthrene-d10	17.20	188	562643	20.00	ng/ul	-0.02
75) Chrysene-d12	21.39	240	634221	20.00	ng/ul	-0.02
83) Perylene-d12	23.68	264	644150	20.00	ng/ul	-0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	4448	2.02	ng/uL	-0.01
5) Phenol-d5	6.99	99	75660	7.03	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	7.16	67	238414	35.05	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.36	132	220799	27.98	ng/ul	-0.01
13) 4-Methylphenol-d8	8.53	113	112063	13.09	ng/ul	-0.01
19) Nitrobenzene-d5	8.99	128	125980	37.42	ng/ul	-0.02
22) 2-Nitrophenol-d4	9.70	143	131692	38.31	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.24	165	236686	31.17	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.76	131	6520	0.76	ng/ul	-0.02
43) Dimethylphthalate-d6	13.87	166	797236	35.78	ng/ul	-0.01
46) Acenaphthylene-d8	14.16	160	924755	34.65	ng/ul	-0.02
51) 4-Nitrophenol-d4	14.65	143	15542	4.29	ng/ul	-0.01
57) Fluorene-d10	15.46	176	666315	34.83	ng/ul	-0.02
62) 4,6-Dinitro-2-methylphenol	15.57	200	81264	30.48	ng/ul	-0.02
70) Anthracene-d10	17.30	188	939033	36.09	ng/ul	-0.01
76) Pyrene-d10	19.60	212	1023658	34.99	ng/ul	-0.02
87) Benzo(a)pyrene-d12	23.53	264	1093399	37.40	ng/ul	-0.04


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	37208	1.68	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011315\
Data File : BM000182.D
Acq On : 13 Jan 2015 23:33
Operator : TP/IZ
Sample : G1063-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AQ2

Quant Time: Jan 14 12:59:49 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 14 12:47:10 2015
Response via : Initial Calibration

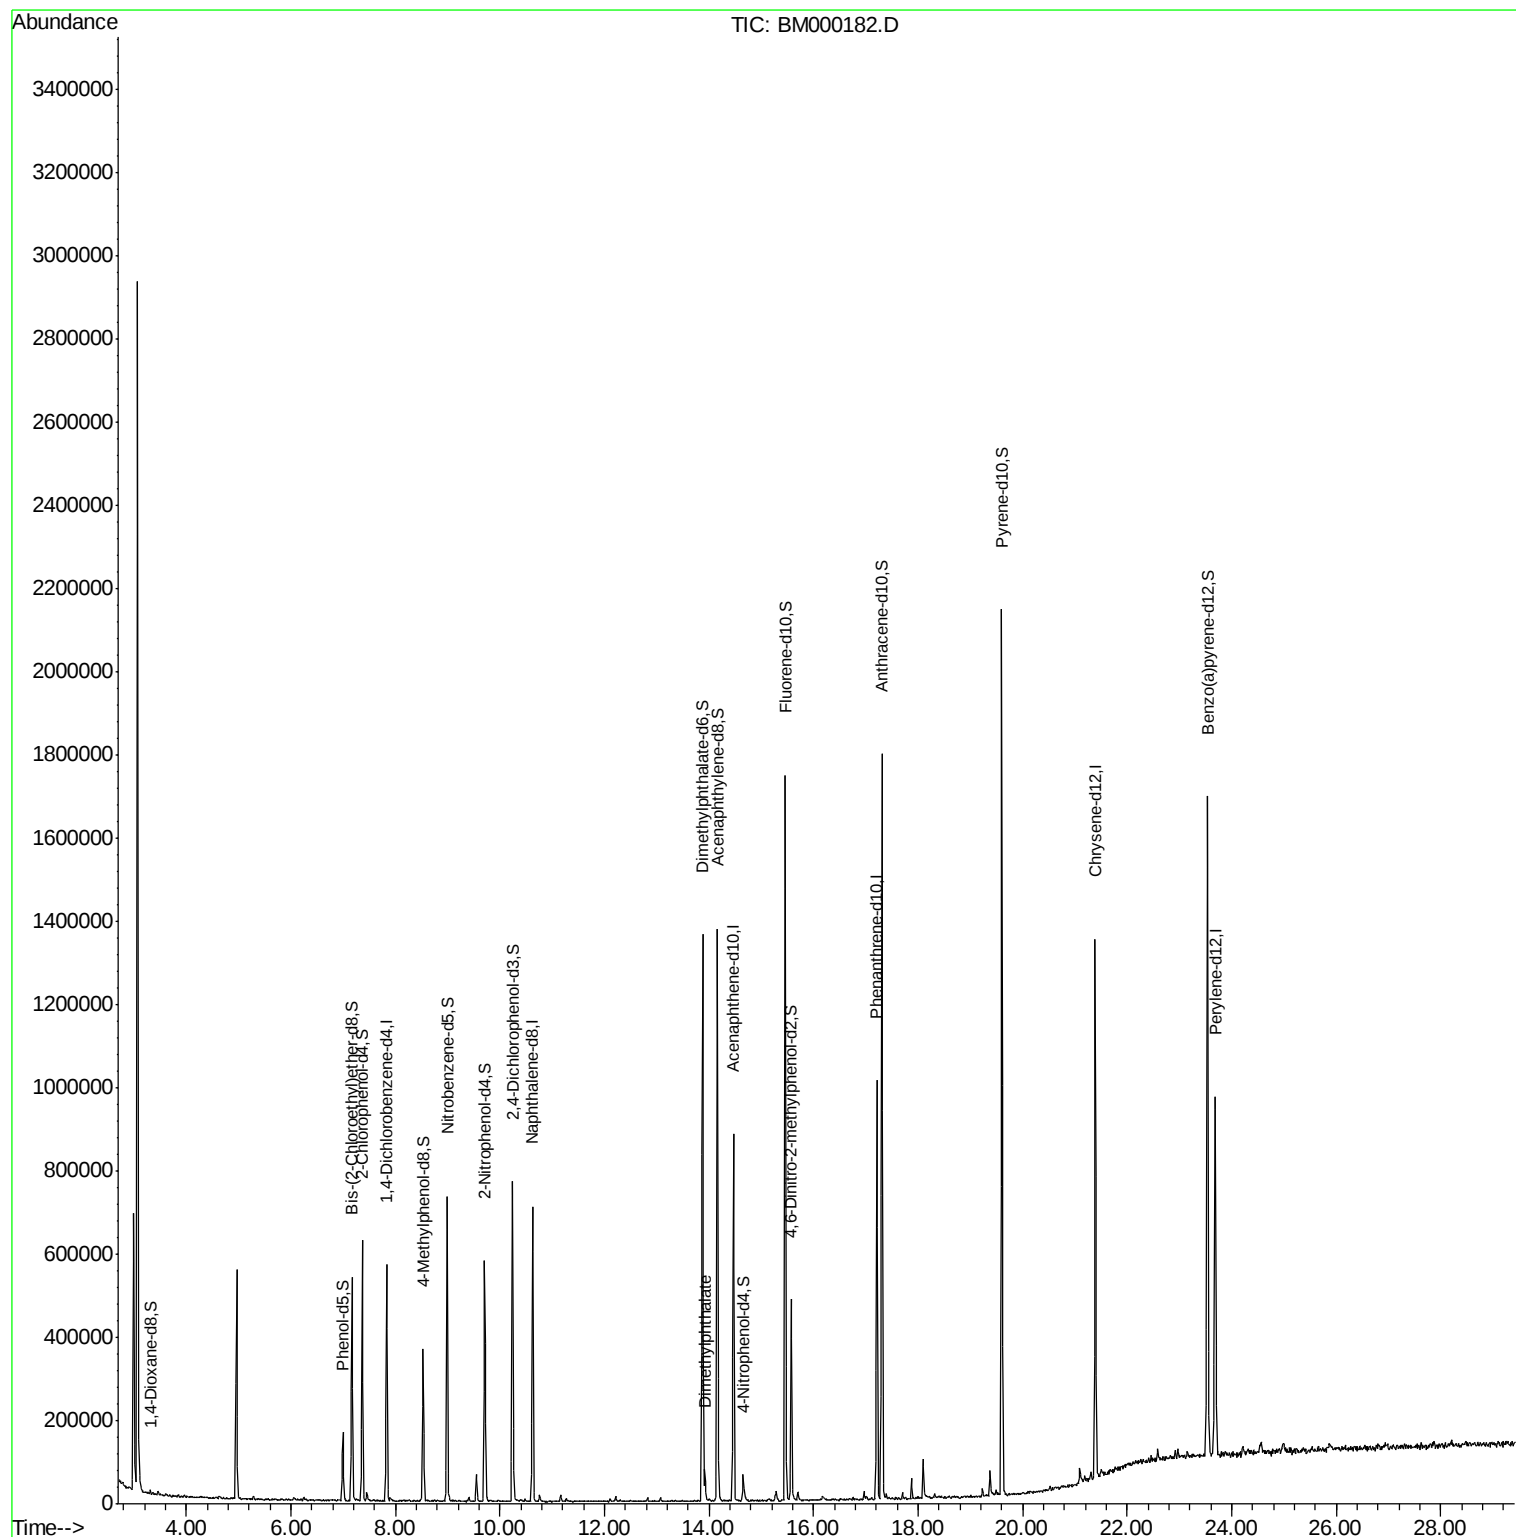

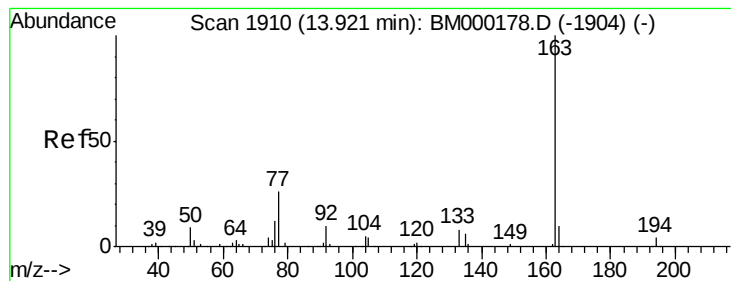

#44

Dimethylphthalate

Concen: 1.68 ng/ul

RT: 13.92 min Scan# 1910

Delta R.T. -0.01 min

Lab File: BM000182.D


Acq: 13 Jan 2015 23:33

Instrument :

BNA_M

ClientSampleId :

C0AQ2

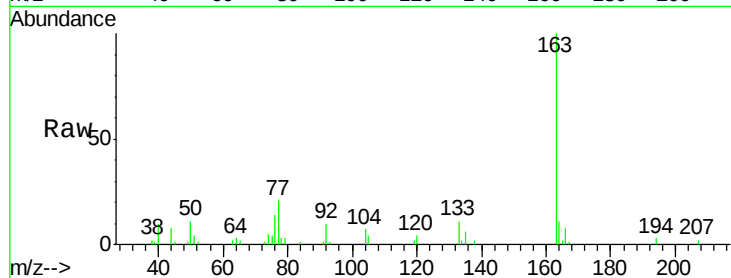

Tgt Ion:	163	Resp:	37208
Ion	Ratio	Lower	Upper
163	100		
194	3.0	3.0	4.4#
164	11.2	8.5	12.7

