

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011315\
 Data File : BM000183.D
 Acq On : 14 Jan 2015 00:09
 Operator : TP/IZ
 Sample : G1063-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AQ3

Quant Time: Jan 14 14:10:05 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 14 12:47:10 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	125205	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.62	136	488240	20.00	ng/ul	-0.02
35) Acenaphthene-d10	14.46	164	302003	20.00	ng/ul	-0.02
61) Phenanthrene-d10	17.20	188	544146	20.00	ng/ul	-0.02
75) Chrysene-d12	21.39	240	570088	20.00	ng/ul	-0.02
83) Perylene-d12	23.68	264	591503	20.00	ng/ul	-0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	4426	2.05	ng/uL	0.00
5) Phenol-d5	6.99	99	85423	8.11	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	7.16	67	251612	37.79	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.36	132	239939	31.07	ng/ul	-0.01
13) 4-Methylphenol-d8	8.53	113	137738	16.44	ng/ul	-0.01
19) Nitrobenzene-d5	8.99	128	136853	40.53	ng/ul	-0.02
22) 2-Nitrophenol-d4	9.70	143	142892	41.46	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.24	165	258299	33.92	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.76	131	13521	1.56	ng/ul	-0.02
43) Dimethylphthalate-d6	13.87	166	845734	37.97	ng/ul	-0.01
46) Acenaphthylene-d8	14.16	160	986587	36.97	ng/ul	-0.02
51) 4-Nitrophenol-d4	14.65	143	16746	4.62	ng/ul	-0.01
57) Fluorene-d10	15.46	176	698934	36.54	ng/ul	-0.02
62) 4,6-Dinitro-2-methylphenol	15.57	200	86587	33.58	ng/ul	-0.02
70) Anthracene-d10	17.30	188	1018519	40.48	ng/ul	-0.01
76) Pyrene-d10	19.60	212	1053309	40.05	ng/ul	-0.02
87) Benzo(a)pyrene-d12	23.53	264	1125687	41.93	ng/ul	-0.04


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	38053	1.72	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011315\
Data File : BM000183.D
Acq On : 14 Jan 2015 00:09
Operator : TP/IZ
Sample : G1063-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AQ3

Quant Time: Jan 14 14:10:05 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 14 12:47:10 2015
Response via : Initial Calibration

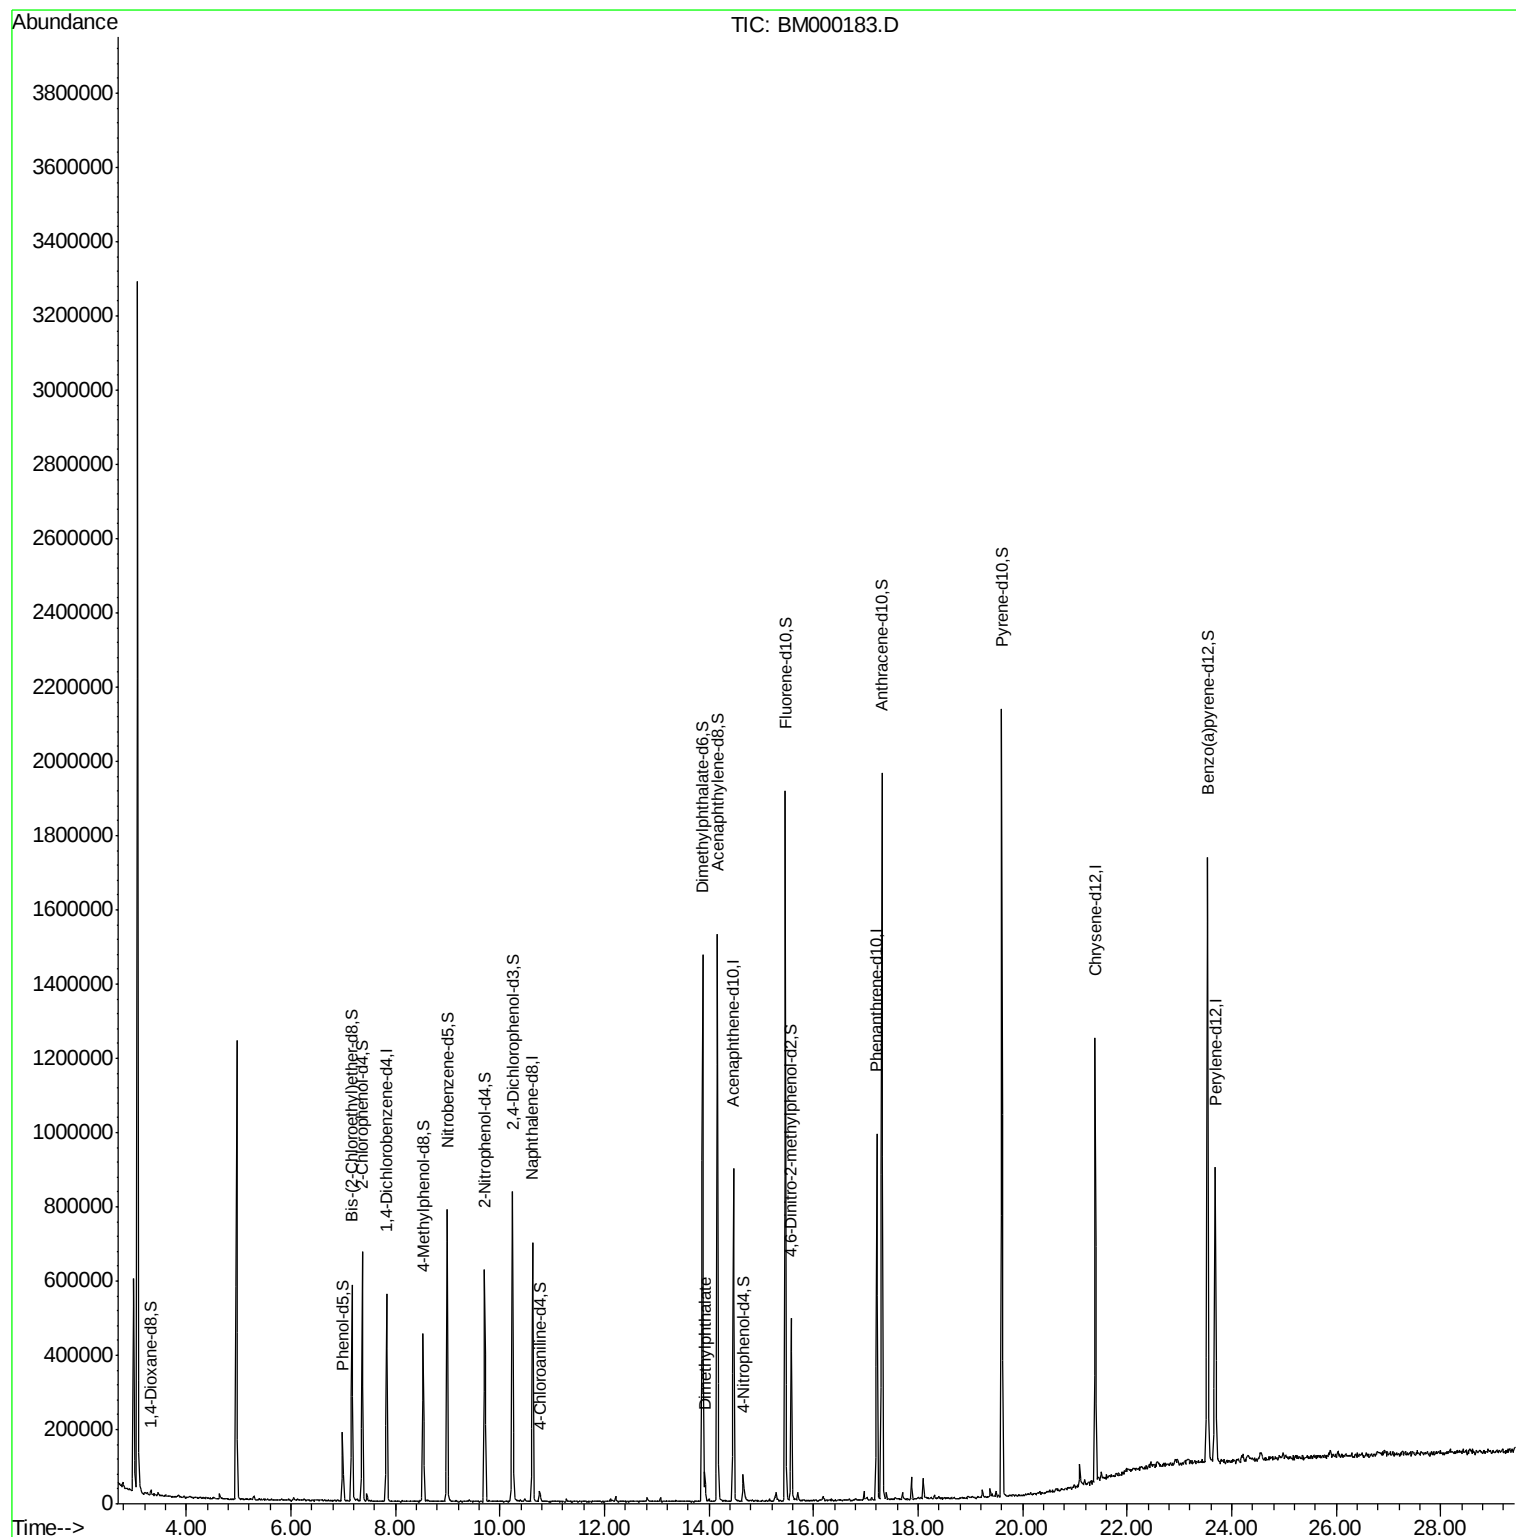

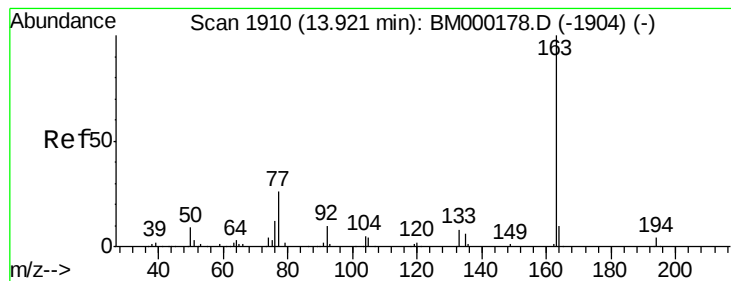

#44

Dimethylphthalate

Concen: 1.72 ng/ul

RT: 13.92 min Scan# 1909

Delta R.T. -0.02 min

Lab File: BM000183.D

Acq: 14 Jan 2015 00:09

Instrument :

BNA_M

ClientSampleId :

C0AQ3


Tgt Ion:163 Resp: 38053

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.4

164 10.8 8.5 12.7

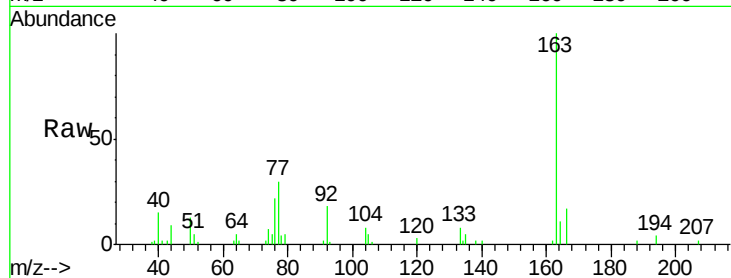

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

