

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011316\
 Data File : BM003969.D
 Acq On : 12 Jan 2016 23:43
 Operator : SJ/UM
 Sample : H1095-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC980

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	15	rVB	7774	10128	0.65%	0.078%
2	6.846	633	639	650	rBV	175844	278381	17.90%	2.149%
3	7.004	660	666	676	rBV	150667	233243	15.00%	1.800%
4	7.198	693	699	710	rBB	188611	291721	18.76%	2.252%
5	7.663	773	778	787	rBB	115332	179795	11.56%	1.388%
6	8.375	893	899	913	rBB	234839	378618	24.35%	2.923%
7	8.822	969	975	987	rBB	180013	280130	18.01%	2.162%
8	9.545	1092	1098	1106	rBB	145655	231317	14.88%	1.786%
9	10.081	1183	1189	1201	rBV	230795	370717	23.84%	2.862%
10	10.451	1246	1252	1262	rBB	187541	303659	19.53%	2.344%
11	10.592	1270	1276	1297	rBB	226316	389363	25.04%	3.006%
12	12.051	1521	1524	1528	rBB	2328	3422	0.22%	0.026%
13	13.733	1804	1810	1814	rBV	473669	639187	41.11%	4.934%
14	13.780	1814	1818	1824	rVB	121275	164536	10.58%	1.270%
15	14.010	1851	1857	1870	rBV	536272	778310	50.05%	6.008%
16	14.222	1890	1893	1896	rBB	6421	7019	0.45%	0.054%
17	14.322	1904	1910	1917	rBB2	297548	438332	28.19%	3.384%
18	14.539	1942	1947	1962	rBV	184390	271117	17.44%	2.093%
19	15.174	2051	2055	2059	rBB	13755	14989	0.96%	0.116%
20	15.321	2073	2080	2090	rBB	697787	1012122	65.09%	7.813%
21	15.451	2097	2102	2108	rBV	178962	241675	15.54%	1.866%
22	15.563	2117	2121	2123	rBV	6511	8959	0.58%	0.069%
23	15.733	2146	2150	2153	rBV	1540	1903	0.12%	0.015%
24	16.039	2198	2202	2212	rBV	15645	25602	1.65%	0.198%
25	16.380	2255	2260	2264	rBV2	2075	3122	0.20%	0.024%
26	16.833	2333	2337	2340	rBV	8368	10352	0.67%	0.080%
27	16.880	2340	2345	2348	rVB3	2303	3409	0.22%	0.026%
28	17.074	2372	2378	2388	rVB2	388003	546899	35.17%	4.222%
29	17.168	2388	2394	2406	rBV2	785275	1125807	72.40%	8.690%
30	17.568	2459	2462	2464	rBV	1942	1587	0.10%	0.012%
31	17.968	2527	2530	2537	rBV	12972	14776	0.95%	0.114%
32	19.109	2720	2724	2727	rBV	6857	8965	0.58%	0.069%
33	19.139	2727	2729	2732	rVB	1821	1772	0.11%	0.014%
34	19.362	2763	2767	2771	rVB	5797	6837	0.44%	0.053%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011316\
 Data File : BM003969.D
 Acq On : 12 Jan 2016 23:43
 Operator : SJ/UM
 Sample : H1095-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC980

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

35	19.474	2780	2786	2795	rBV	1019231	1386627	89.17%	10.704%
36	20.633	2980	2983	2986	rBV	3555	3564	0.23%	0.028%
37	20.980	3038	3042	3056	rBV	38469	62985	4.05%	0.486%
38	21.186	3074	3077	3080	rBV	4483	4312	0.28%	0.033%
39	21.274	3087	3092	3100	rBV	592869	737703	47.44%	5.695%
40	21.386	3108	3111	3115	rBV2	4163	4403	0.28%	0.034%
41	21.421	3115	3117	3121	rVB3	1714	1940	0.12%	0.015%
42	21.856	3188	3191	3193	rBV	3260	3062	0.20%	0.024%
43	22.309	3264	3268	3272	rBV3	9433	12082	0.78%	0.093%
44	22.445	3286	3291	3295	rBV	8259	10710	0.69%	0.083%
45	22.774	3343	3347	3350	rBV2	8491	11824	0.76%	0.091%
46	22.815	3350	3354	3360	rVB2	12813	17867	1.15%	0.138%
47	23.368	3440	3448	3463	rBV	832423	1555009	100.00%	12.004%
48	23.509	3465	3472	3485	rVB	386001	713045	45.85%	5.504%
49	24.015	3553	3558	3566	rVB2	21364	38074	2.45%	0.294%
50	24.109	3570	3574	3577	rVB4	3480	5799	0.37%	0.045%
51	24.756	3677	3684	3691	rBV2	20403	43814	2.82%	0.338%
52	25.615	3825	3830	3841	rVB3	14650	35132	2.26%	0.271%
53	26.627	3997	4002	4012	rVB3	11436	28801	1.85%	0.222%


Sum of corrected areas: 12954524

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011316\
Data File : BM003969.D
Acq On : 12 Jan 2016 23:43
Operator : SJ/UM
Sample : H1095-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC980

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

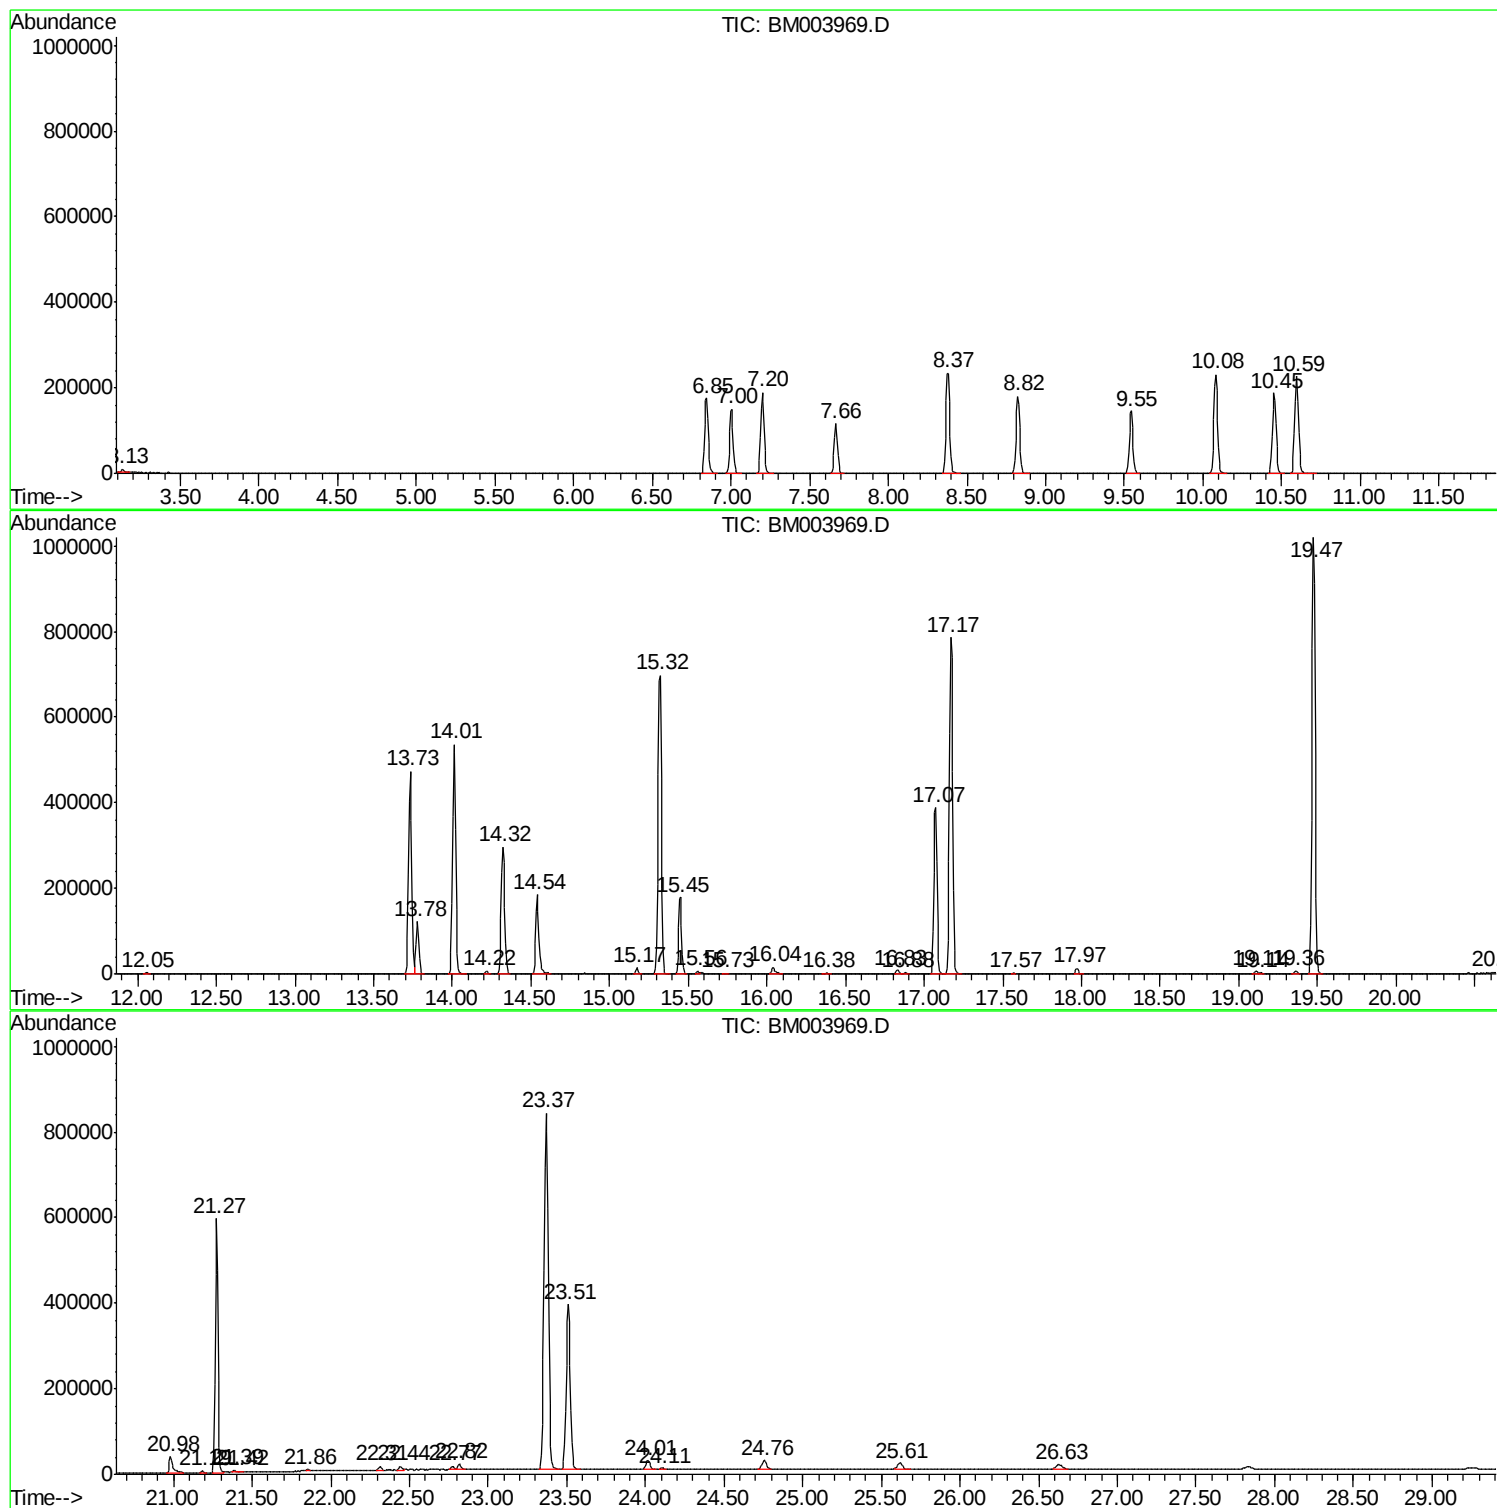

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011316\
Data File : BM003969.D
Acq On : 12 Jan 2016 23:43
Operator : SJ/UM
Sample : H1095-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC980

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011316\
Data File : BM003969.D
Acq On : 12 Jan 2016 23:43
Operator : SJ/UM
Sample : H1095-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC980

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc