

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011316\
 Data File : BM003979.D
 Acq On : 13 Jan 2016 06:17
 Operator : SJ/UM
 Sample : H1095-14 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC977

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.651	92	96	100	rBV	5788	7109	0.87%	0.159%
2	6.851	636	640	647	rVB	3093	4983	0.61%	0.111%
3	7.004	661	666	671	rBB	4987	6700	0.82%	0.149%
4	7.198	696	699	705	rBV	3985	6133	0.75%	0.137%
5	7.663	773	778	788	rBB	131769	204573	25.06%	4.563%
6	8.386	898	901	906	rBB	1845	2747	0.34%	0.061%
7	8.828	972	976	981	rBB	3220	5052	0.62%	0.113%
8	9.545	1096	1098	1102	rBB	1397	1482	0.18%	0.033%
9	10.092	1186	1191	1197	rBB	2829	4585	0.56%	0.102%
10	10.451	1245	1252	1259	rBV	213968	351990	43.12%	7.851%
11	10.616	1276	1280	1282	rBV	1395	1858	0.23%	0.041%
12	13.733	1805	1810	1814	rBV	12839	17096	2.09%	0.381%
13	13.774	1814	1817	1822	rVB	3499	5154	0.63%	0.115%
14	14.010	1853	1857	1862	rBV	15859	22398	2.74%	0.500%
15	14.321	1904	1910	1918	rBV2	346020	516362	63.26%	11.517%
16	15.315	2075	2079	2086	rBB	26397	37052	4.54%	0.826%
17	15.374	2087	2089	2092	rBV	1098	1336	0.16%	0.030%
18	16.856	2336	2341	2344	rBV2	1267	2062	0.25%	0.046%
19	17.068	2371	2377	2382	rBV2	448681	637892	78.15%	14.227%
20	17.109	2382	2384	2390	rVV	36381	44578	5.46%	0.994%
21	17.168	2390	2394	2398	rVV2	26957	37661	4.61%	0.840%
22	17.204	2398	2400	2404	rVV	4732	5551	0.68%	0.124%
23	17.268	2407	2411	2415	rVB2	883	1601	0.20%	0.036%
24	17.480	2443	2447	2451	rVB	920	1281	0.16%	0.029%
25	17.592	2464	2466	2468	rBV	1681	1357	0.17%	0.030%
26	17.651	2473	2476	2479	rVB	1348	1499	0.18%	0.033%
27	17.945	2522	2526	2531	rBV	10441	13787	1.69%	0.308%
28	17.992	2531	2534	2540	rVB	12264	16077	1.97%	0.359%
29	18.074	2545	2548	2554	rBV	1597	2229	0.27%	0.050%
30	18.139	2554	2559	2563	rVV2	16305	28093	3.44%	0.627%
31	18.180	2563	2566	2570	rVB	9670	12663	1.55%	0.282%
32	18.450	2609	2612	2616	rBV	3881	4890	0.60%	0.109%
33	18.498	2616	2620	2625	rVV2	3229	4448	0.54%	0.099%
34	18.698	2650	2654	2657	rVB	2863	3308	0.41%	0.074%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011316\
 Data File : BM003979.D
 Acq On : 13 Jan 2016 06:17
 Operator : SJ/UM
 Sample : H1095-14 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC977

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

35	18.750	2660	2663	2666	rVV	3816	4335	0.53%	0.097%
36	18.792	2666	2670	2673	rVB2	2518	2682	0.33%	0.060%
37	18.874	2679	2684	2688	rBV	13890	19692	2.41%	0.439%
38	18.939	2688	2695	2697	rVV2	6395	13131	1.61%	0.293%
39	18.962	2697	2699	2703	rVV	3655	4437	0.54%	0.099%
40	19.015	2703	2708	2715	rVB4	4666	10747	1.32%	0.240%
41	19.139	2723	2729	2736	rVB	82838	107769	13.20%	2.404%
42	19.203	2736	2740	2743	rBV	1364	1595	0.20%	0.036%
43	19.239	2743	2746	2751	rVV	3259	2871	0.35%	0.064%
44	19.345	2760	2764	2767	rBV	953	1115	0.14%	0.025%
45	19.386	2767	2771	2774	rBV	2425	3200	0.39%	0.071%
46	19.421	2774	2777	2779	rVB	1128	1072	0.13%	0.024%
47	19.474	2781	2786	2788	rVV2	48866	68882	8.44%	1.536%
48	19.503	2788	2791	2799	rVB	103775	135298	16.58%	3.018%
49	19.580	2799	2804	2809	rBV3	5921	8590	1.05%	0.192%
50	19.686	2815	2822	2827	rVB3	2475	5448	0.67%	0.122%
51	19.745	2827	2832	2838	rBV3	3663	5320	0.65%	0.119%
52	19.833	2842	2847	2854	rVV4	8781	18707	2.29%	0.417%
53	19.915	2859	2861	2865	rBV2	1296	1548	0.19%	0.035%
54	19.997	2865	2875	2881	rVB	16578	37619	4.61%	0.839%
55	20.074	2885	2888	2889	rBV	1613	1255	0.15%	0.028%
56	20.103	2889	2893	2897	rVB	9814	11189	1.37%	0.250%
57	20.162	2897	2903	2907	rVB2	17303	24223	2.97%	0.540%
58	20.203	2907	2910	2913	rBV2	2574	3486	0.43%	0.078%
59	20.244	2913	2917	2920	rVB3	2042	2976	0.36%	0.066%
60	20.303	2920	2927	2930	rBV	15985	22193	2.72%	0.495%
61	20.344	2930	2934	2938	rVV	15220	19898	2.44%	0.444%
62	20.386	2938	2941	2944	rVB3	1707	2583	0.32%	0.058%
63	20.474	2953	2956	2959	rBV2	1409	1420	0.17%	0.032%
64	20.515	2961	2963	2968	rVV3	1481	1746	0.21%	0.039%
65	20.562	2968	2971	2975	rVV2	4559	6828	0.84%	0.152%
66	20.603	2975	2978	2980	rVV2	2552	3536	0.43%	0.079%
67	20.627	2980	2982	2986	rVB3	3195	3561	0.44%	0.079%
68	20.668	2987	2989	2992	rVB2	1370	1352	0.17%	0.030%
69	20.721	2992	2998	3001	rBV2	3263	6669	0.82%	0.149%
70	20.756	3001	3004	3011	rVB3	7268	10147	1.24%	0.226%
71	20.844	3015	3019	3023	rBV2	3465	4595	0.56%	0.102%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011316\
 Data File : BM003979.D
 Acq On : 13 Jan 2016 06:17
 Operator : SJ/UM
 Sample : H1095-14 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC977

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION

72	20.897	3023	3028	3029	rBV2	3929	4934	0.60%	0.110%
73	20.927	3029	3033	3036	rVV	7388	10288	1.26%	0.229%
74	20.962	3036	3039	3042	rVV	7267	8176	1.00%	0.182%
75	20.997	3042	3045	3050	rVV2	6608	11106	1.36%	0.248%
76	21.056	3052	3055	3062	rVB3	4745	7136	0.87%	0.159%
77	21.168	3072	3074	3075	rBV	1085	1017	0.12%	0.023%
78	21.274	3085	3092	3096	rBV	617151	816267	100.00%	18.206%
79	21.309	3096	3098	3107	rVB	55733	67099	8.22%	1.497%
80	21.397	3111	3113	3115	rVB3	2927	2047	0.25%	0.046%
81	21.427	3115	3118	3122	rBV	7483	9941	1.22%	0.222%
82	21.491	3127	3129	3130	rBV3	1786	1661	0.20%	0.037%
83	21.639	3150	3154	3158	rBV4	3470	6071	0.74%	0.135%
84	21.733	3166	3170	3174	rVB5	2330	3509	0.43%	0.078%
85	21.768	3174	3176	3179	rBV2	3538	4400	0.54%	0.098%
86	21.827	3179	3186	3189	rVV	16158	28148	3.45%	0.628%
87	21.874	3192	3194	3199	rVB	9831	12361	1.51%	0.276%
88	21.939	3202	3205	3209	rBV3	4169	6562	0.80%	0.146%
89	21.974	3209	3211	3215	rBV2	4026	4879	0.60%	0.109%
90	22.021	3215	3219	3222	rBV	9208	11638	1.43%	0.260%
91	22.315	3265	3269	3278	rBV6	6488	14907	1.83%	0.332%
92	22.838	3350	3358	3363	rBV2	28959	75900	9.30%	1.693%
93	23.009	3384	3387	3393	rVB2	4910	7812	0.96%	0.174%
94	23.315	3434	3439	3443	rBV2	20018	35645	4.37%	0.795%
95	23.368	3443	3448	3452	rVV2	23154	42218	5.17%	0.942%
96	23.409	3452	3455	3464	rVB	28452	46836	5.74%	1.045%
97	23.509	3464	3472	3479	rBV	307397	577624	70.76%	12.883%
98	24.015	3553	3558	3564	rVB2	7747	13933	1.71%	0.311%
99	25.750	3847	3853	3864	rVB	11305	27732	3.40%	0.619%
100	26.444	3964	3971	3980	rVB2	9222	26424	3.24%	0.589%


Sum of corrected areas: 4483573

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011316\
Data File : BM003979.D
Acq On : 13 Jan 2016 06:17
Operator : SJ/UM
Sample : H1095-14 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC977

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

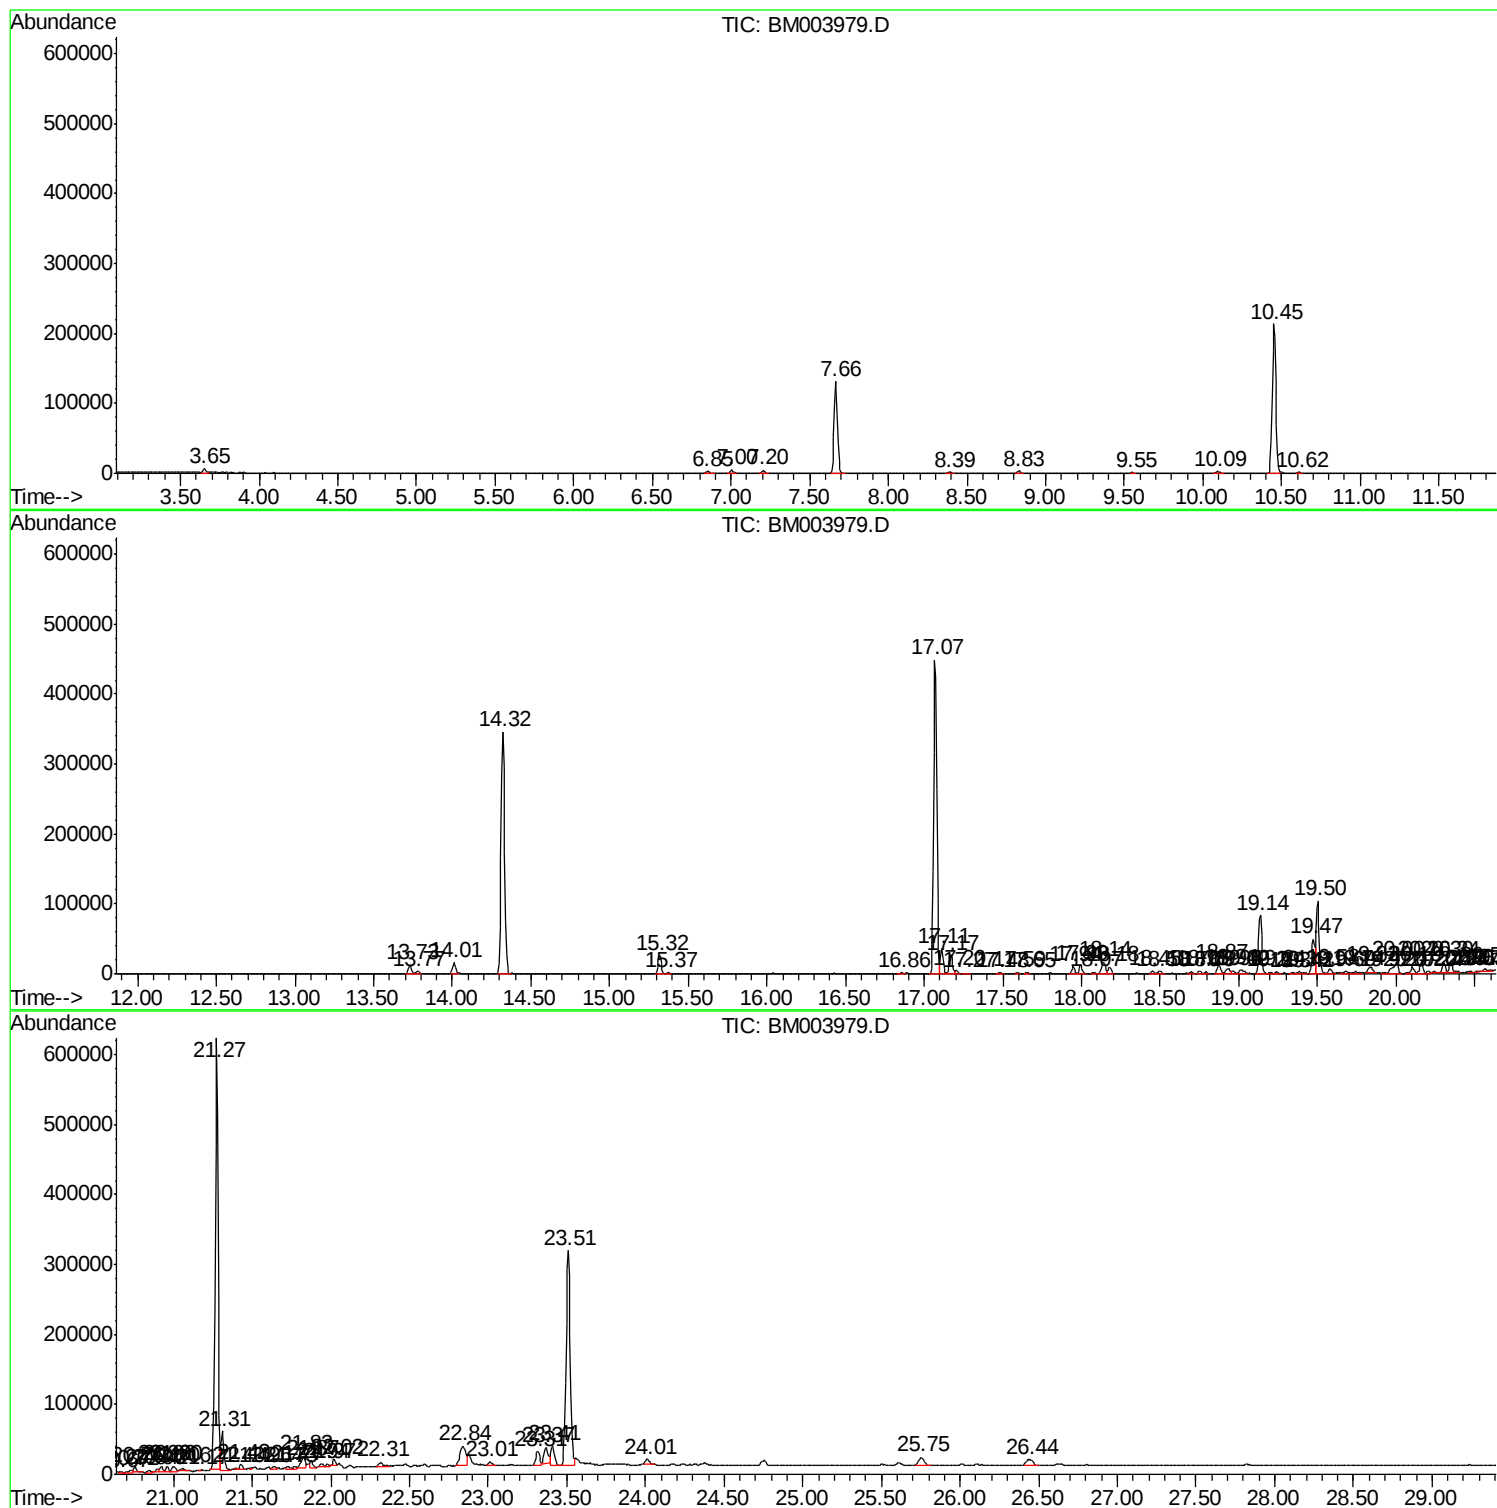

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011316\
Data File : BM003979.D
Acq On : 13 Jan 2016 06:17
Operator : SJ/UM
Sample : H1095-14 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC977

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011316\
Data File : BM003979.D
Acq On : 13 Jan 2016 06:17
Operator : SJ/UM
Sample : H1095-14 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC977

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc