


Data Path : Z:\HPCHEM1\BNA M\DATA\BM011316\
Data File : BM003958.D
Acq On : 12 Jan 2016 17:06
Operator : SJ/UM
Sample : DFTPP36
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP36

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Title : SVOA CALIBRATION
Last Update : Wed Jan 13 06:45:02 2016

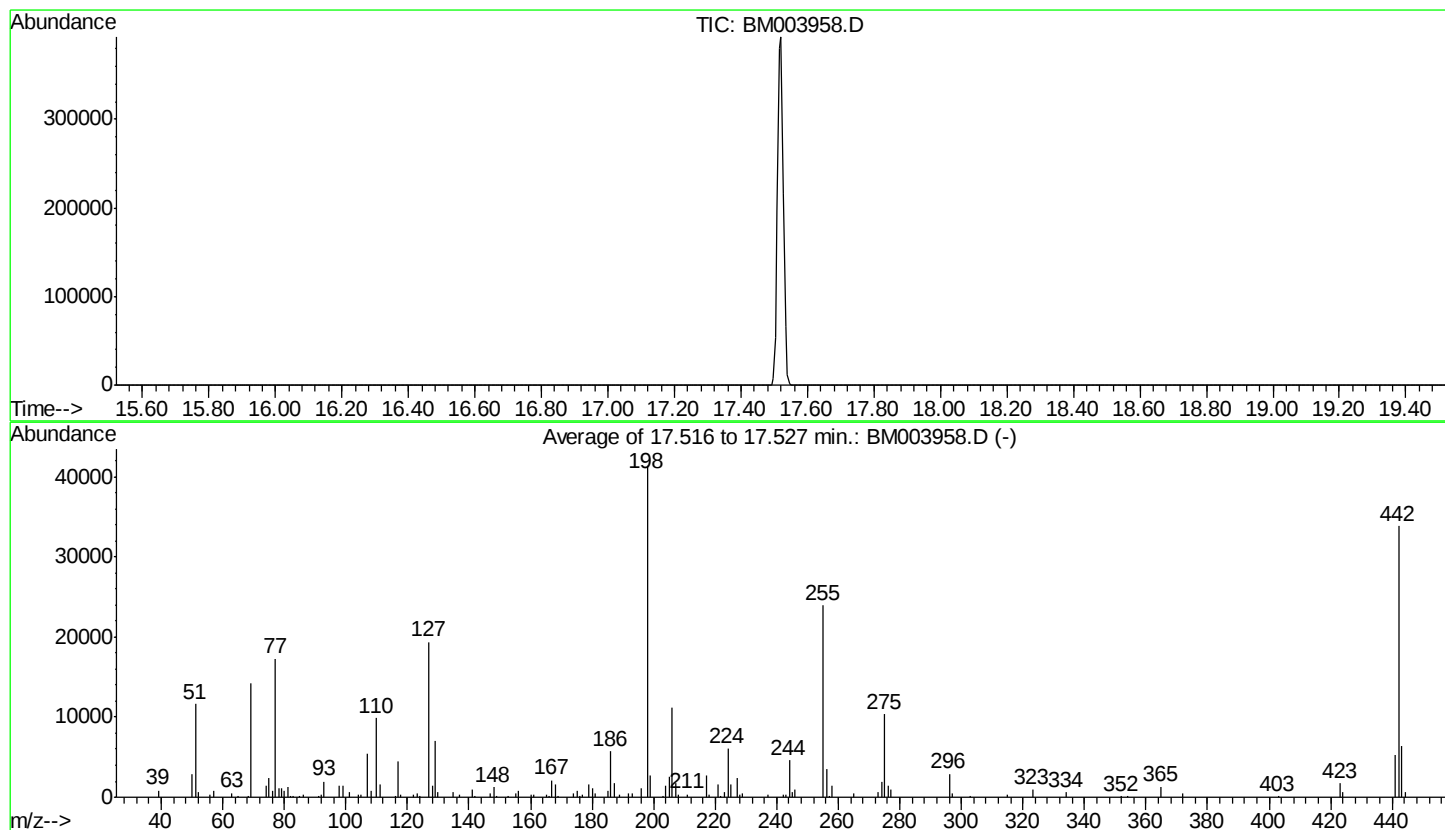

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	11598	PASS
68	69	0.00	2	0.7	104	PASS
69	198	0.00	100	34.2	14169	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.8	19376	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41389	PASS
199	198	5	9	6.7	2766	PASS
275	198	10	60	25.1	10381	PASS
365	198	1	100	3.1	1282	PASS
441	443	0.01	100	81.6	5238	PASS
442	198	50	100	81.8	33861	PASS
443	442	15	24	19.0	6417	PASS

m/z	Abundance
39.00	1159.0
50.10	3702.0
51.10	15073.0
52.00	775.0
56.00	455.0
57.00	1092.0
63.00	632.0
65.00	355.0
68.10	312.0
69.00	18224.0
74.00	1859.0
75.00	3116.0
76.10	1076.0
77.10	21912.0
78.10	1557.0
79.00	1424.0
80.00	1015.0
81.00	1574.0
82.00	429.0
83.00	306.0
85.00	359.0
86.00	412.0
92.00	440.0
93.00	2577.0
98.00	1845.0
99.00	1937.0
101.00	910.0
104.00	549.0
105.00	455.0
107.00	6881.0
108.00	1088.0
110.00	12429.0
111.00	1995.0
116.00	341.0
117.00	5457.0
117.90	465.0
122.00	416.0
123.00	664.0
124.00	317.0
127.00	23864.0
128.00	1744.0
129.00	8641.0
130.00	817.0
135.00	797.0
137.00	567.0
141.00	1162.0
142.00	365.0
147.00	598.0
148.00	1445.0
149.00	353.0
152.90	373.0
155.10	640.0
156.00	977.0
160.00	424.0
161.00	605.0
165.00	467.0
166.00	322.0
167.00	2508.0
168.00	2100.0
169.00	321.0
174.00	575.0
175.00	996.0
177.00	376.0
179.00	1773.0
180.00	1446.0
181.00	505.0
185.00	876.0
186.10	6496.0
187.10	1943.0
189.00	457.0
192.00	610.0
193.00	626.0
196.00	1415.0
198.00	47520.0
199.00	3299.0
203.00	309.0
204.00	1772.0
205.10	2837.0
206.10	12576.0
207.10	1981.0
208.00	438.0
211.00	501.0
217.00	2968.0
218.00	368.0
221.00	1688.0
223.00	689.0
224.10	6606.0
225.10	1858.0
227.00	2627.0
228.00	413.0
229.00	543.0
237.00	390.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

242.00	393.0
243.10	385.0
244.10	5125.0
245.00	649.0
246.00	988.0
255.10	25800.0
256.10	3877.0
257.00	364.0
258.00	1480.0
265.00	553.0
273.00	755.0
274.00	2044.0
275.10	10867.0
276.10	1558.0
277.00	973.0
296.00	2925.0
297.00	430.0
315.00	352.0
323.10	946.0
334.10	577.0
354.10	327.0
365.00	1241.0
372.10	441.0
423.10	1592.0
424.10	743.0
441.10	4763.0
442.10	30400.0
443.10	6107.0
444.10	623.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

m/z	Abundance
39.00	1029.0
50.10	3316.0
51.10	13226.0
52.10	670.0
56.00	399.0
57.00	1017.0
63.00	583.0
65.00	313.0
69.00	16180.0
74.00	1659.0
75.00	2673.0
76.10	901.0
77.10	20040.0
78.10	1347.0
79.00	1267.0
80.00	944.0
81.00	1386.0
83.00	305.0
86.00	380.0
91.00	310.0
92.00	384.0
93.00	2060.0
98.00	1714.0
99.00	1602.0
101.00	796.0
104.00	488.0
104.90	441.0
107.00	6355.0
108.00	1004.0
110.00	11334.0
111.00	1736.0
117.00	5318.0
118.00	431.0
122.00	385.0
123.00	587.0
127.00	22408.0
128.00	1697.0
129.00	8304.0
130.00	701.0
135.00	662.0
137.00	429.0
141.00	1021.0
142.00	341.0
147.00	658.0
148.00	1412.0
155.00	633.0
156.00	1022.0
160.00	363.0
161.00	590.0
165.00	428.0
166.00	340.0
167.00	2545.0
168.00	1708.0
174.00	504.0
175.00	996.0
176.00	304.0
177.00	393.0
179.00	1865.0
180.00	1290.0
181.00	549.0
185.10	902.0
186.10	6798.0
187.00	2009.0
189.00	444.0
192.00	547.0
193.00	635.0
196.00	1462.0
198.00	49176.0
199.00	3118.0
203.00	359.0
204.00	1888.0
205.10	3077.0
206.10	13542.0
207.10	1969.0
208.00	443.0
211.00	521.0
217.00	3252.0
218.00	438.0
221.10	2077.0
221.80	481.0
223.00	756.0
224.10	7374.0
225.00	1842.0
227.00	2933.0
228.00	447.0
229.00	575.0
237.00	357.0
242.00	420.0
243.00	381.0
244.10	5636.0
245.00	696.0
246.00	1075.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

255.10	28624.0
256.10	4136.0
257.00	341.0
258.00	1725.0
265.00	674.0
273.00	788.0
274.10	2233.0
275.10	12838.0
276.10	1681.0
277.00	1175.0
296.00	3615.0
297.00	514.0
303.00	400.0
315.00	421.0
323.10	1104.0
334.10	819.0
352.10	339.0
354.10	387.0
365.00	1556.0
372.10	649.0
403.10	334.0
423.10	2129.0
424.10	695.0
441.10	6411.0
442.10	41512.0
443.10	7693.0
444.10	721.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

m/z	Abundance
39.00	444.0
50.00	1598.0
51.10	6495.0
52.00	352.0
57.00	459.0
63.00	307.0
69.00	8103.0
74.00	867.0
75.00	1398.0
76.10	424.0
77.10	9918.0
78.00	665.0
79.00	598.0
80.00	491.0
81.00	757.0
93.00	1131.0
98.00	776.0
99.00	772.0
101.00	396.0
107.00	3027.0
108.00	524.0
110.00	5852.0
111.00	913.0
117.00	2703.0
123.00	360.0
127.00	11857.0
128.00	856.0
129.00	4378.0
130.00	410.0
135.00	388.0
141.00	593.0
147.00	327.0
148.00	770.0
155.00	342.0
156.00	531.0
167.00	1356.0
168.00	973.0
173.90	318.0
175.00	494.0
179.00	965.0
180.00	814.0
181.00	334.0
185.00	465.0
186.00	3902.0
187.00	1111.0
192.00	351.0
193.00	367.0
196.00	712.0
198.00	27472.0
199.00	1883.0
204.00	887.0
205.00	1744.0
206.10	7293.0
207.00	1219.0
217.00	1917.0
221.10	1082.0
223.00	412.0
224.10	4164.0
225.00	989.0
227.00	1681.0
229.00	364.0
244.10	3114.0
245.10	378.0
246.00	591.0
255.10	17392.0
256.00	2468.0
258.00	982.0
265.00	324.0
273.00	512.0
274.00	1473.0
275.10	7439.0
276.00	949.0
277.00	637.0
296.00	2255.0
297.00	300.0
323.10	696.0
334.10	479.0
365.00	1049.0
372.00	352.0
423.10	1474.0
424.10	526.0
441.10	4540.0
442.10	29672.0
443.10	5451.0
444.10	426.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

Instrument :

BNA_M

ClientSampleId :

DFTPP36