
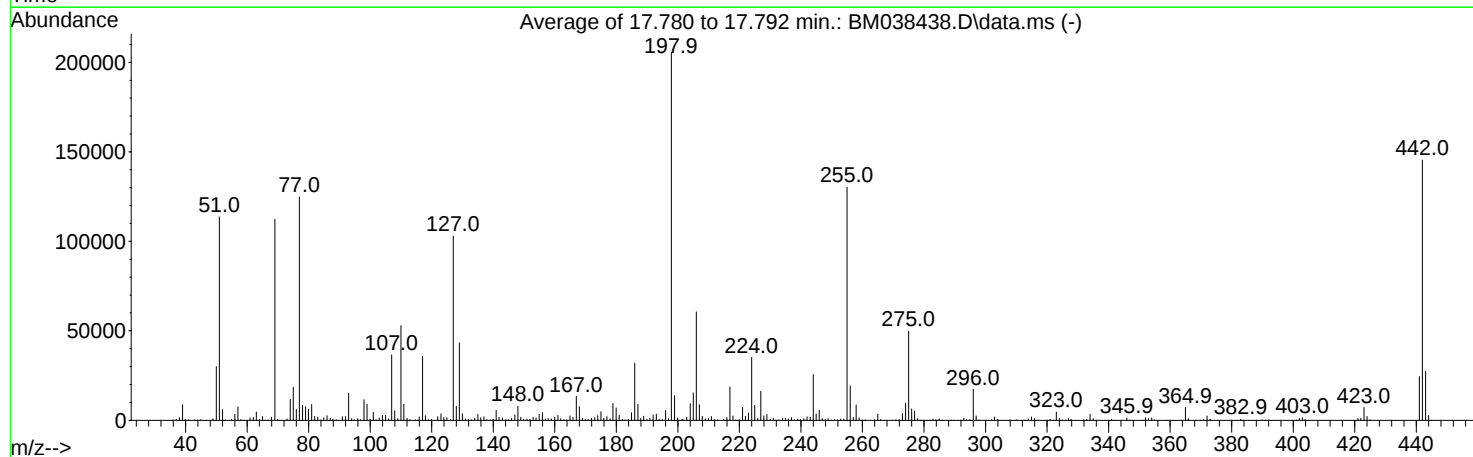


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011323\
 Data File : BM038438.D
 Acq On : 12 Jan 2023 15:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 13 01:05:13 2023

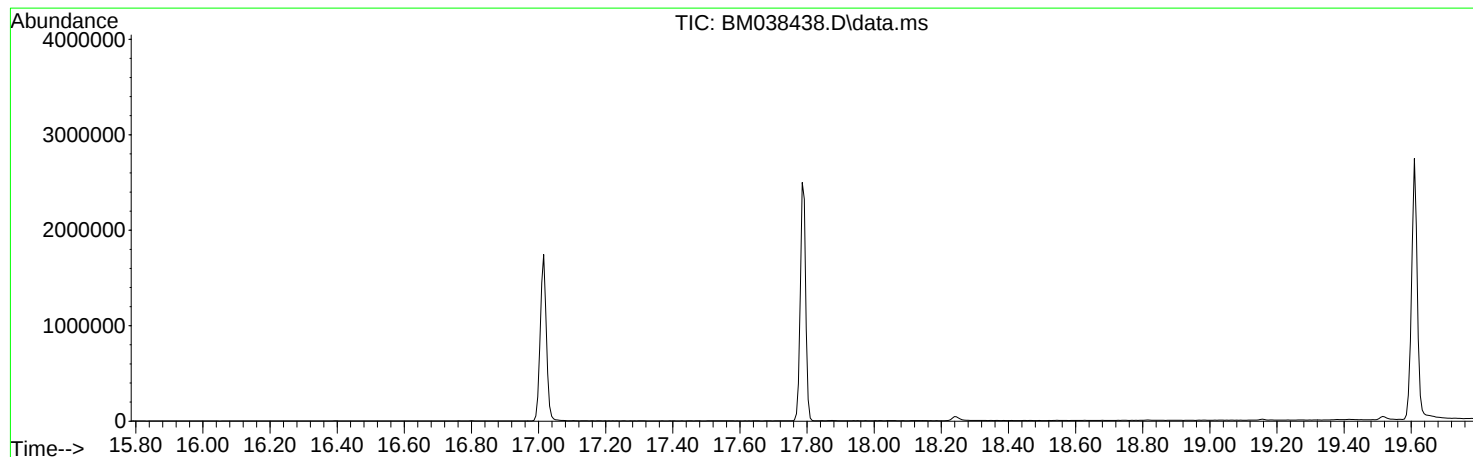




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.3	113648	PASS
68	69	0.00	2	1.6	1770	PASS
69	198	0.00	100	54.7	112384	PASS
70	69	0.00	2	0.5	563	PASS
127	198	10	80	50.1	102925	PASS
197	198	0.00	2	0.5	927	PASS
198	198	100	100	100.0	205568	PASS
199	198	5	9	6.7	13829	PASS
275	198	10	60	24.2	49757	PASS
365	198	1	100	3.5	7179	PASS
441	198	0.01	100	11.9	24469	PASS
442	442	50	100	100.0	145400	PASS
443	442	15	24	18.8	27321	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011323\
Data File : BM038438.D
Acq On : 12 Jan 2023 15:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 13 06:22:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 13 01:05:13 2023
Response via : Initial Calibration

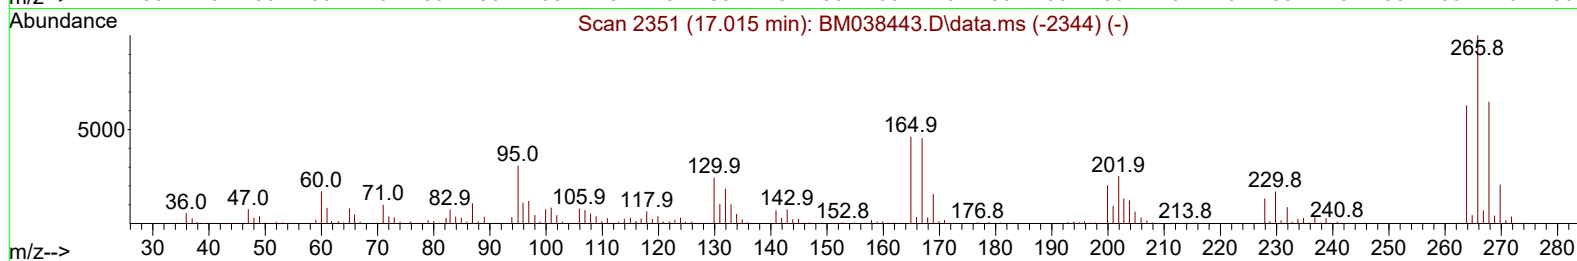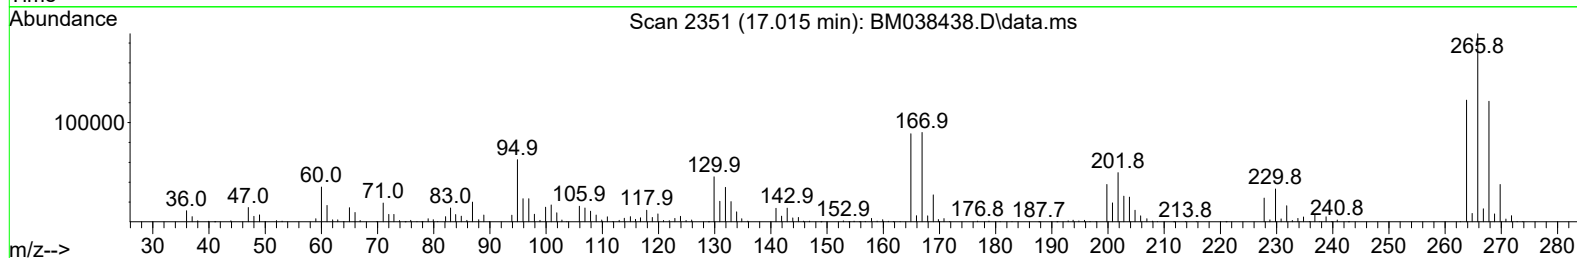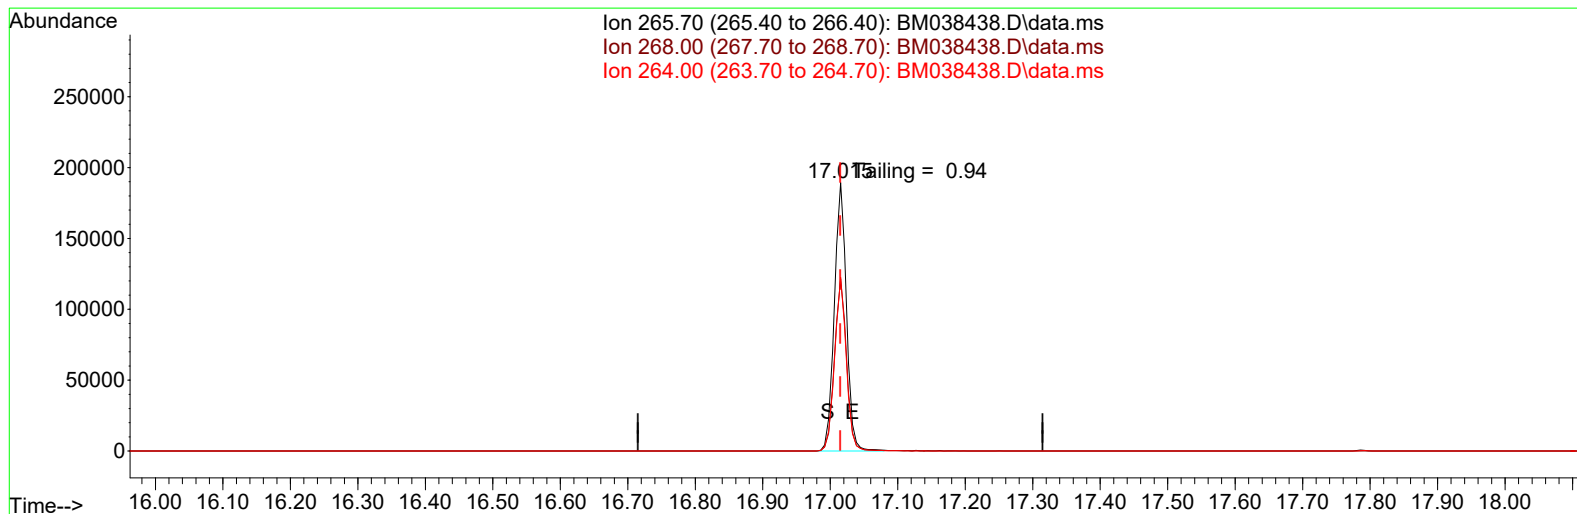

TIC: BM038438.D\data.ms

(70) Pentachlorophenol (C)

17.015min (+ 0.000) 0.00 ng




response 237495

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.15
264.00	62.70	64.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011323\
Data File : BM038438.D
Acq On : 12 Jan 2023 15:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 13 06:22:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 13 01:05:13 2023
Response via : Initial Calibration

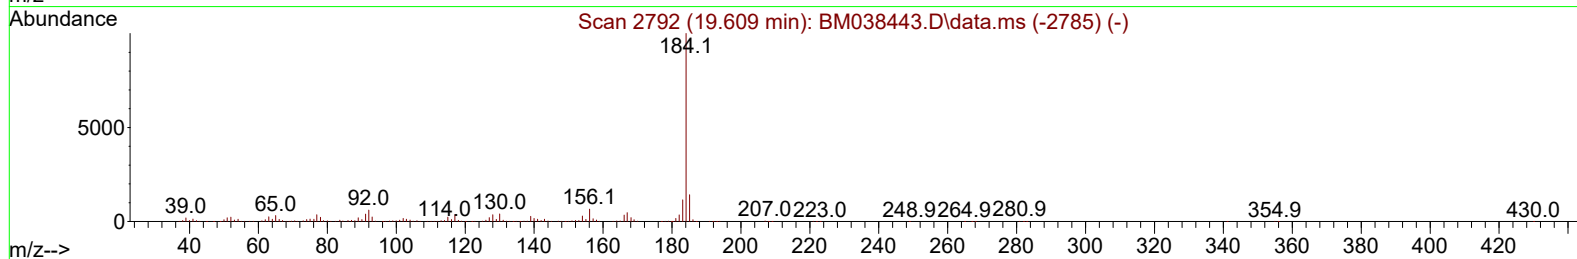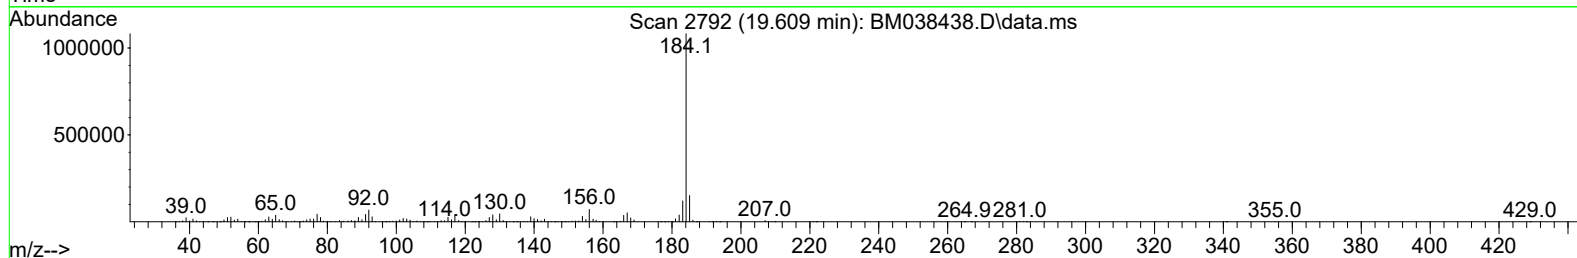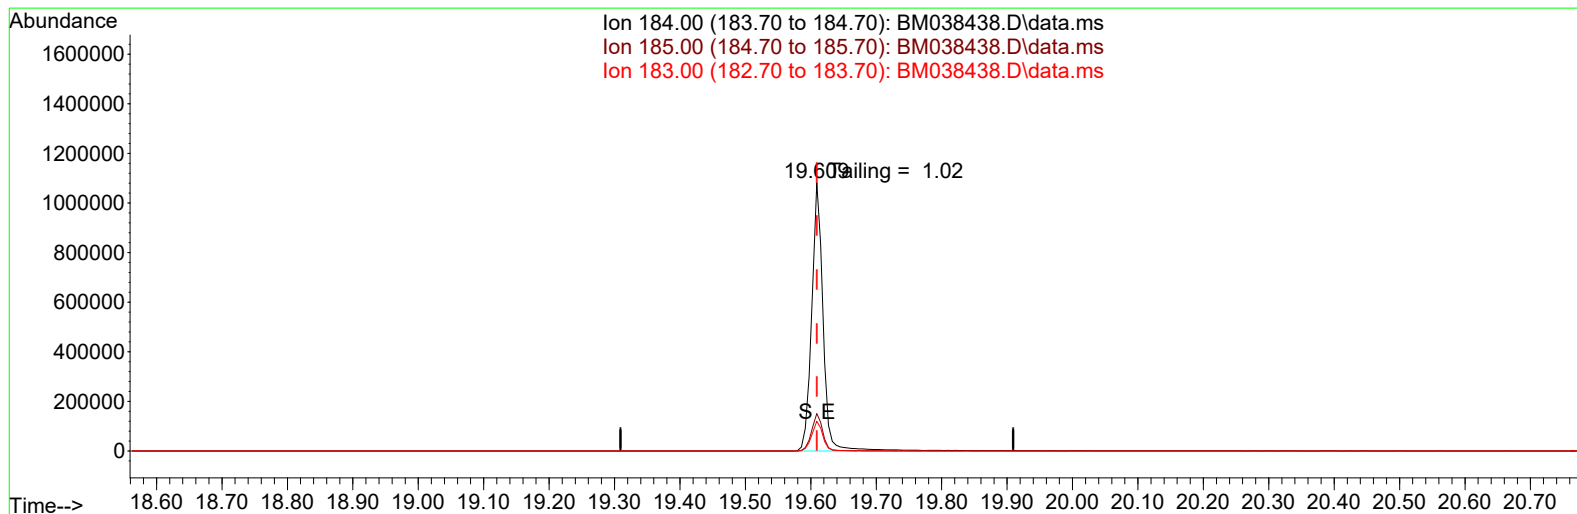

TIC: BM038438.D\data.ms

(77) Benzidine

19.609min (-0.000) 0.00 ng

response 1303215

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.98
183.00	11.50	11.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/13/2023	BNA_M	<u>BM038438.D</u>
Compound Name	Response	Retention Time
DDT	802643	20.827
DDD	5905	20.439
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5905	808548	0.73

Instrument :
BNA_M
ClientSampleId :
DFTPP