


Data Path : Z:\HPCHEM1\BNA M\Data\BM011415\
Data File : BM000187.D
Acq On : 14 Jan 2015 14:52
Operator : TP/IZ
Sample : DFTPP07
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ClientSampleId :

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Title : SVOA CALIBRATION
Last Update : Wed Jan 14 12:47:10 2015

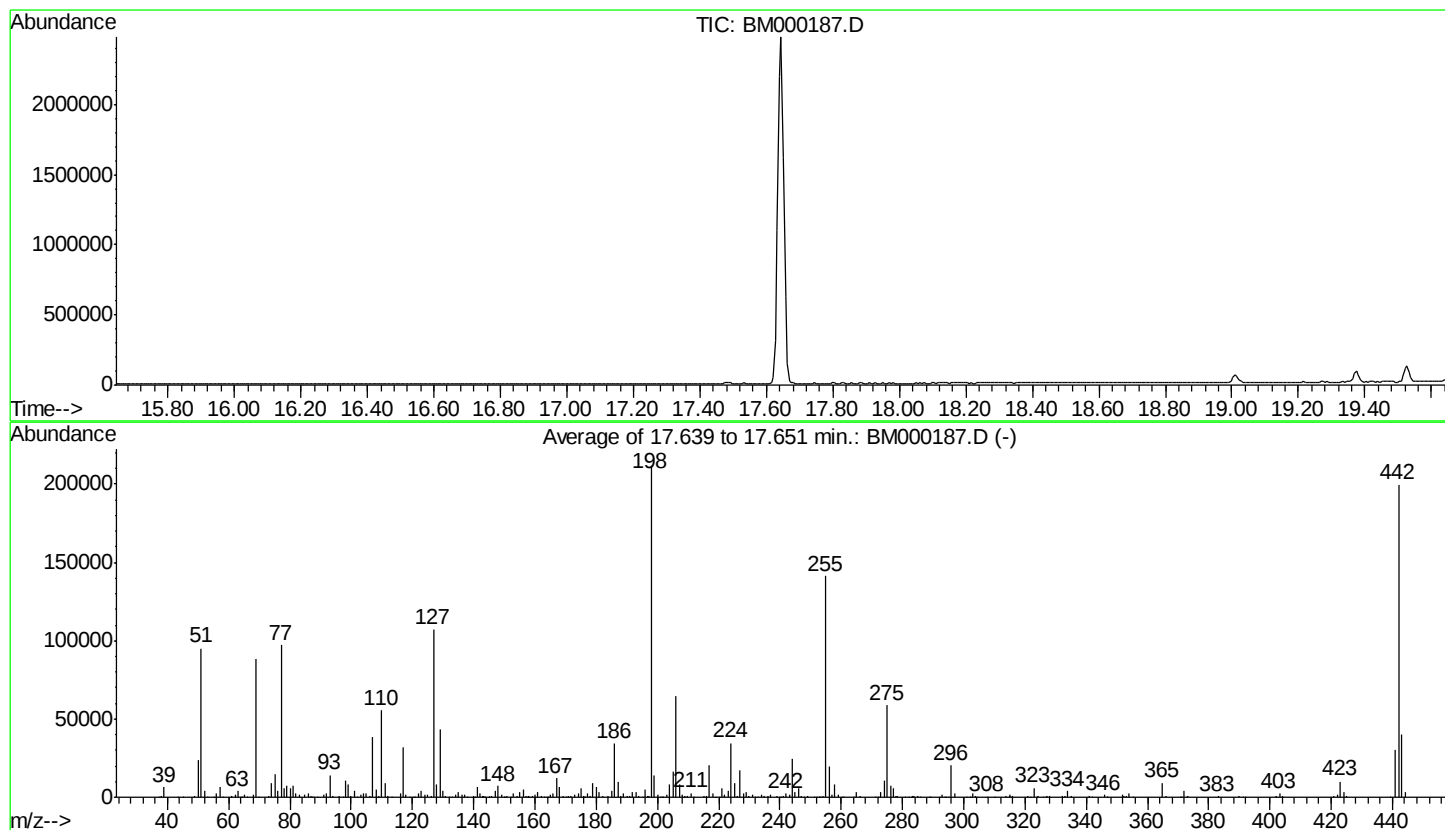

AutoFind: Scans 2542, 2543, 2544; Background Corrected with Scan 2536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	95032	PASS
68	69	0.00	2	1.6	1381	PASS
69	198	0.00	100	41.8	88637	PASS
70	69	0.00	2	0.5	413	PASS
127	198	10	80	50.4	106813	PASS
197	198	0.00	2	0.5	1102	PASS
198	198	100	100	100.0	211818	PASS
199	198	5	9	6.5	13675	PASS
275	198	10	60	27.7	58600	PASS
365	198	1	100	4.4	9346	PASS
441	443	0.01	100	75.6	30221	PASS
442	198	50	100	94.3	199786	PASS
443	442	15	24	20.0	39957	PASS