

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011415\
 Data File : BM000195.D
 Acq On : 14 Jan 2015 19:39
 Operator : TP/IZ
 Sample : G1063-08DL 25X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 C0AN7DL

Quant Time: Jan 14 22:19:24 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 14 21:49:10 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	116707	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	461202	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	309539	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	643496	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	737956	20.00	ng/ul	0.00
83) Perylene-d12	23.68	264	693770	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	292	0.15	ng/uL	0.00
5) Phenol-d5	6.99	99	3150	0.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	8004	1.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	6744	0.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	3490	0.45	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	3645	1.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	2985	0.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	5827	0.81	ng/ul	0.01
29) 4-Chloroaniline-d4	10.62	131	963	0.12	ng/ul	-0.14
43) Dimethylphthalate-d6	13.87	166	23139	1.01	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	26502	0.97	ng/ul	0.00
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.46	176	26047	1.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	1291	0.42	ng/ul	0.00
70) Anthracene-d10	17.30	188	37508	1.26	ng/ul	0.00
76) Pyrene-d10	19.60	212	38331	1.13	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.53	264	35304	1.12	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.35	88	31753	11.38	ng/uL	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011415\
Data File : BM000195.D
Acq On : 14 Jan 2015 19:39
Operator : TP/IZ
Sample : G1063-08DL 25X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ClientSampleId :
C0AN7DL

Quant Time: Jan 14 22:19:24 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 14 21:49:10 2015
Response via : Initial Calibration

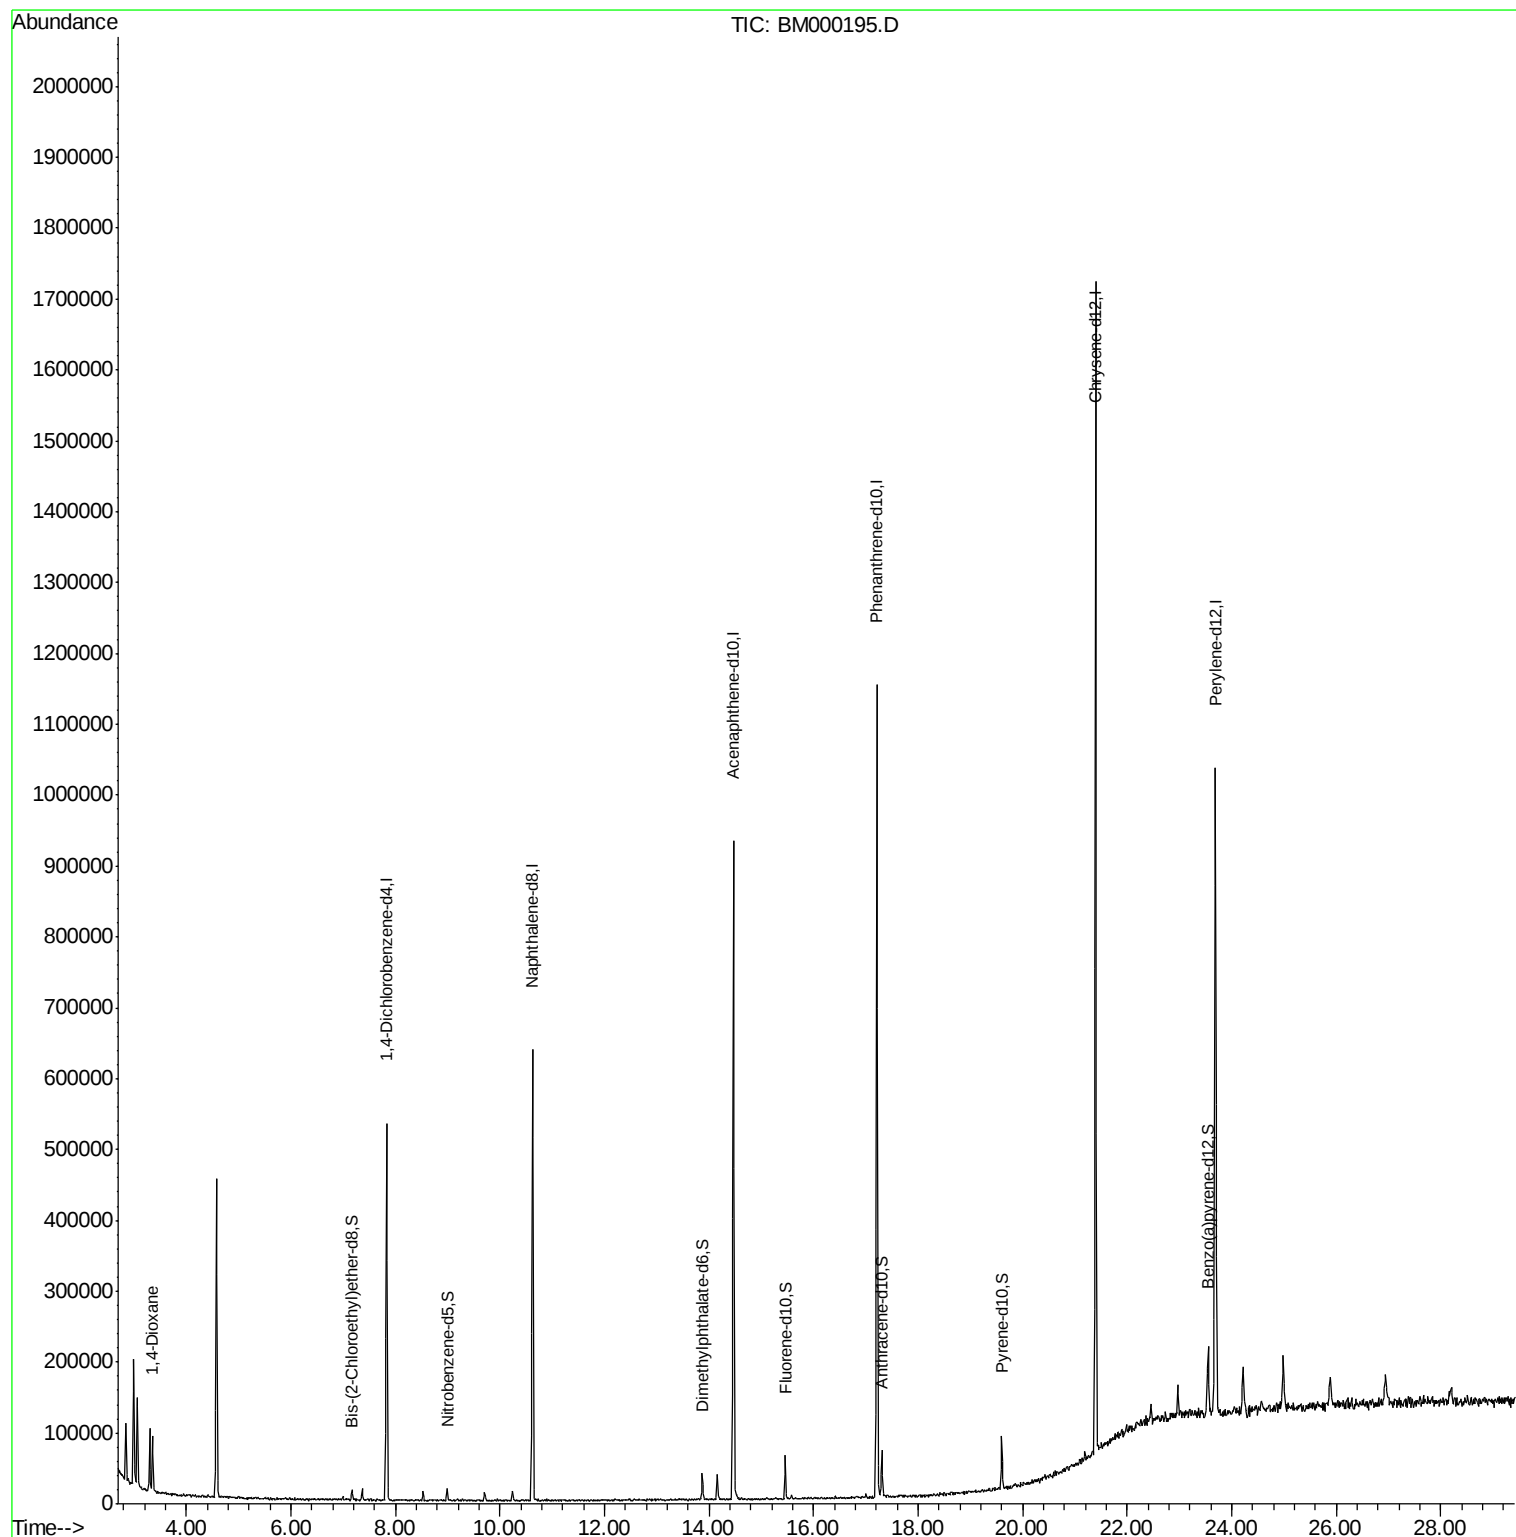

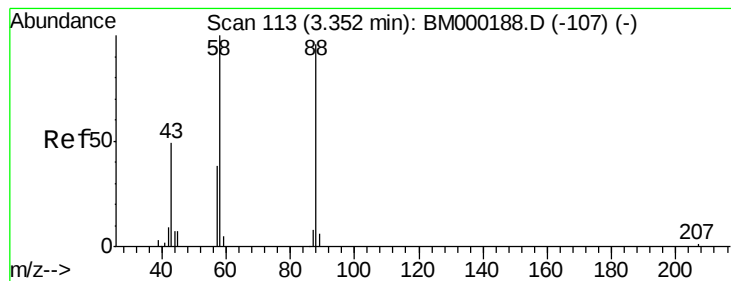

#2

1,4-Dioxane

Concen: 11.38 ng/uL

RT: 3.35 min Scan# 113

Delta R.T. 0.01 min

Lab File: BM000195.D

Acq: 14 Jan 2015 19:39

Instrument :

ClientSampleId :

C0AN7DL

Tgt Ion: 88 Resp: 31753

Ion Ratio Lower Upper

88 100

43 41.6 34.9 52.3

58 90.8 67.3 100.9

