

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011415\
 Data File : BM000190.D
 Acq On : 14 Jan 2015 16:41
 Operator : TP/IZ
 Sample : G1063-05DL 2X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 C0AN1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.840	21	26	46	rVV	3265301	4571842	16.70%	6.537%
2	2.987	46	51	59	rVV	384583	594716	2.17%	0.850%
3	3.058	59	63	76	rVB	1071799	1388793	5.07%	1.986%
4	3.293	97	103	111	rBV	11793512	16133623	58.94%	23.068%
5	4.152	245	249	256	rVB4	18932	30199	0.11%	0.043%
6	4.575	314	321	336	rBV	19276335	27373779	100.00%	39.139%
7	5.287	437	442	448	rVB2	43934	66272	0.24%	0.095%
8	6.987	725	731	739	rBV2	59514	99745	0.36%	0.143%
9	7.163	755	761	769	rBV	191746	300954	1.10%	0.430%
10	7.357	788	794	803	rVB	214971	338234	1.24%	0.484%
11	7.828	867	874	882	rBV	513956	830650	3.03%	1.188%
12	8.528	986	993	1000	rBV	159748	259589	0.95%	0.371%
13	8.987	1064	1071	1077	rBV	254572	425686	1.56%	0.609%
14	9.704	1185	1193	1200	rBV	204499	338217	1.24%	0.484%
15	10.234	1277	1283	1291	rBV	294404	488260	1.78%	0.698%
16	10.622	1341	1349	1357	rBV	648594	1091163	3.99%	1.560%
17	13.869	1895	1901	1907	rBV	689179	954732	3.49%	1.365%
18	14.157	1944	1950	1958	rBV	646132	948206	3.46%	1.356%
19	14.463	1996	2002	2011	rBV	960261	1379394	5.04%	1.972%
20	14.657	2029	2035	2042	rBV2	27753	49210	0.18%	0.070%
21	15.457	2165	2171	2180	rBV	891738	1294446	4.73%	1.851%
22	15.569	2185	2190	2197	rVV	220823	321154	1.17%	0.459%
23	17.204	2462	2468	2475	rBV2	1153125	1688775	6.17%	2.415%
24	17.304	2479	2485	2495	rVV	1053438	1505257	5.50%	2.152%
25	18.092	2615	2619	2625	rBV4	40718	58136	0.21%	0.083%
26	19.374	2834	2837	2842	rBV4	30908	41232	0.15%	0.059%
27	19.598	2869	2875	2882	rBV	1291299	1746772	6.38%	2.498%
28	21.098	3125	3130	3135	rBV3	86175	115970	0.42%	0.166%
29	21.392	3175	3180	3186	rBV	1603566	2013460	7.36%	2.879%
30	23.539	3537	3545	3553	rBV2	859364	1643511	6.00%	2.350%
31	23.686	3562	3570	3578	rVB	933953	1848780	6.75%	2.643%


Sum of corrected areas: 69940757

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011415\
Data File : BM000190.D
Acq On : 14 Jan 2015 16:41
Operator : TP/IZ
Sample : G1063-05DL 2X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ClientSampled :
C0AN1DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

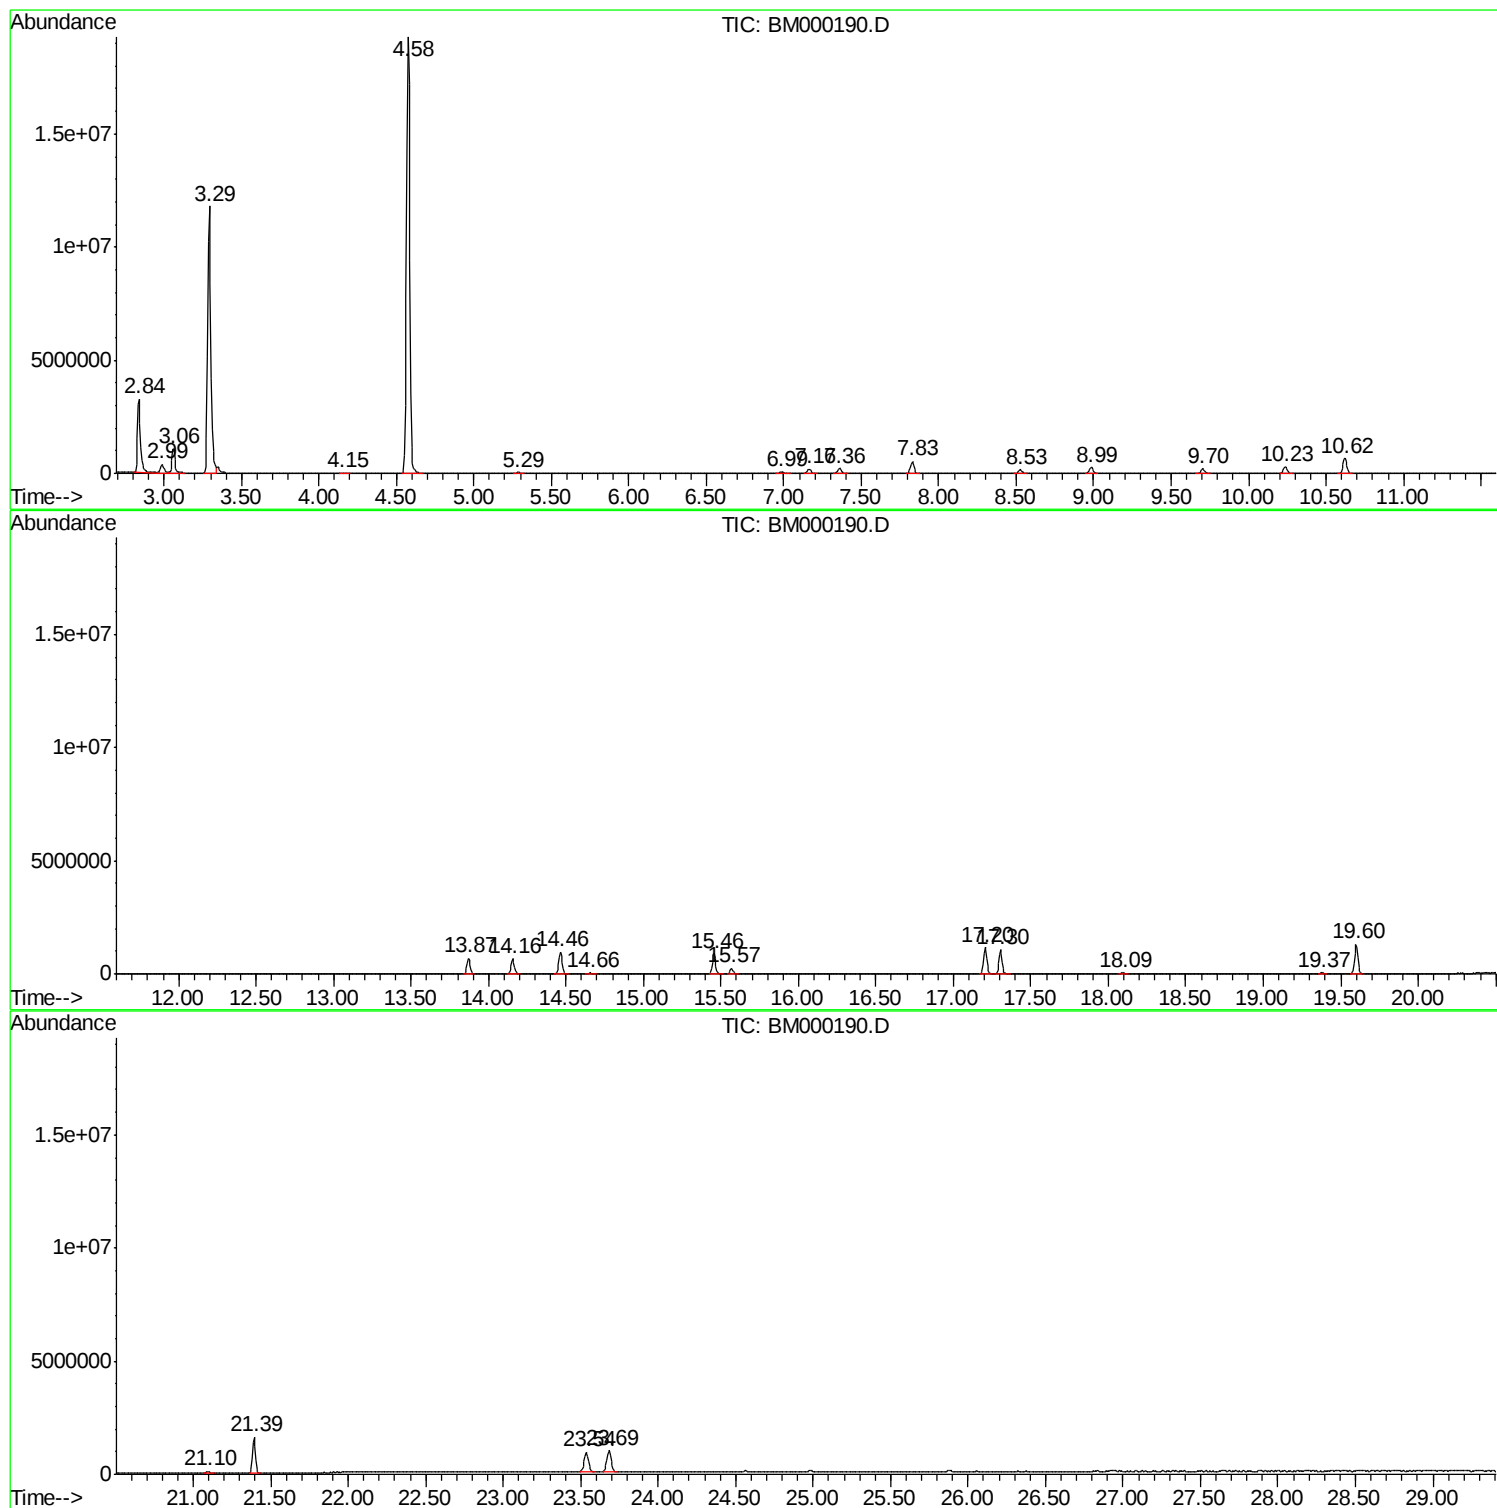

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011415\
Data File : BM000190.D
Acq On : 14 Jan 2015 16:41
Operator : TP/IZ
Sample : G1063-05DL 2X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ClientSampleId :
C0AN1DL










Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.06	33.44 ng/ul	1388790	1,4-Dichlorobenzene-d4	7.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
3		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4		Silane, tetramethyl-	88	C4H12Si	000075-76-3	38
5		Silane, tetramethyl-	88	C4H12Si	000075-76-3	17

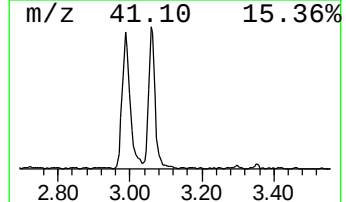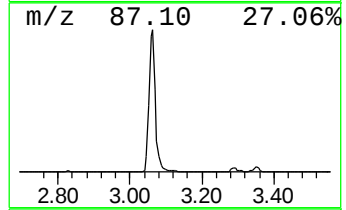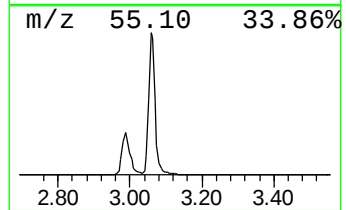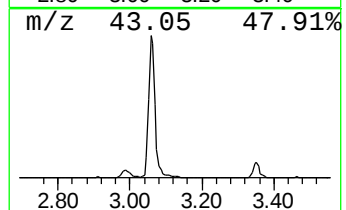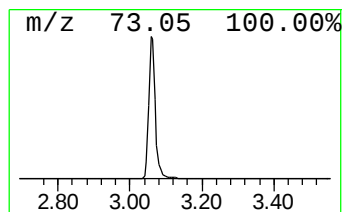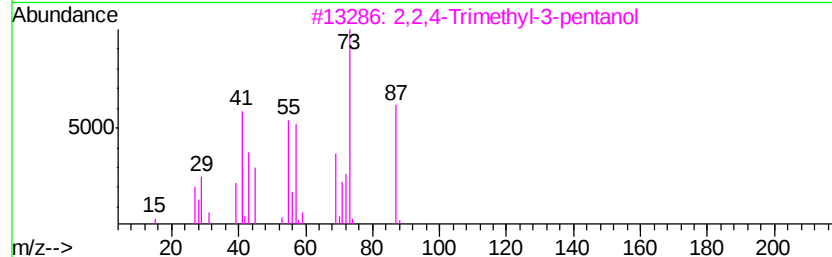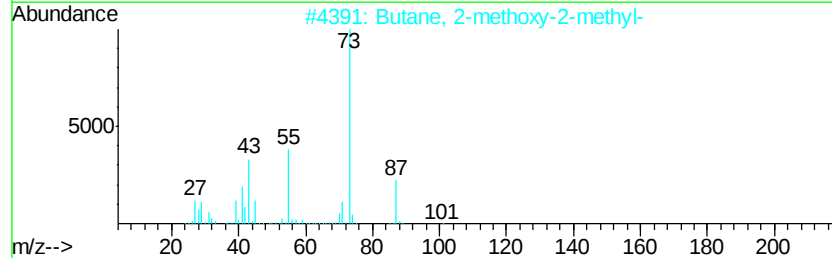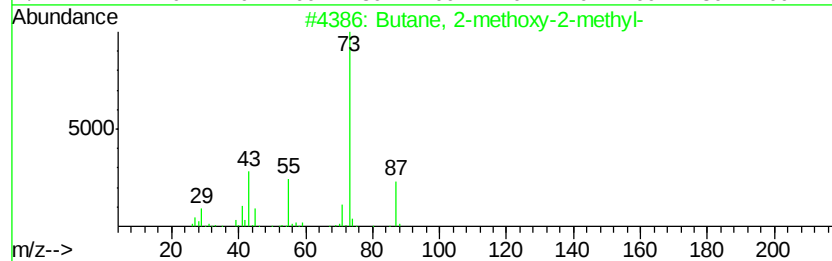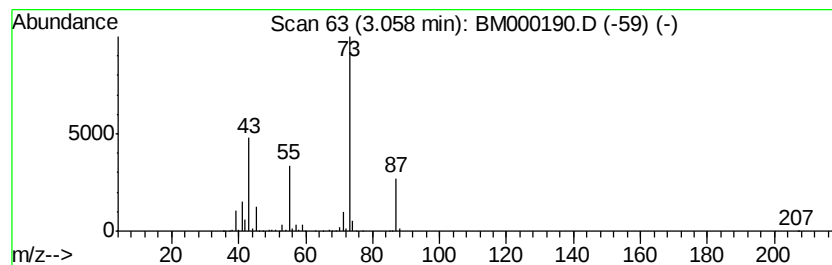

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011415\
Data File : BM000190.D
Acq On : 14 Jan 2015 16:41
Operator : TP/IZ
Sample : G1063-05DL 2X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ClientSampleId :
C0AN1DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Butane, 2-methoxy...	3.06	33.4	ng/ul	1388790	1	7.83	830650	20.0