


Data Path : Z:\HPCHEM1\BNA_M\Data\BM011415\
Data File : BM000187.D
Acq On : 14 Jan 2015 14:52
Operator : TP/IZ
Sample : DFTPP07
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ClientSampleId :
DFTPP07

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Title : SVOA CALIBRATION
Last Update : Wed Jan 14 12:47:10 2015

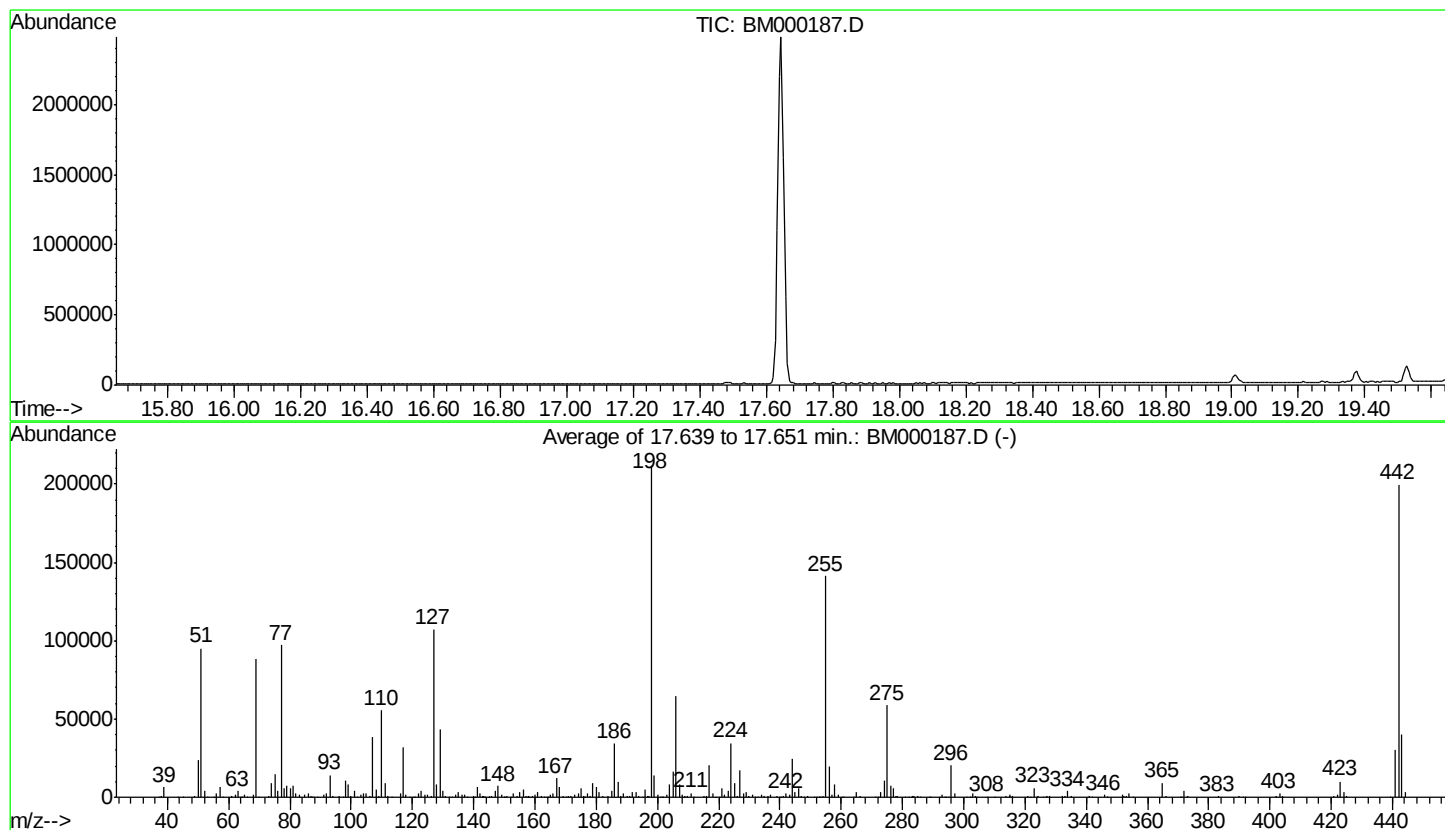

AutoFind: Scans 2542, 2543, 2544; Background Corrected with Scan 2536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	95032	PASS
68	69	0.00	2	1.6	1381	PASS
69	198	0.00	100	41.8	88637	PASS
70	69	0.00	2	0.5	413	PASS
127	198	10	80	50.4	106813	PASS
197	198	0.00	2	0.5	1102	PASS
198	198	100	100	100.0	211818	PASS
199	198	5	9	6.5	13675	PASS
275	198	10	60	27.7	58600	PASS
365	198	1	100	4.4	9346	PASS
441	443	0.01	100	75.6	30221	PASS
442	198	50	100	94.3	199786	PASS
443	442	15	24	20.0	39957	PASS

m/z	Abundance
36.90	473.0
38.00	1432.0
39.00	8492.0
40.00	3663.0
43.20	409.0
44.00	5426.0
49.00	885.0
50.10	29088.0
51.10	111672.0
52.10	5577.0
55.00	662.0
56.00	3366.0
57.00	8277.0
57.90	377.0
61.00	1477.0
62.00	1363.0
63.00	5122.0
64.20	602.0
65.00	2018.0
68.10	1269.0
69.00	105776.0
69.90	466.0
72.90	1089.0
74.00	10162.0
75.00	17600.0
76.00	5400.0
77.00	116728.0
78.00	7232.0
79.00	8533.0
80.00	5871.0
81.00	10407.0
82.00	2484.0
83.00	1983.0
85.00	1725.0
86.00	2469.0
86.90	1359.0
91.10	2347.0
92.00	2509.0
93.00	16744.0
94.10	829.0
96.00	747.0
98.00	14174.0
99.00	9848.0
100.00	866.0
101.00	6034.0
101.90	340.0
103.00	2071.0
104.10	3279.0
105.10	2550.0
106.10	1288.0
107.00	43544.0
108.00	5615.0
108.90	1147.0
110.00	61640.0
111.00	9873.0
112.00	1376.0
113.10	529.0
116.10	2114.0
117.00	35848.0
117.90	1977.0
120.10	520.0
120.90	307.0
122.00	2688.0
123.00	4470.0
124.10	1381.0
124.90	1674.0
126.00	463.0
127.00	120432.0
128.00	9579.0
129.00	48400.0
130.00	3998.0
131.00	1106.0
132.00	356.0
133.00	459.0
134.00	1524.0
135.00	3562.0
136.10	1597.0
136.90	1853.0
137.90	612.0
139.80	418.0
140.20	461.0
141.10	6131.0
141.90	2370.0
142.90	1555.0
143.90	407.0
144.90	491.0
145.90	1365.0
147.00	4130.0
148.00	7786.0
149.00	1650.0
149.80	547.0

Instrument :
ClientSampleId :
DFTPP07

151.10	739.0
151.90	624.0
153.00	2999.0
154.00	1470.0
155.00	3654.0
156.10	5790.0
157.00	1420.0
157.90	1313.0
158.90	1041.0
160.10	1317.0
161.00	3150.0
162.10	1176.0
163.00	315.0
163.90	414.0
164.90	2619.0
166.00	2378.0
167.00	12362.0
168.00	7273.0
169.00	1202.0
170.90	766.0
171.90	1490.0
173.10	1491.0
174.00	3301.0
175.10	5527.0
176.00	1202.0
177.00	2631.0
178.00	570.0
178.90	9611.0
180.00	7830.0
181.00	4541.0
181.90	361.0
183.90	800.0
185.10	3862.0
186.00	37672.0
187.00	10367.0
187.90	1054.0
189.10	2190.0
190.00	391.0
190.90	1542.0
192.00	3385.0
193.10	3441.0
194.00	767.0
194.90	523.0
196.00	5635.0
196.90	1593.0
198.00	226752.0
199.00	15535.0
200.10	1637.0
201.00	329.0
201.40	444.0
201.70	432.0
203.10	2141.0
204.10	8197.0
205.10	16544.0
206.10	65216.0
207.10	11186.0
208.00	2403.0
209.00	681.0
210.00	1057.0
211.00	3147.0
212.00	351.0
215.10	975.0
216.00	781.0
217.00	20320.0
218.00	2734.0
219.10	312.0
220.00	481.0
221.00	5774.0
221.90	2075.0
223.10	4061.0
224.00	34312.0
225.00	9341.0
226.10	1533.0
227.00	17760.0
228.00	2417.0
228.90	2899.0
229.80	340.0
231.00	944.0
234.00	1067.0
235.00	877.0
235.90	754.0
237.00	1691.0
239.10	884.0
239.90	644.0
241.10	856.0
242.00	2430.0
243.00	1485.0
244.10	24856.0
245.00	3037.0
246.00	6383.0
247.10	1488.0
249.00	1029.0
251.10	328.0
253.10	636.0
254.10	1219.0

Instrument :
ClientSampleId :
DFTPP07

255.00	133184.0
256.00	19800.0
257.00	1574.0
258.00	7512.0
259.00	1452.0
260.20	313.0
264.00	341.0
265.10	3566.0
266.10	779.0
271.90	311.0
272.90	3868.0
274.00	9605.0
275.00	57864.0
276.00	7013.0
277.00	5093.0
277.80	593.0
278.20	508.0
282.80	438.0
283.10	531.0
283.90	699.0
285.00	630.0
285.80	342.0
288.90	319.0
292.10	459.0
293.00	1258.0
294.00	365.0
295.00	420.0
296.00	19856.0
297.00	2486.0
301.00	373.0
303.00	2081.0
304.00	647.0
307.70	354.0
310.10	336.0
313.90	470.0
314.90	1989.0
315.90	1359.0
321.00	617.0
321.80	329.0
323.00	5755.0
323.90	812.0
325.90	433.0
327.10	1425.0
328.10	430.0
332.20	536.0
332.90	605.0
334.00	3546.0
335.10	816.0
341.20	797.0
341.80	368.0
345.90	1383.0
352.00	1620.0
353.00	851.0
354.00	1791.0
355.00	521.0
365.00	8900.0
366.00	1326.0
370.80	551.0
372.10	3009.0
372.80	412.0
383.10	753.0
389.90	452.0
390.90	482.0
402.10	1226.0
403.00	2364.0
403.90	472.0
421.10	735.0
421.90	1586.0
423.00	8470.0
423.90	3598.0
425.10	584.0
441.00	25408.0
442.00	164352.0
443.00	31928.0
444.10	3588.0

Instrument :
ClientSampleId :
DFTPP07

m/z	Abundance
37.00	506.0
38.00	1209.0
39.00	7173.0
40.00	3602.0
44.00	5517.0
45.00	305.0
49.00	630.0
50.10	26136.0
51.00	111024.0
52.10	5215.0
53.10	345.0
55.00	657.0
56.10	2944.0
57.00	7391.0
61.00	1060.0
62.10	2222.0
63.10	4531.0
63.90	502.0
65.00	1832.0
65.90	463.0
68.00	1682.0
69.00	99648.0
69.90	439.0
72.90	988.0
74.00	10553.0
75.00	18280.0
76.00	5385.0
77.10	109800.0
78.10	7602.0
79.00	8369.0
80.00	7209.0
81.00	7773.0
82.00	2643.0
83.00	2086.0
85.00	1803.0
85.90	3402.0
87.00	1142.0
87.90	624.0
89.00	300.0
90.90	1405.0
92.00	2730.0
93.00	15958.0
94.00	824.0
96.00	427.0
98.00	11490.0
99.00	9100.0
99.90	954.0
101.00	4006.0
103.10	1021.0
103.90	3503.0
104.90	2627.0
106.00	1380.0
107.00	47168.0
107.90	5588.0
108.90	1296.0
110.00	65328.0
111.00	10404.0
112.10	1284.0
112.90	610.0
116.10	2363.0
117.00	36352.0
118.00	2073.0
118.90	453.0
120.10	666.0
120.90	434.0
122.10	2918.0
123.00	3886.0
124.00	2089.0
125.00	1389.0
126.10	934.0
127.00	123928.0
128.00	8881.0
129.00	51416.0
130.00	4249.0
130.90	957.0
134.10	1268.0
135.00	3965.0
135.90	2636.0
137.10	2139.0
137.90	494.0
139.90	894.0
141.00	8313.0
142.00	2246.0
142.80	1198.0
143.20	1460.0
143.90	490.0
145.10	522.0
146.00	736.0
147.10	4997.0
148.00	8080.0
149.00	1562.0

Instrument :
ClientSampleId :
DFTPP07

150.00	533.0
150.90	695.0
151.90	392.0
153.00	2685.0
154.00	1305.0
155.10	4612.0
156.00	6520.0
157.00	882.0
158.10	1232.0
159.00	1768.0
160.00	2141.0
161.00	3563.0
162.10	1624.0
162.90	772.0
163.90	354.0
165.10	2551.0
166.10	2181.0
167.00	14253.0
168.00	8081.0
169.00	1447.0
170.10	606.0
170.80	682.0
171.90	1423.0
173.00	1871.0
174.10	2972.0
175.00	7093.0
176.10	1541.0
177.10	3252.0
178.00	944.0
179.00	10567.0
180.00	6225.0
181.10	3730.0
182.00	802.0
183.90	765.0
185.10	5019.0
186.10	40416.0
187.00	12249.0
188.00	682.0
189.00	3688.0
190.00	610.0
190.90	923.0
192.00	2723.0
193.10	4086.0
193.90	1412.0
195.00	475.0
196.00	5541.0
197.10	2260.0
198.00	250112.0
199.00	16680.0
200.00	1862.0
201.20	743.0
201.70	727.0
203.00	2514.0
204.00	10014.0
205.10	19976.0
206.10	78048.0
207.10	10815.0
208.10	2608.0
209.00	1382.0
209.90	1627.0
211.00	2357.0
215.00	1111.0
215.90	1494.0
217.00	24152.0
218.10	2036.0
221.00	6180.0
222.10	2348.0
223.00	6081.0
224.00	42320.0
225.00	10193.0
225.90	974.0
227.00	21752.0
228.10	2410.0
229.00	3720.0
229.90	811.0
230.90	1378.0
232.10	304.0
232.90	451.0
234.00	1989.0
234.80	1144.0
236.00	1039.0
237.00	2021.0
239.00	606.0
240.10	420.0
241.00	1152.0
242.00	2695.0
243.00	2641.0
244.00	28312.0
245.00	3630.0
246.00	7135.0
247.00	1446.0
248.00	324.0
248.90	1316.0
251.90	771.0
252.90	663.0

Instrument :
ClientSampleId :
DFTPP07

254.10	1361.0
255.00	170560.0
256.00	23216.0
257.00	2191.0
258.00	10579.0
259.10	2313.0
260.90	318.0
264.10	573.0
265.00	4201.0
265.90	561.0
271.10	465.0
273.00	3962.0
274.10	12439.0
275.00	72008.0
276.00	8935.0
277.00	8025.0
278.10	1354.0
280.90	352.0
282.00	310.0
283.00	833.0
283.80	488.0
285.00	1423.0
289.10	464.0
292.00	506.0
293.00	1647.0
294.10	429.0
296.00	24048.0
297.00	3446.0
302.00	471.0
303.00	2666.0
303.80	1193.0
307.80	600.0
314.00	1315.0
315.10	2723.0
315.90	874.0
316.10	924.0
321.00	688.0
323.00	6777.0
324.10	1018.0
327.10	1412.0
328.10	597.0
332.10	581.0
332.80	818.0
334.00	5009.0
335.00	1270.0
341.00	1156.0
346.00	1619.0
346.70	409.0
347.00	460.0
352.20	3122.0
353.00	1552.0
354.10	2505.0
365.00	11341.0
365.90	1041.0
370.90	728.0
372.00	4327.0
373.10	625.0
383.00	844.0
389.90	824.0
391.00	521.0
391.90	363.0
402.00	1736.0
403.10	2259.0
403.90	987.0
421.00	1477.0
422.00	2161.0
423.00	13309.0
424.00	3428.0
425.00	532.0
439.10	373.0
441.00	36504.0
442.00	240576.0
443.00	47896.0
444.00	3901.0

Instrument :
ClientSampleId :
DFTPP07

m/z	Abundance
38.00	827.0
39.10	3064.0
40.00	3641.0
44.00	5970.0
45.00	309.0
49.00	657.0
50.10	14842.0
51.10	62400.0
52.10	2518.0
56.10	2173.0
57.00	4656.0
61.00	814.0
62.00	996.0
63.00	2301.0
63.90	510.0
65.00	1310.0
68.00	1192.0
69.00	60488.0
69.90	336.0
73.00	1322.0
74.00	6099.0
75.00	9332.0
76.10	2743.0
77.10	65336.0
78.10	3390.0
78.90	4403.0
80.10	3572.0
81.00	4979.0
82.00	1658.0
83.00	1525.0
84.90	1219.0
86.00	1887.0
87.20	597.0
91.00	1398.0
92.00	1616.0
93.00	9112.0
94.10	540.0
96.10	754.0
97.20	309.0
98.00	6667.0
99.00	5079.0
100.10	413.0
101.10	2705.0
103.00	858.0
104.00	1815.0
105.00	2338.0
106.00	350.0
107.00	25840.0
108.10	3541.0
109.00	581.0
110.00	39448.0
111.00	6724.0
112.00	724.0
116.00	1757.0
117.00	23960.0
118.00	1657.0
122.00	1833.0
122.90	3155.0
124.10	1231.0
124.90	1300.0
127.00	76080.0
128.00	5697.0
129.00	31448.0
129.90	3172.0
131.00	709.0
132.90	311.0
134.00	1081.0
135.00	2649.0
135.90	1252.0
137.00	1873.0
139.90	350.0
141.00	5064.0
142.10	1676.0
143.00	1112.0
144.90	433.0
146.00	618.0
147.00	2416.0
148.10	5424.0
148.90	1237.0
150.90	655.0
153.10	1970.0
154.10	975.0
155.00	2639.0
156.00	3067.0
156.80	688.0
157.30	322.0
157.90	775.0
159.10	731.0
159.90	1075.0
161.00	2758.0
162.00	368.0

Instrument :
ClientSampleId :
DFTPP07

164.20	408.0
165.10	1876.0
165.90	1730.0
167.10	9212.0
168.00	4739.0
169.00	1116.0
170.90	566.0
171.90	799.0
173.00	642.0
174.00	2204.0
175.00	3647.0
175.80	1114.0
176.30	856.0
177.00	2482.0
177.90	578.0
179.00	7548.0
180.00	4787.0
180.90	2260.0
182.00	414.0
185.10	4580.0
186.00	24032.0
187.10	7655.0
188.00	689.0
189.10	1806.0
189.80	509.0
190.80	730.0
191.90	2928.0
193.00	3068.0
193.90	609.0
196.10	4280.0
196.80	932.0
197.10	1048.0
198.00	158592.0
198.90	8811.0
200.10	1124.0
203.00	1402.0
204.00	7144.0
205.00	12402.0
206.10	50584.0
207.00	6755.0
208.00	1660.0
209.10	719.0
209.90	1053.0
211.10	2321.0
215.90	1262.0
217.00	15762.0
218.00	1763.0
221.10	4742.0
222.00	2082.0
223.10	3077.0
224.00	27200.0
225.00	6822.0
226.00	364.0
227.00	11431.0
227.90	2243.0
229.00	2338.0
230.00	320.0
231.00	1560.0
234.00	1147.0
234.90	839.0
236.00	741.0
237.00	917.0
239.00	878.0
240.10	592.0
241.10	380.0
242.10	1380.0
243.00	1063.0
244.10	19928.0
245.10	2206.0
246.00	4223.0
247.10	762.0
247.90	467.0
248.90	435.0
252.70	307.0
253.30	830.0
254.20	954.0
255.00	120304.0
256.00	15547.0
257.10	1206.0
258.00	6432.0
259.00	1292.0
263.90	388.0
265.10	3334.0
272.00	744.0
273.00	2587.0
274.00	10012.0
275.00	45928.0
276.00	6606.0
277.00	3974.0
277.90	953.0
283.20	561.0
284.00	331.0
285.00	737.0
289.00	333.0
293.00	1097.0

Instrument :
ClientSampleId :
DFTPP07

293.80	404.0
294.80	487.0
296.00	16544.0
297.00	1961.0
302.20	481.0
303.00	2547.0
304.20	757.0
313.90	919.0
314.90	2397.0
316.10	566.0
320.80	431.0
323.00	5124.0
324.10	724.0
326.80	1185.0
328.00	980.0
332.10	313.0
333.00	682.0
334.00	3072.0
335.10	846.0
341.00	839.0
345.90	1145.0
352.00	2220.0
353.10	1351.0
354.10	2315.0
365.00	7797.0
366.00	1234.0
371.10	549.0
372.10	3947.0
373.10	1128.0
383.00	734.0
390.00	506.0
391.00	306.0
401.80	1209.0
403.00	2363.0
403.90	620.0
420.90	1508.0
422.10	1457.0
423.00	8687.0
424.00	3307.0
425.00	639.0
441.00	28752.0
442.00	194432.0
443.00	40048.0
444.00	2697.0

Instrument :
ClientSampleId :
DFTPP07

Scan 2536 (17.604 min): BM000187.D
DFTPP07

m/z	Abundance
40.00	4018.0
44.00	5710.0
73.00	517.0
207.10	1374.0
208.10	388.0

Instrument :
ClientSampleId :
DFTPP07