

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011416\
 Data File : BM003999.D
 Acq On : 13 Jan 2016 23:54
 Operator : SJ/UM
 Sample : H1098-20
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC971

Quant Time: Jan 14 11:15:16 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 13 06:45:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	41654	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	199322	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.32	164	118881	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.07	188	264099	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	241054	20.00	ng/ul	0.00
86) Perylene-d12	23.51	264	201640	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	4970	5.34	ng/uL	0.00
5) Phenol-d5	6.84	99	120634	34.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	71062	36.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	100795	35.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	105086	37.50	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	51225	34.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	57403	34.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	100174	34.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	132963	34.44	ng/ul	0.00
44) Dimethylphthalate-d6	13.73	166	346893	37.17	ng/ul	0.00
47) Acenaphthylene-d8	14.01	160	427102	37.56	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	56885	33.94	ng/ul	0.00
58) Fluorene-d10	15.32	176	308208	38.93	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	43253	29.04	ng/ul	0.00
71) Anthracene-d10	17.17	188	482252	39.48	ng/ul	0.00
79) Pyrene-d10	19.47	212	508840	40.76	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	403837	40.10	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.78	163	193862	20.38	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011416\
Data File : BM003999.D
Acq On : 13 Jan 2016 23:54
Operator : SJ/UM
Sample : H1098-20
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC971

Quant Time: Jan 14 11:15:16 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 13 06:45:02 2016
Response via : Initial Calibration

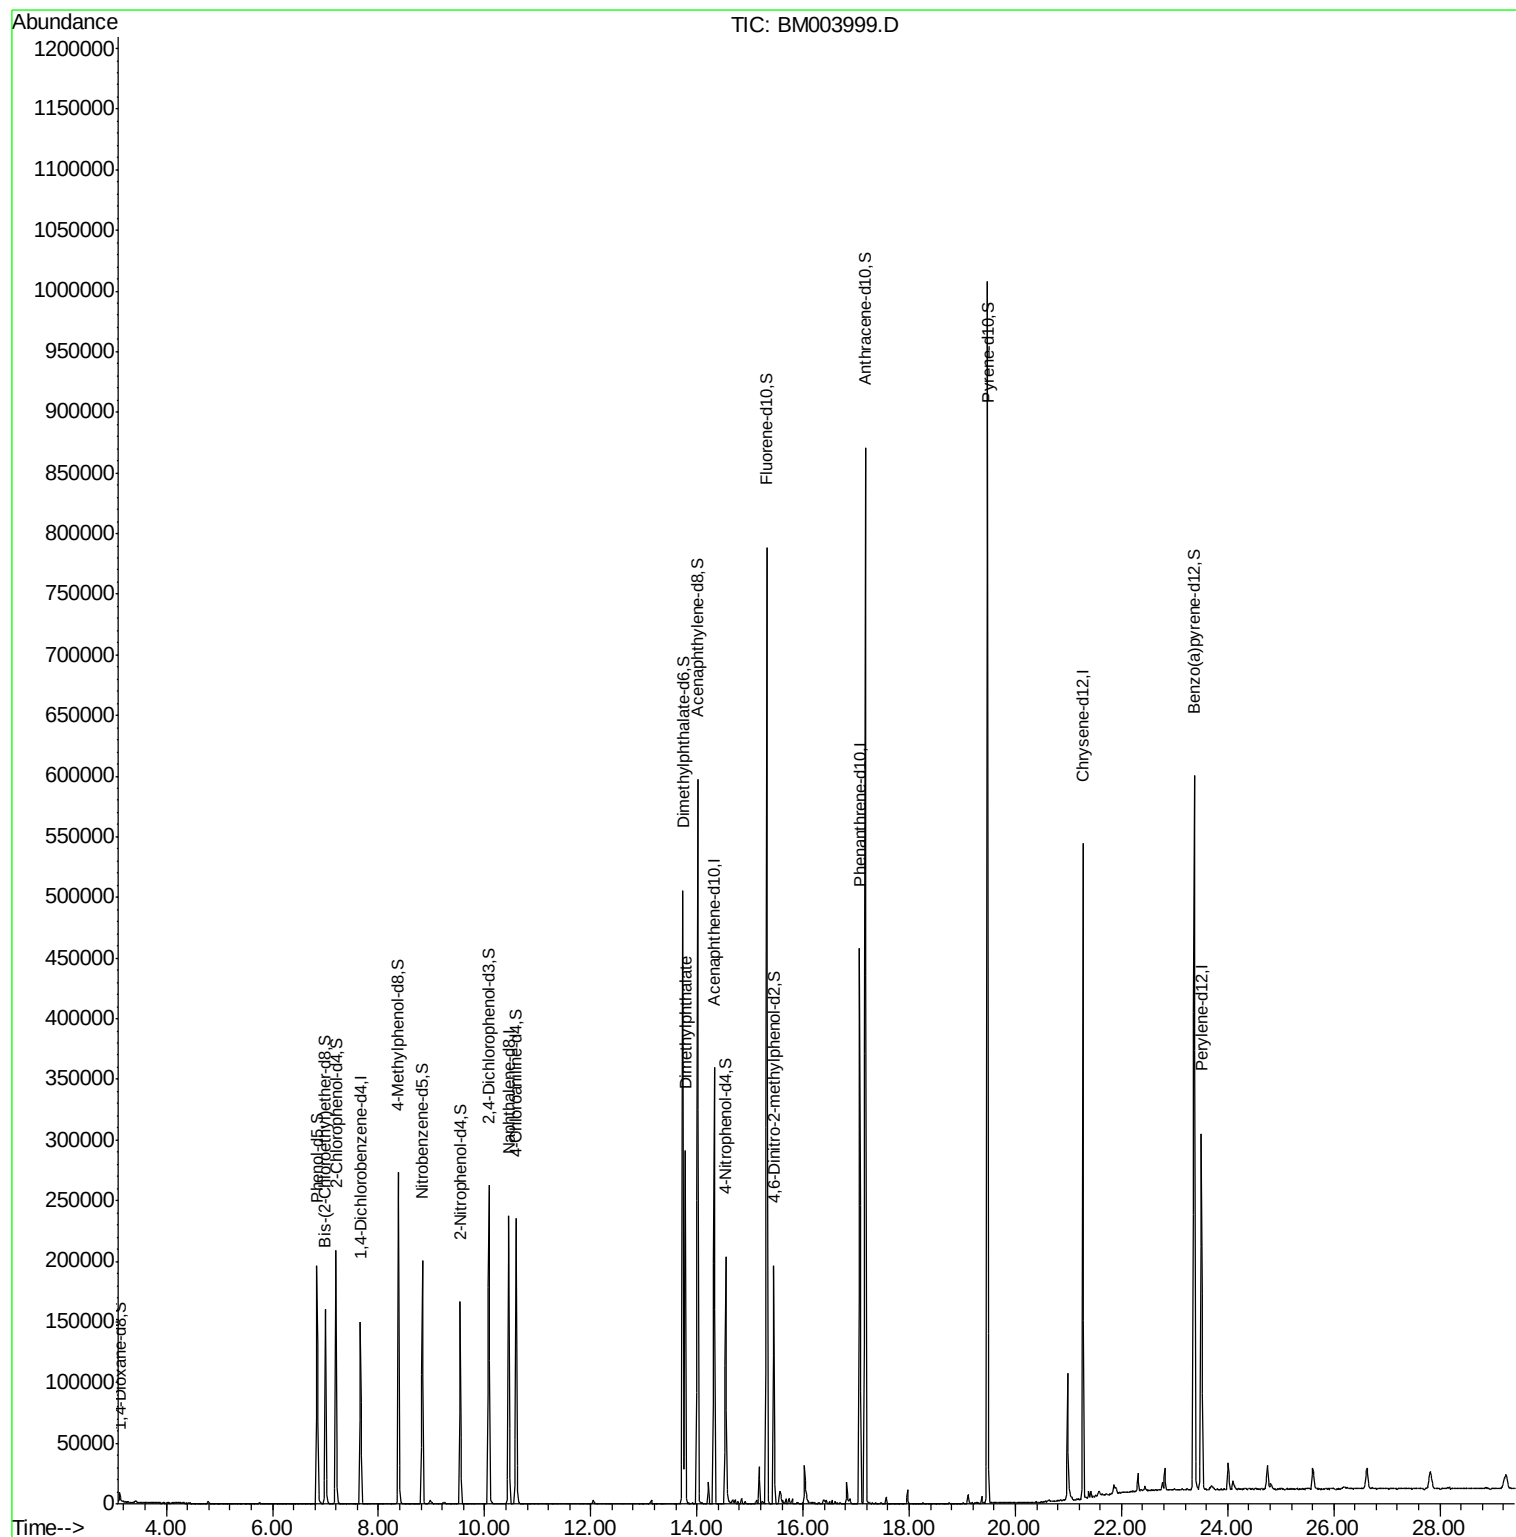

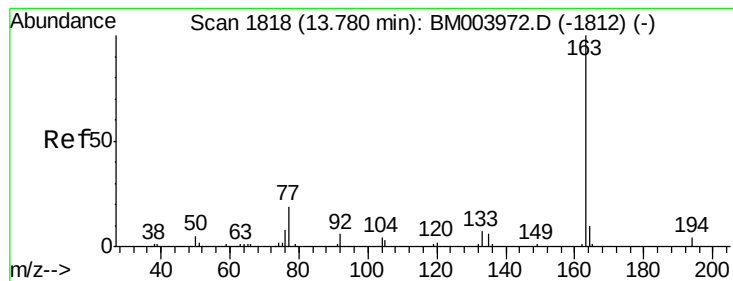

#45

Dimethylphthalate

Concen: 20.38 ng/ul

RT: 13.78 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BM003999.D


Acq: 13 Jan 2016 23:54

Instrument :

BNA_M

ClientSampleId :

BC971

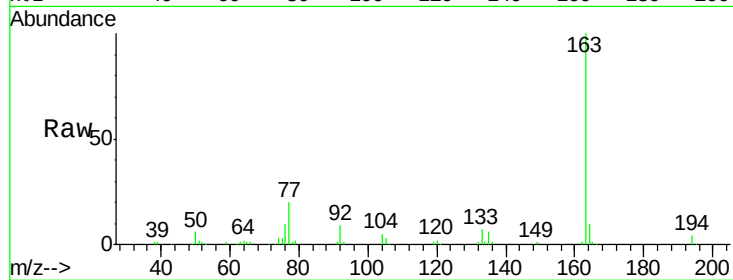

Tgt Ion:	163	Resp:	193862
Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.2	4.8
164	10.0	7.8	11.8

