

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011416\
 Data File : BM003992.D
 Acq On : 13 Jan 2016 19:45
 Operator : SJ/UM
 Sample : H1098-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC949

Quant Time: Jan 14 10:51:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 13 06:45:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	35070	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	170695	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.32	164	102182	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.07	188	230952	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	233275	20.00	ng/ul	0.00
86) Perylene-d12	23.52	264	186947	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	3977	5.07	ng/uL	0.00
5) Phenol-d5	6.84	99	97617	33.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	57336	34.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	81881	34.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	83716	35.48	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	42121	32.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	46812	33.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	82058	32.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	123128	37.24	ng/ul	0.00
44) Dimethylphthalate-d6	13.73	166	283523	35.34	ng/ul	0.00
47) Acenaphthylene-d8	14.01	160	348446	35.66	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	44521	30.90	ng/ul	0.00
58) Fluorene-d10	15.32	176	249061	36.60	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	34433	26.44	ng/ul	0.00
71) Anthracene-d10	17.17	188	392150	36.71	ng/ul	0.00
79) Pyrene-d10	19.47	212	433321	35.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	355408	38.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.78	163	162285	19.84	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011416\
Data File : BM003992.D
Acq On : 13 Jan 2016 19:45
Operator : SJ/UM
Sample : H1098-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC949

Quant Time: Jan 14 10:51:13 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 13 06:45:02 2016
Response via : Initial Calibration

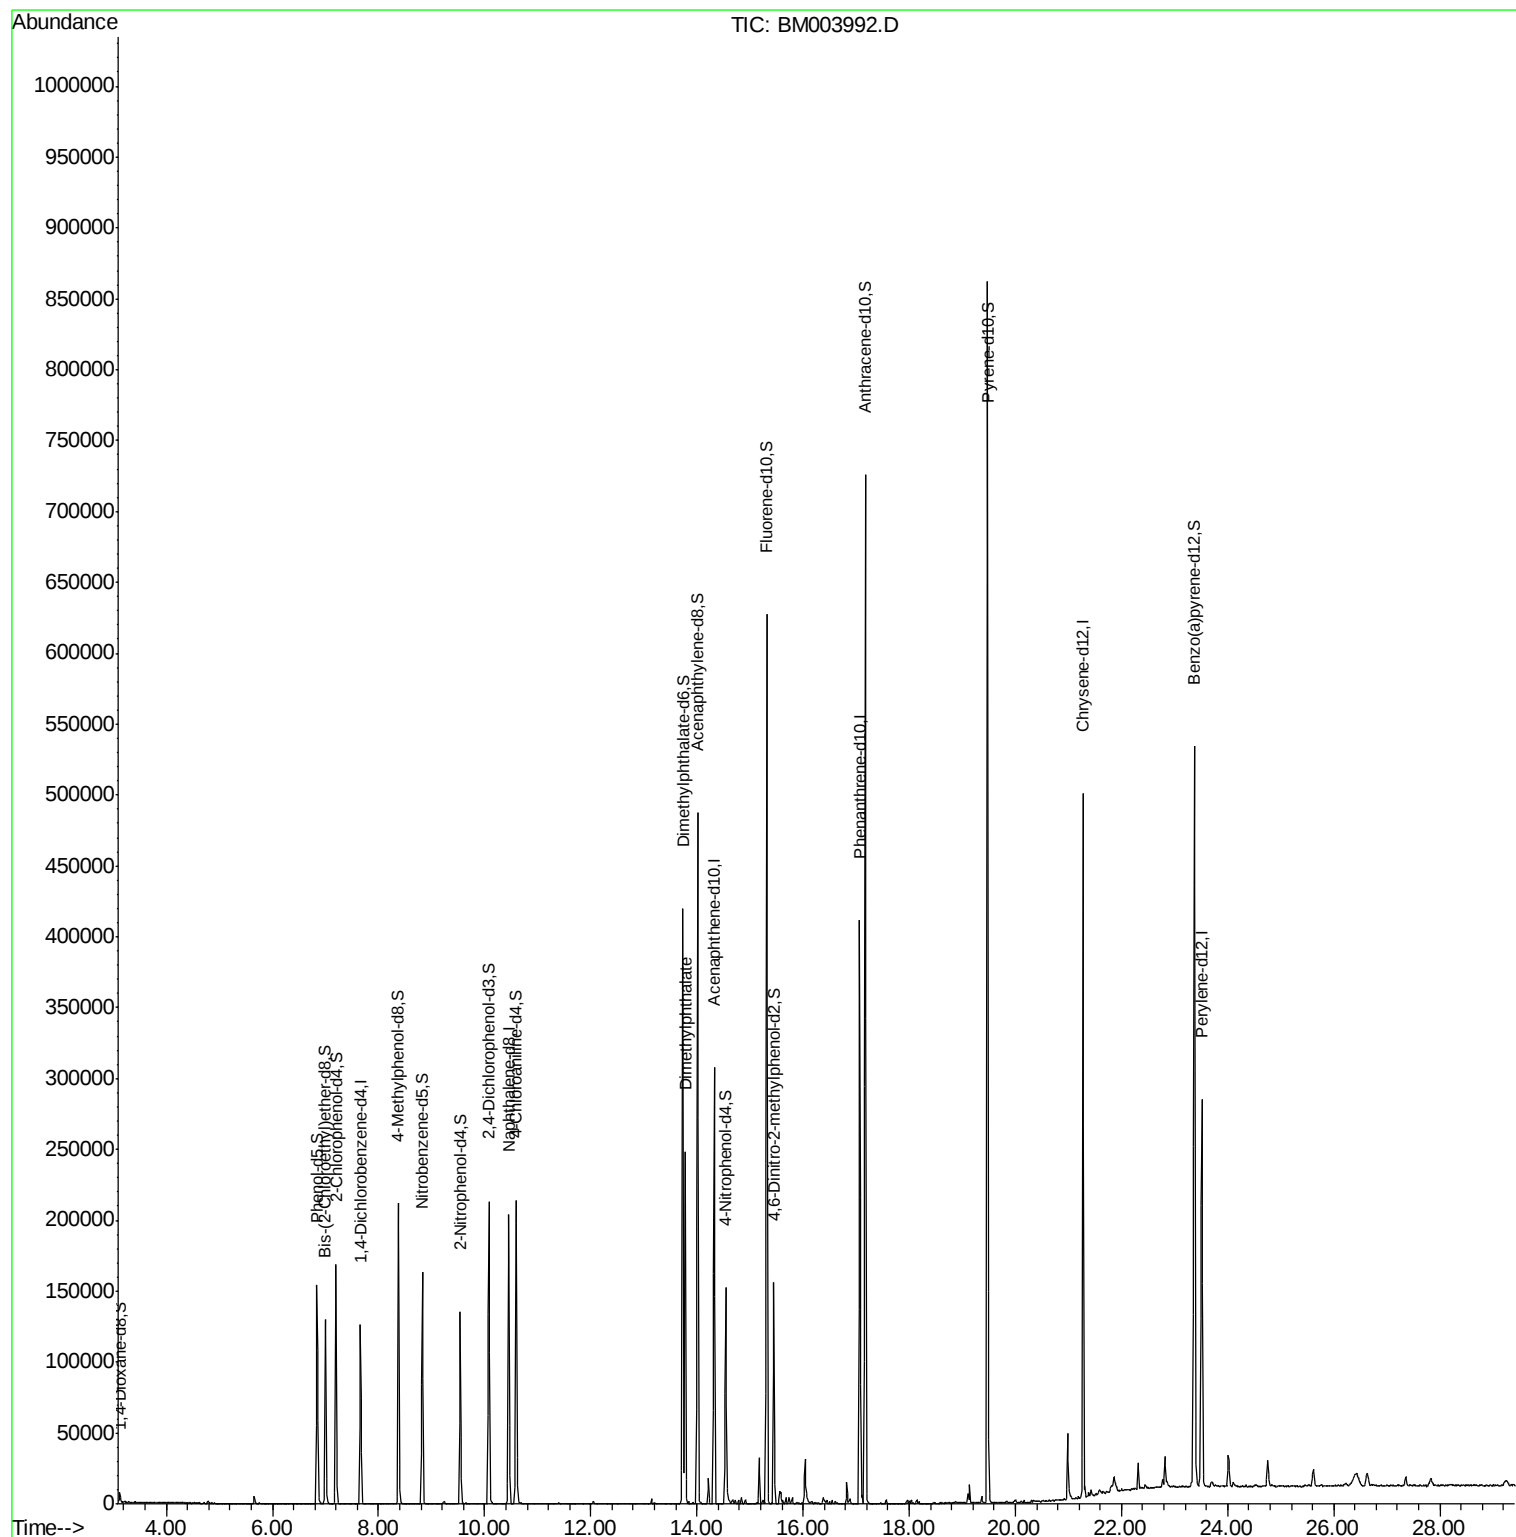

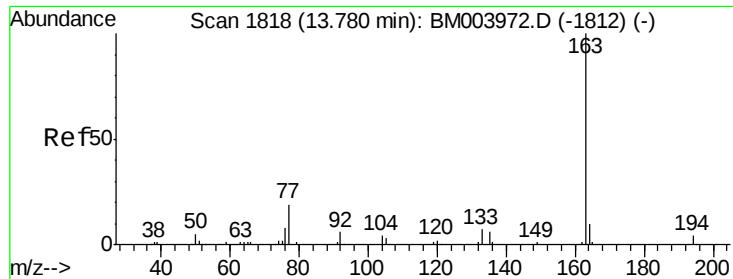

#45

Dimethylphthalate

Concen: 19.84 ng/ul

RT: 13.78 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BM003992.D


Acq: 13 Jan 2016 19:45

Instrument :

BNA_M

ClientSampleId :

BC949

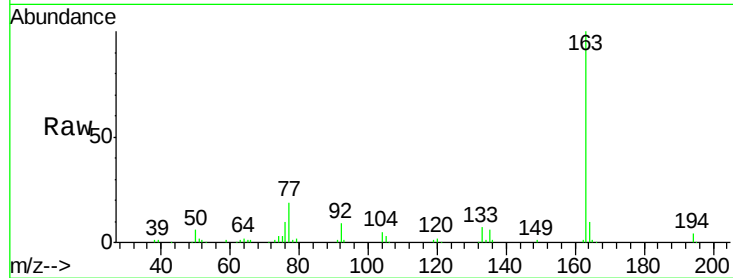

Tgt Ion:163 Resp: 162285

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 9.7 7.8 11.8

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

