

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011416\
 Data File : BM004008.D
 Acq On : 14 Jan 2016 05:50
 Operator : SJ/UM
 Sample : H1098-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC963

Manual Integrations
 APPROVED

MMdadoda
 1/14/2016 5:56:56 PM

Quant Time: Jan 14 12:55:18 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 13 06:45:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	43523	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	211032	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.32	164	123900	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.07	188	272937	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	255493	20.00	ng/ul	0.00
86) Perylene-d12	23.51	264	211666	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	2789	2.87	ng/uL	0.00
5) Phenol-d5	6.84	99	67781	18.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	41699	20.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	58471	19.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	52444	17.91	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	30053	18.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	32656	18.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	56935	18.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	68280	16.71	ng/ul	0.00
44) Dimethylphthalate-d6	13.73	166	193255	19.87	ng/ul	0.00
47) Acenaphthylene-d8	14.01	160	240918	20.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	20898	11.96	ng/ul	0.00
58) Fluorene-d10	15.32	176	173832	21.07	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	18515	12.03	ng/ul	0.00
71) Anthracene-d10	17.17	188	270698	21.44	ng/ul	0.00
79) Pyrene-d10	19.47	212	291723	22.05	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	230832	21.84	ng/ul	0.00

Target Compounds

						Qvalue
45) Dimethylphthalate	13.77	163	110166	11.11	ng/ul	99
70) Phenanthrene	17.11	178	108044	7.04	ng/ul	100
72) Anthracene	17.20	178	20383	1.29	ng/ul	99
77) Fluoranthene	19.14	202	212084	13.30	ng/ul	98
80) Pyrene	19.50	202	303757	17.51	ng/ul	98
83) Benzo(a)anthracene	21.26	228	116097	7.63	ng/ul	97
85) Chrysene	21.32	228	140835	9.74	ng/ul	97
88) Benzo(b)fluoranthene	22.84	252	113269	8.80	ng/ul	98
89) Benzo(k)fluoranthene	22.88	252	34265m	2.80	ng/ul	
91) Benzo(a)pyrene	23.41	252	96444	7.90	ng/ul	99
92) Indeno(1,2,3-cd)pyrene	25.76	276	52472	3.89	ng/ul	95
93) Dibenzo(a,h)anthracene	25.76	278	17829	1.57	ng/ul#	80
94) Benzo(g,h,i)perylene	26.45	276	54938	4.85	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011416\
Data File : BM004008.D
Acq On : 14 Jan 2016 05:50
Operator : SJ/UM
Sample : H1098-12
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleID :
BC963

Manual Integrations
APPROVED

MMdadoda
1/14/2016 5:56:56 PM

Quant Time: Jan 14 12:55:18 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 13 06:45:02 2016
Response via : Initial Calibration

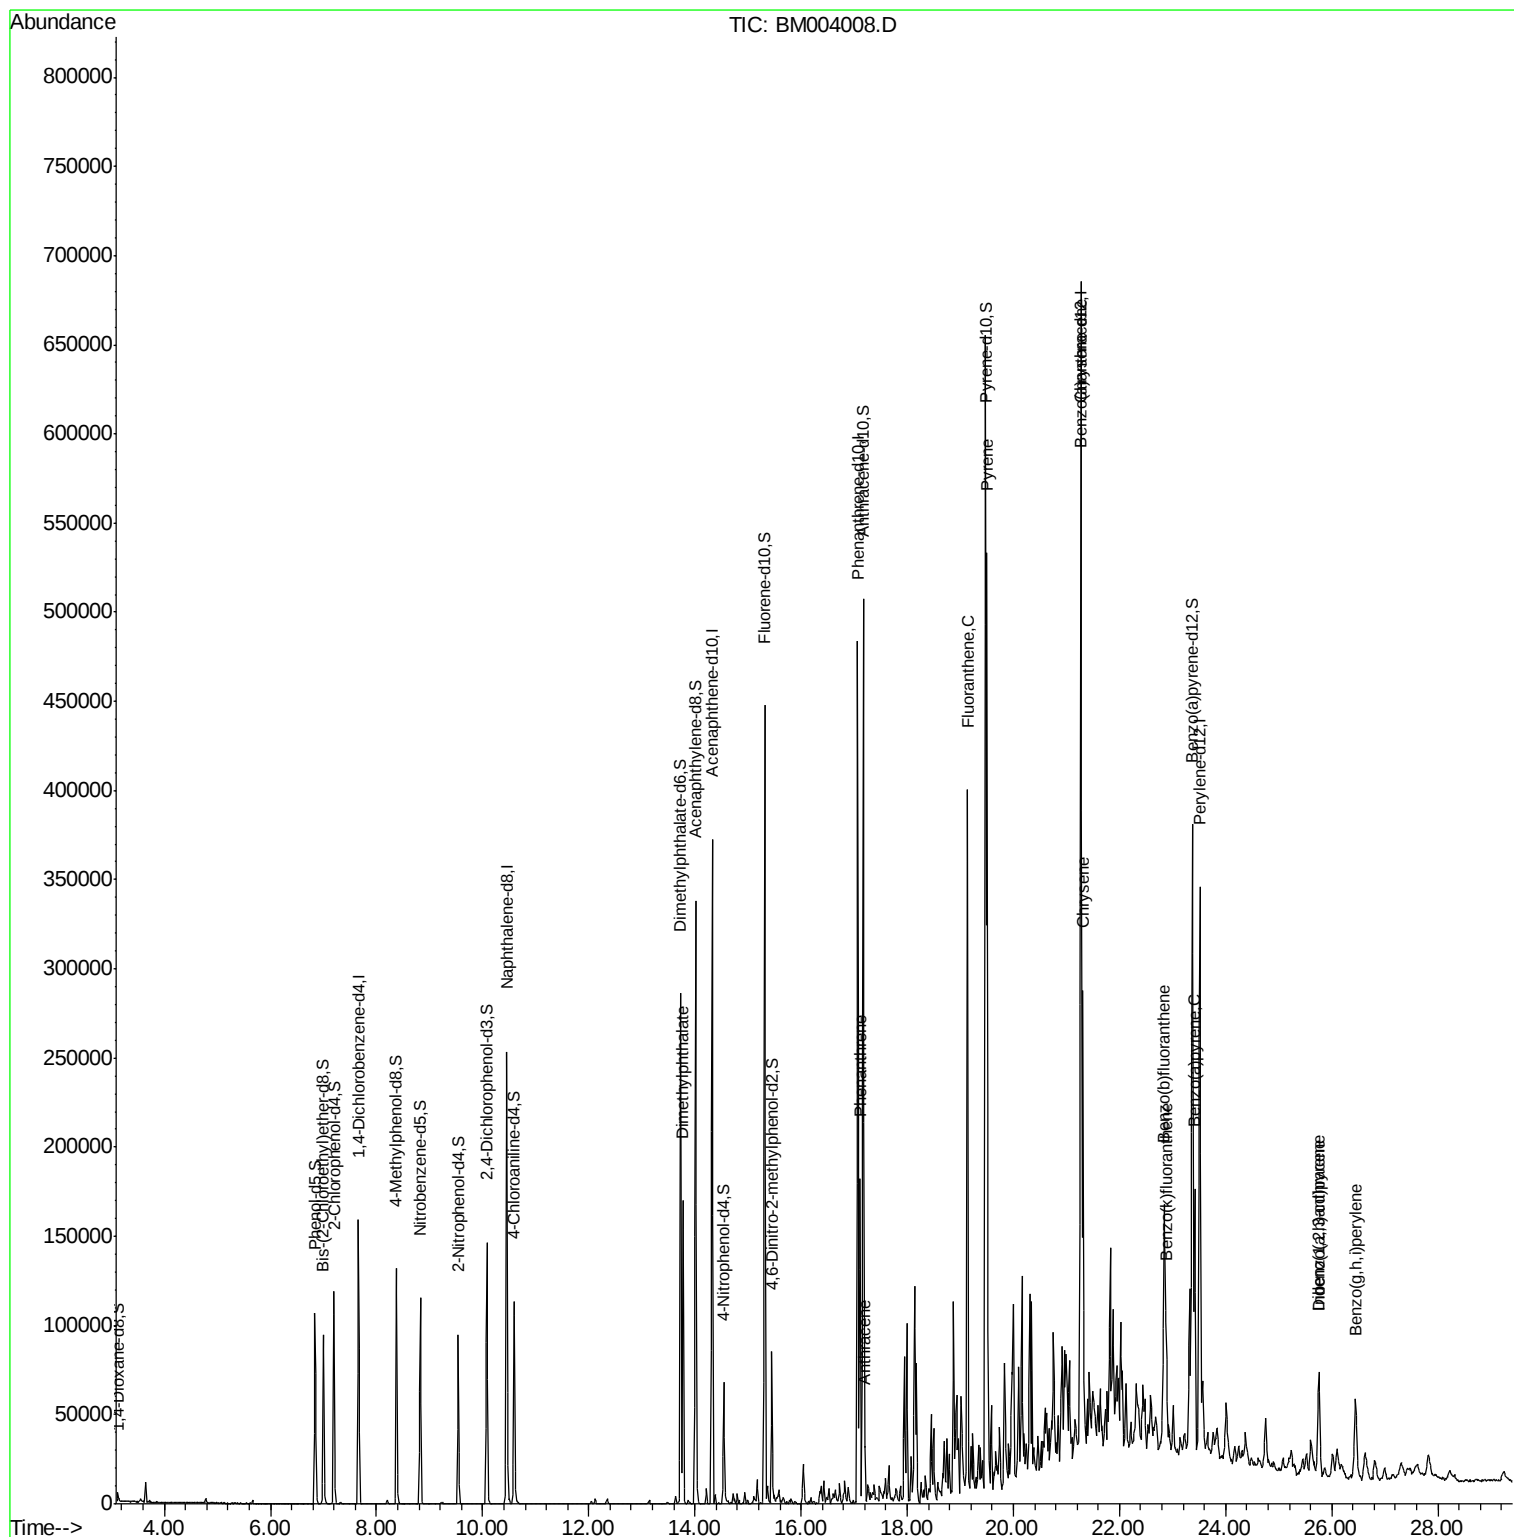

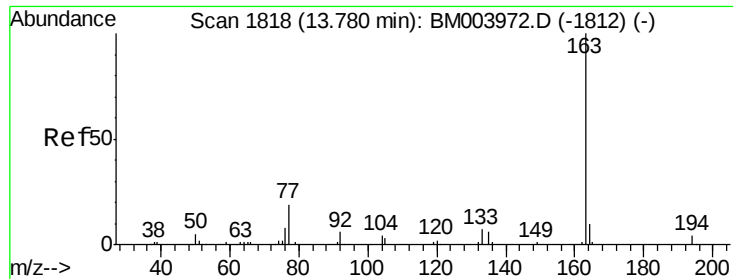





#45
Dimethylphthalate
Concen: 11.11 ng/ul
RT: 13.77 min Scan# 1817
Delta R.T. -0.01 min
Lab File: BM004008.D
Acq: 14 Jan 2016 05:50

Instrument :
BNA_M
ClientSampleId :
BC963

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	110166		
194	3.8		3.2	4.8
164	10.4		7.8	11.8




Manual Integrations
APPROVED


MMdadoda
1/14/2016 5:56:56 PM

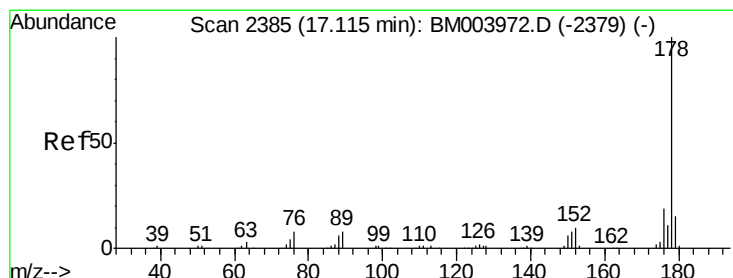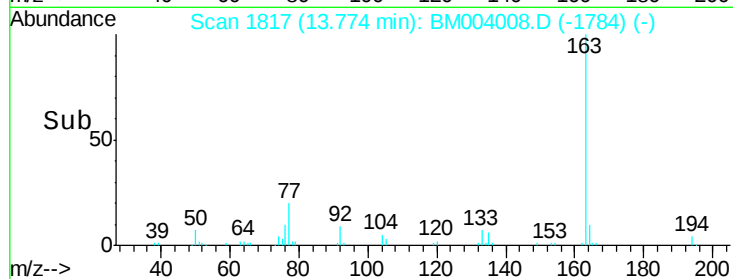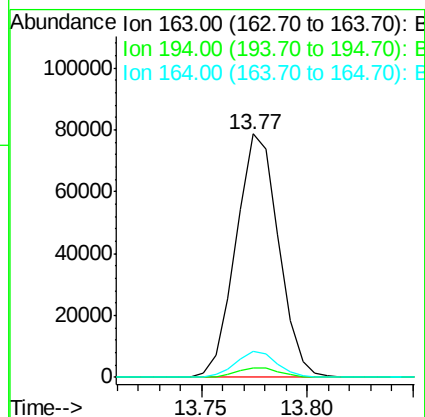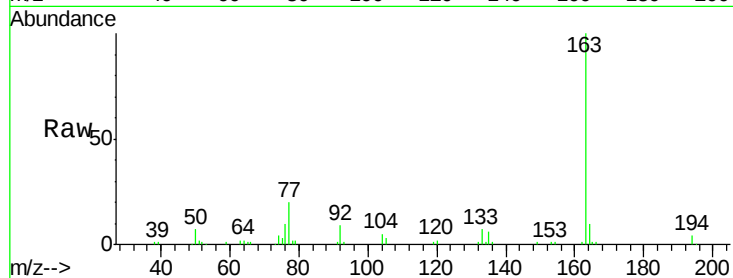

#70
Phenanthrene
Concen: 7.04 ng/ul
RT: 17.11 min Scan# 2384
Delta R.T. -0.01 min
Lab File: BM004008.D
Acq: 14 Jan 2016 05:50

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	108044		
179	15.2		12.2	18.4
176	19.2		15.6	23.4

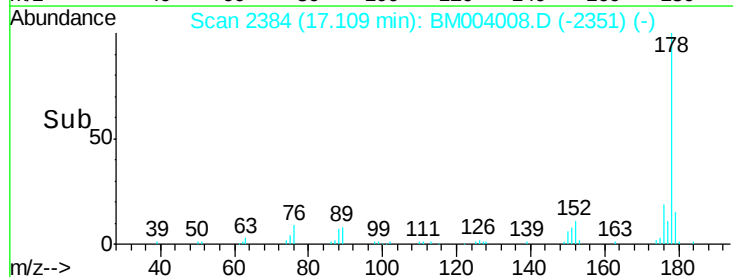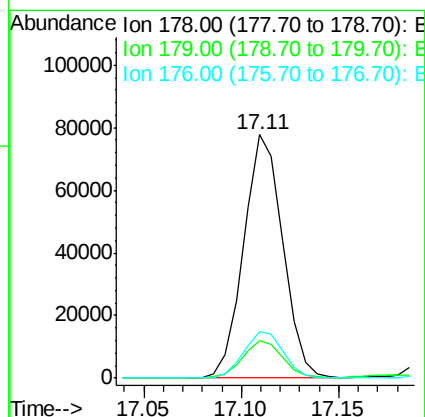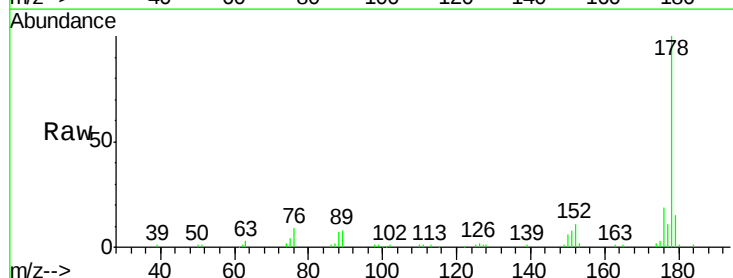

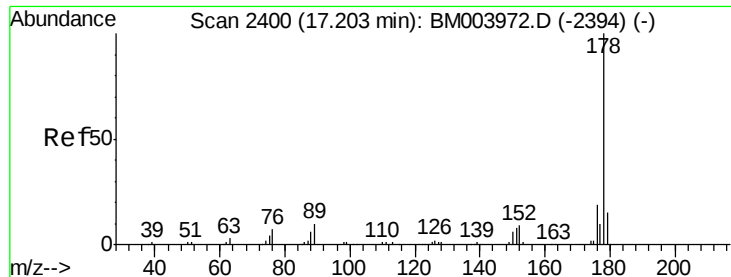

#72

Anthracene

Concen: 1.29 ng/ul

RT: 17.20 min Scan# 2400

Delta R.T. 0.00 min

Lab File: BM004008.D

Acq: 14 Jan 2016 05:50

Instrument :

BNA_M


ClientSampleId :

BC963




Tgt Ion:	178	Resp:	20383
Ion Ratio	Lower	Upper	
178	100		
179	14.7	12.1	18.1
176	18.8	14.8	22.2

Manual Integrations
APPROVED

MMdadoda
1/14/2016 5:56:56 PM

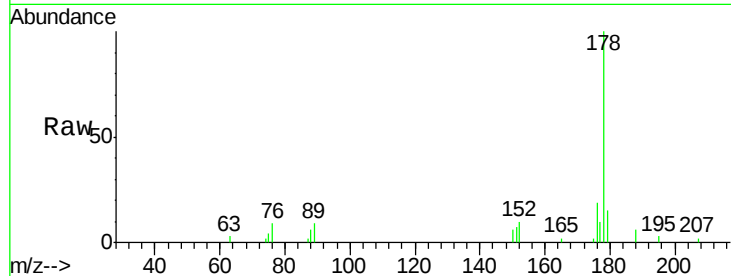

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

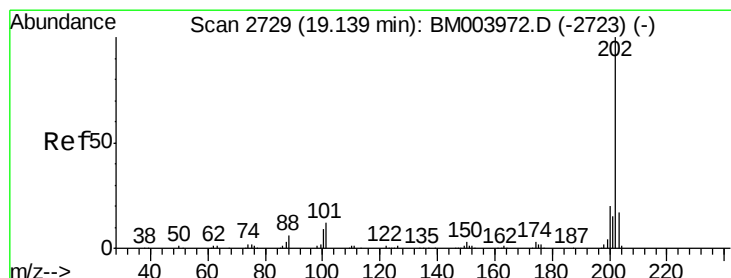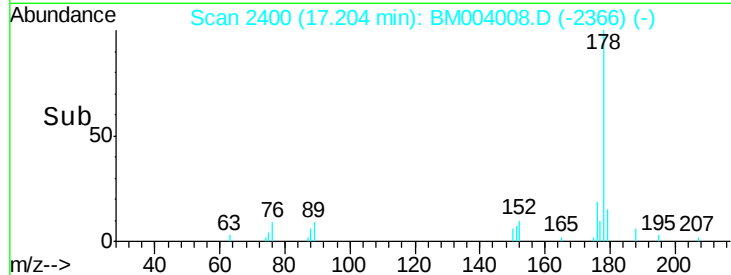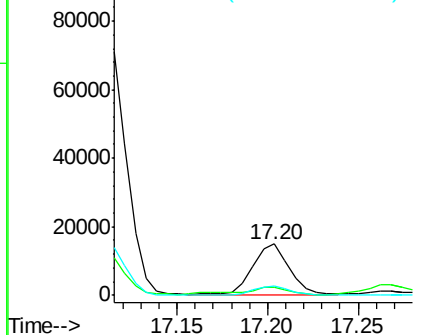

#77

Fluoranthene

Concen: 13.30 ng/ul

RT: 19.14 min Scan# 2729




Delta R.T. 0.00 min


Lab File: BM004008.D

Acq: 14 Jan 2016 05:50

Tgt Ion:	202	Resp:	212084
Ion Ratio	Lower	Upper	
202	100		
101	11.6	8.8	13.2
100	8.7	6.6	9.8

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

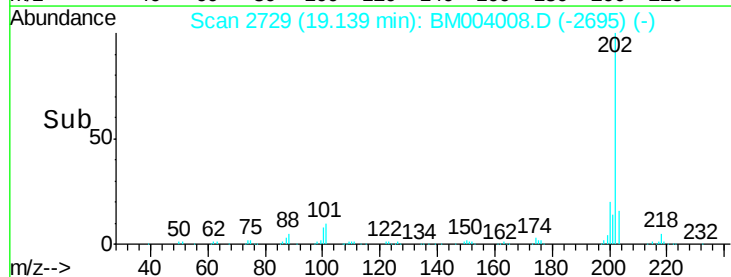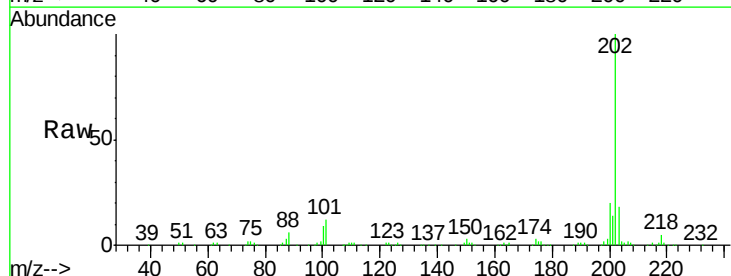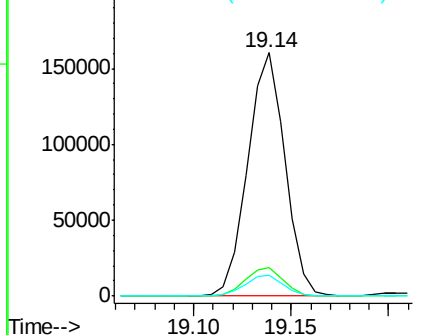

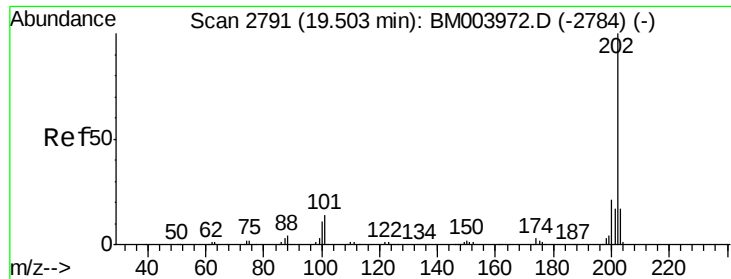





#80
Pyrene
Concen: 17.51 ng/ul
RT: 19.50 min Scan# 2791
Delta R.T. 0.00 min
Lab File: BM004008.D
Acq: 14 Jan 2016 05:50

Instrument :
BNA_M
ClientSampleId :
BC963

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	13.7	10.2	15.2
100	11.1	8.5	12.7




Manual Integrations
APPROVED


MMdadoda
1/14/2016 5:56:56 PM

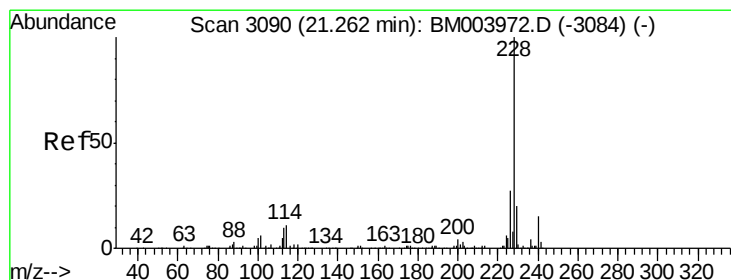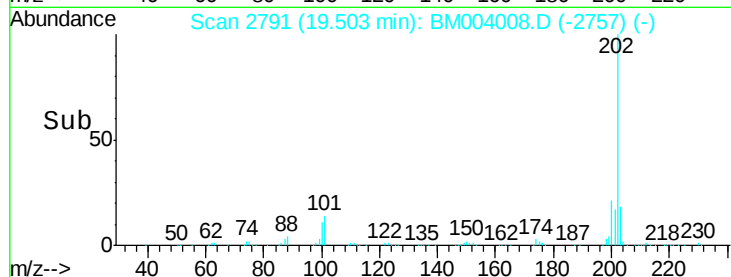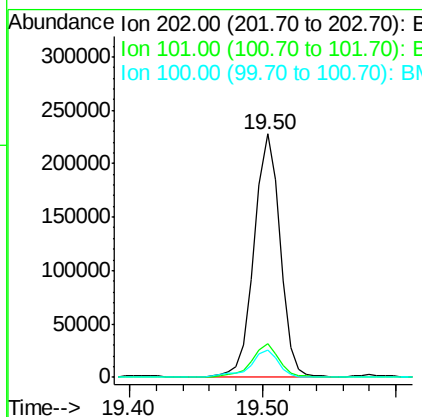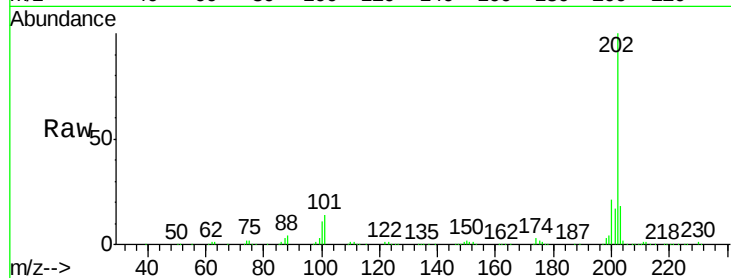

#83
Benzo(a)anthracene
Concen: 7.63 ng/ul
RT: 21.26 min Scan# 3090
Delta R.T. 0.00 min
Lab File: BM004008.D
Acq: 14 Jan 2016 05:50

Tgt Ion	Ratio	Resp Lower	Resp Upper
228	100		
229	21.8	15.7	23.5
226	28.3	21.8	32.6

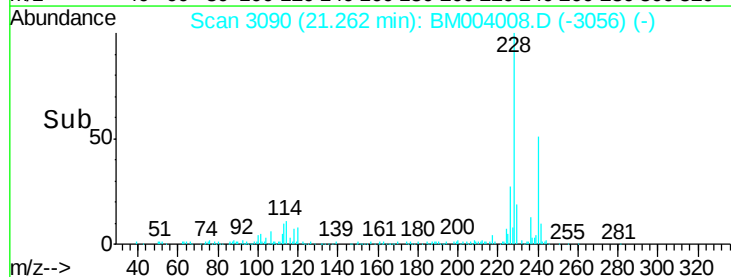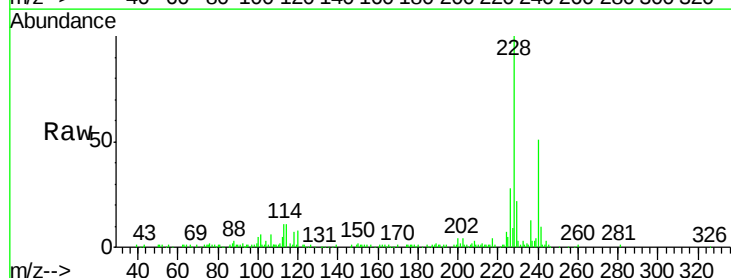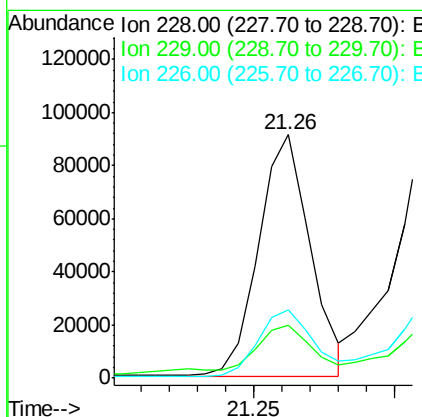

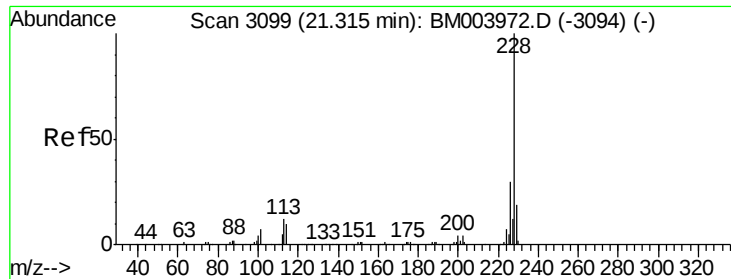

#85

Chrysene

Concen: 9.74 ng/ul

RT: 21.32 min Scan# 3099

Delta R.T. 0.00 min

Lab File: BM004008.D


Acq: 14 Jan 2016 05:50

Instrument :

BNA_M

ClientSampleId :




BC963

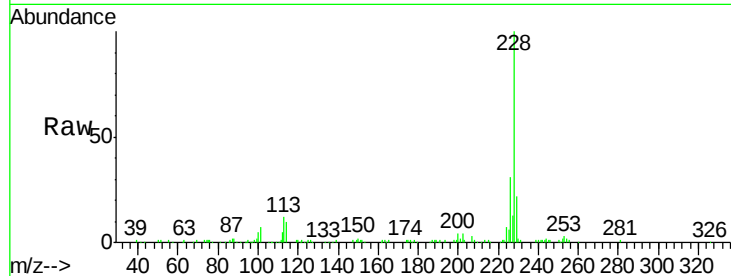

Tgt Ion:	228	Resp:	140835
Ion Ratio	Lower	Upper	
228	100		
226	30.6	24.0	36.0
229	21.9	15.6	23.4

Manual Integrations
APPROVED

MMdadoda
1/14/2016 5:56:56 PM

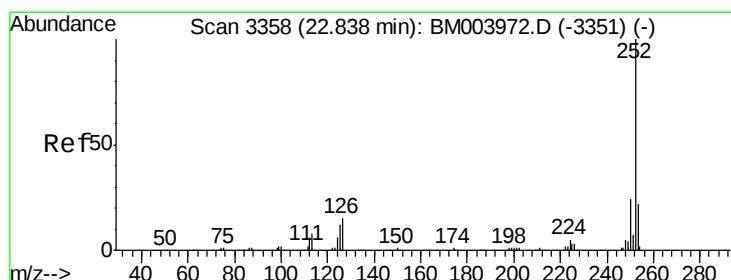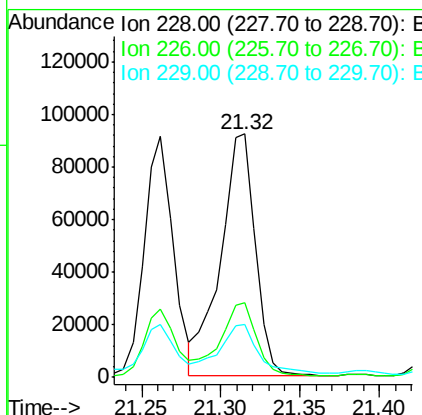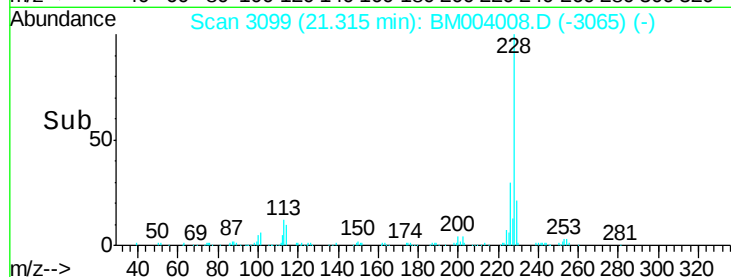

#88

Benzo(b)fluoranthene

Concen: 8.80 ng/ul




RT: 22.84 min Scan# 3359


Delta R.T. 0.01 min

Lab File: BM004008.D

Acq: 14 Jan 2016 05:50

Tgt Ion:	252	Resp:	113269
Ion Ratio	Lower	Upper	
252	100		
253	22.5	17.5	26.3
125	12.4	8.5	12.7

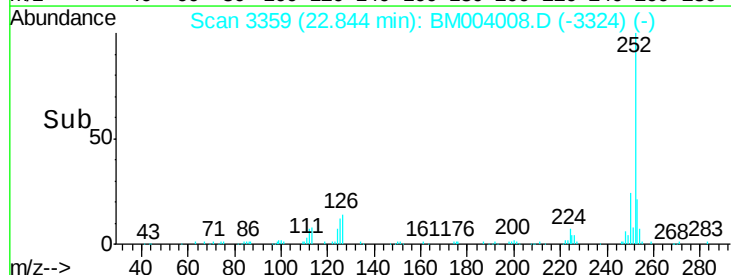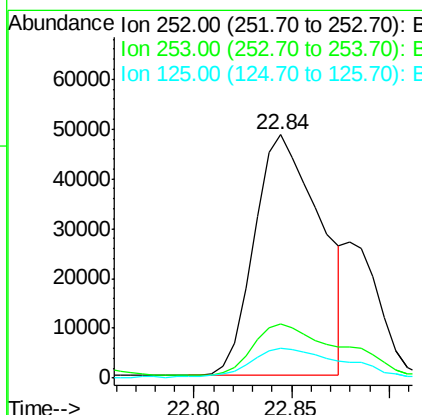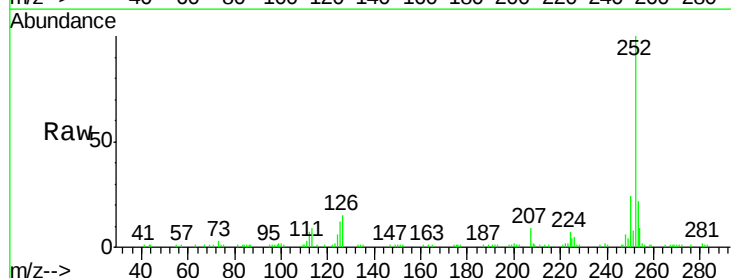

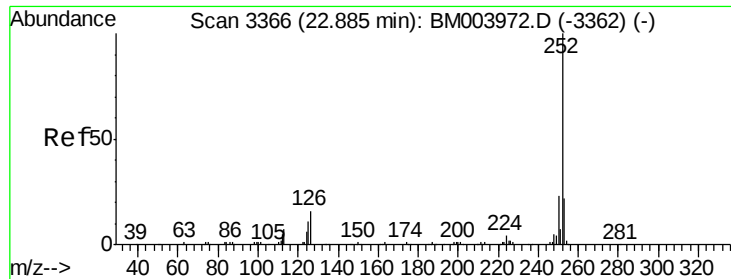

#89

Benzo(k)fluoranthene

Concen: 2.80 ng/ul m

RT: 22.88 min Scan# 3365

Delta R.T. -0.01 min

Lab File: BM004008.D


Acq: 14 Jan 2016 05:50

Instrument :

BNA_M

ClientSampled :




BC963

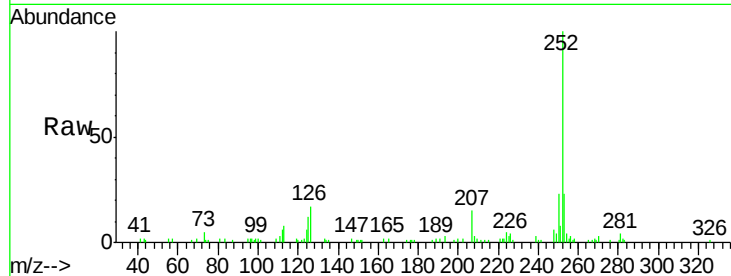

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.3	25.9
125	11.7	8.2	12.2

Manual Integrations
APPROVED

MMdadoda
1/14/2016 5:56:56 PM

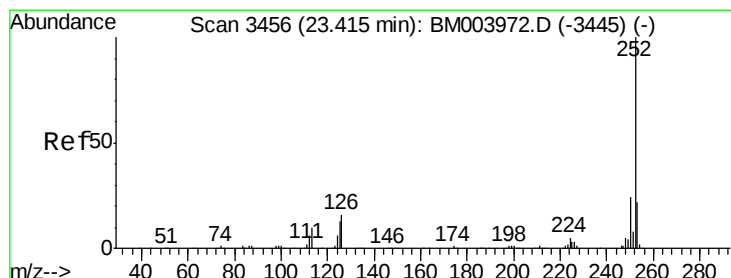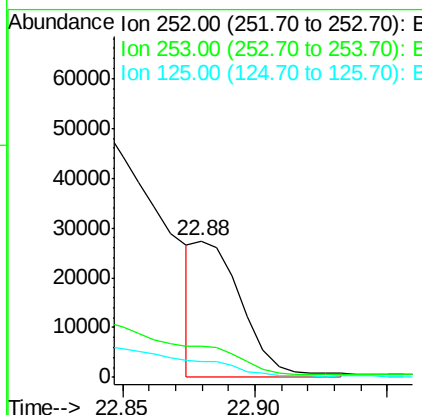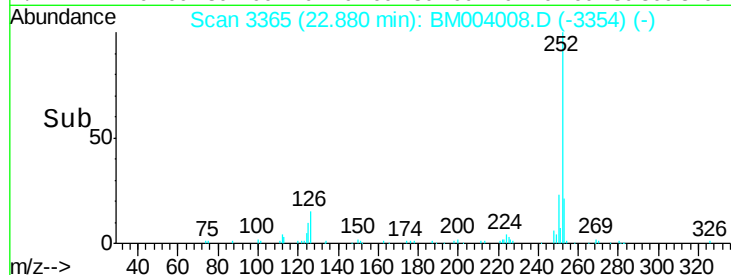

#91

Benzo(a)pyrene

Concen: 7.90 ng/ul




RT: 23.41 min Scan# 3456


Delta R.T. 0.00 min

Lab File: BM004008.D

Acq: 14 Jan 2016 05:50

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.6	17.2	25.8
125	11.9	9.0	13.6

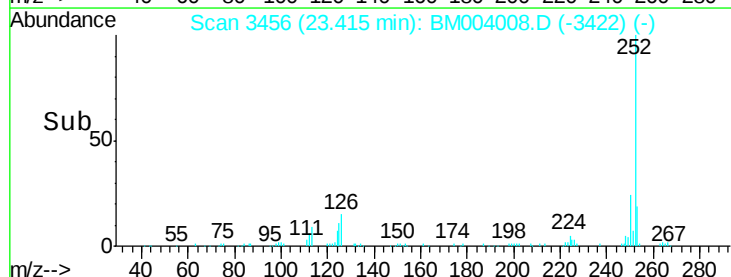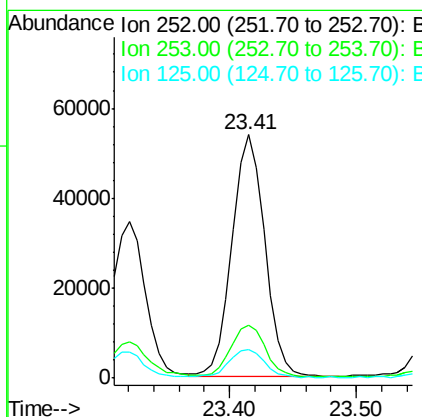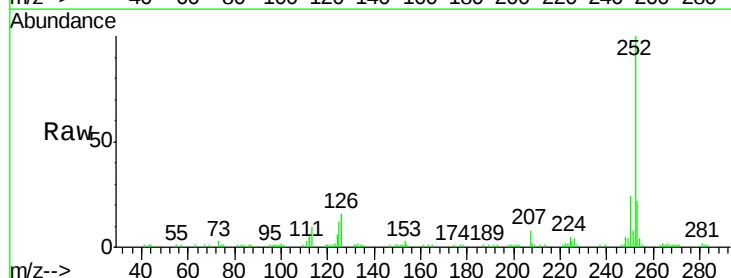

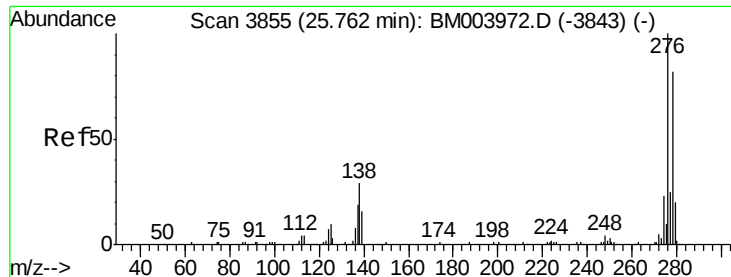





#92
 Indeno(1,2,3-cd)pyrene
 Concen: 3.89 ng/ul
 RT: 25.76 min Scan# 3854
 Delta R.T. -0.01 min
 Lab File: BM004008.D
 Acq: 14 Jan 2016 05:50

Instrument :
 BNA_M
 ClientSampleId :
 BC963

Tgt Ion	Ratio	Lower	Upper
276	100		
138	24.5	22.3	33.5
277	23.0	20.2	30.2




Manual Integrations
 APPROVED


MMdadoda
 1/14/2016 5:56:56 PM

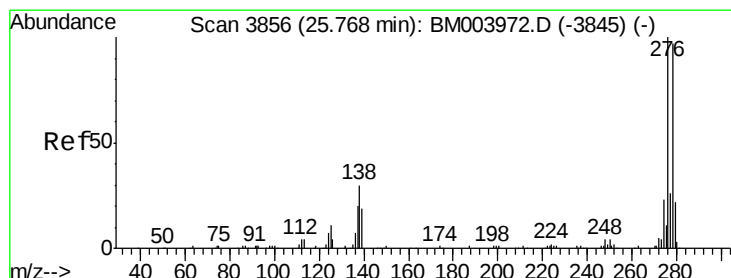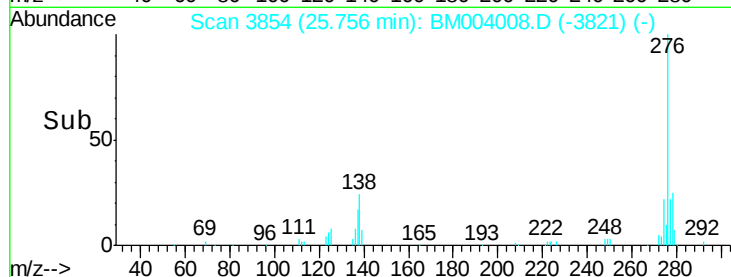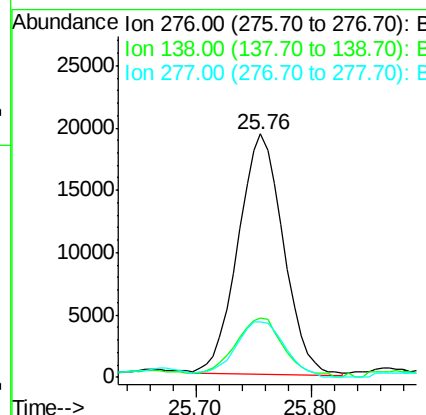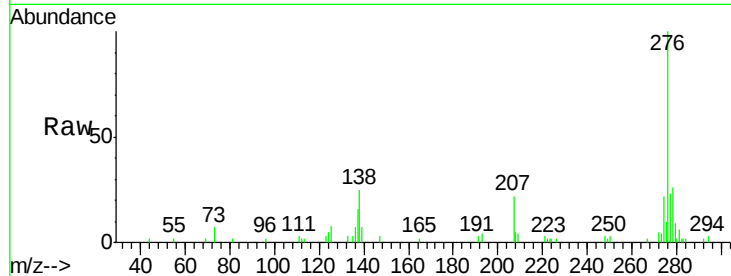

#93
 Dibenzo(a,h)anthracene
 Concen: 1.57 ng/ul
 RT: 25.76 min Scan# 3854
 Delta R.T. -0.01 min
 Lab File: BM004008.D
 Acq: 14 Jan 2016 05:50

Tgt Ion	Ratio	Lower	Upper
278	100		
139	26.4	13.9	20.9#
279	33.4	19.0	28.4#

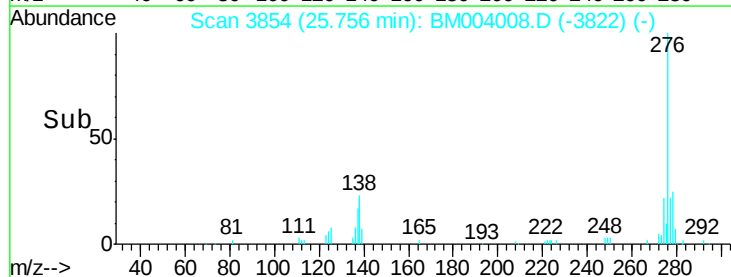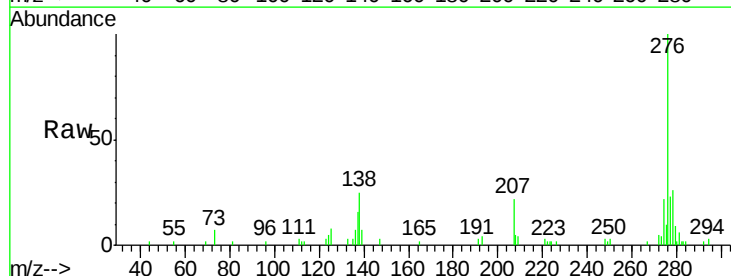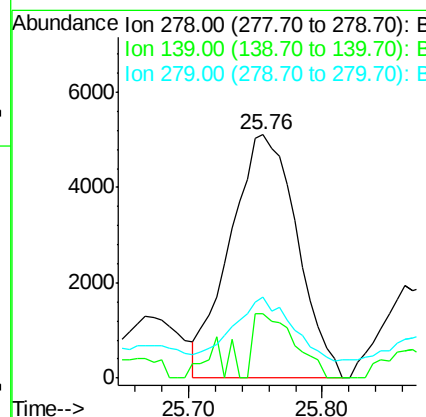

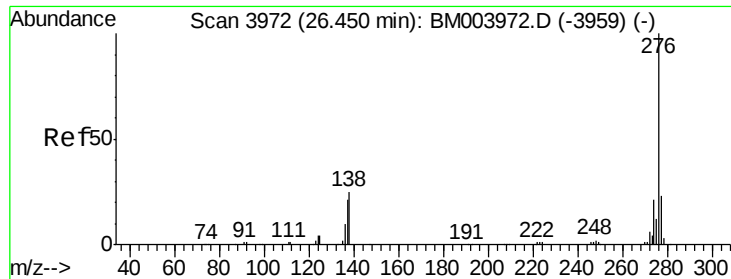

#94
 Benzo(g,h,i)perylene
 Concen: 4.85 ng/ul
 RT: 26.45 min Scan# 3972
 Delta R.T. 0.00 min
 Lab File: BM004008.D
 Acq: 14 Jan 2016 05:50

Instrument :
 BNA_M
 ClientSampleId :
 BC963

Tgt Ion:	276	Resp:	54938
Ion Ratio	Lower	Upper	
276	100		
138	25.1	18.9	28.3
277	24.8	19.2	28.8

Manual Integrations
 APPROVED

MMdadoda
 1/14/2016 5:56:56 PM

