


Data Path : Z:\HPCHEM1\BNA_M\Data\BM011416\
Data File : BM003988.D
Acq On : 13 Jan 2016 15:55
Operator : SJ/UM
Sample : DFTPP37
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP37

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Title : SVOA CALIBRATION
Last Update : Wed Jan 13 06:45:02 2016

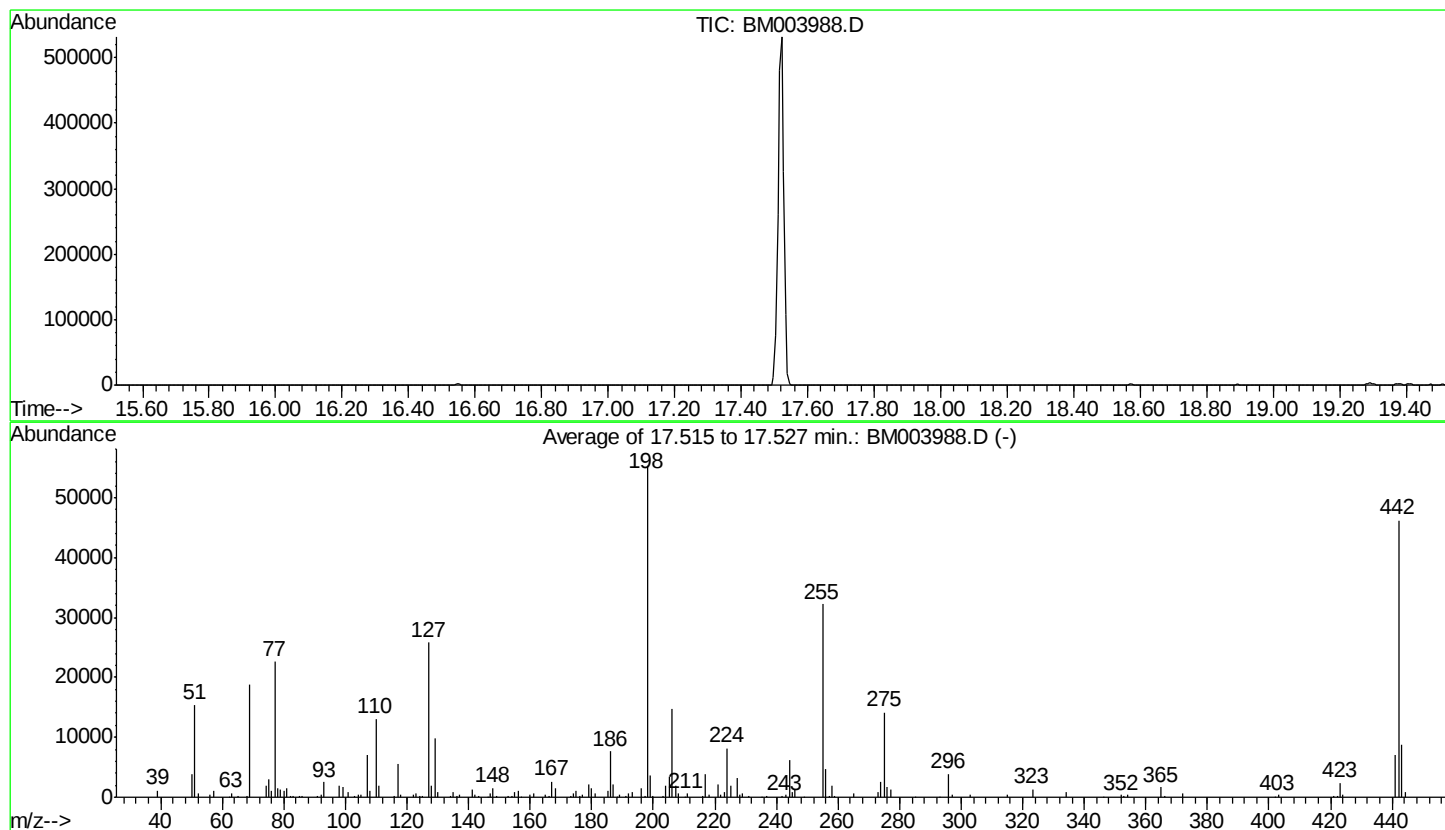

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	15396	PASS
68	69	0.00	2	1.3	235	PASS
69	198	0.00	100	33.8	18713	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	25752	PASS
197	198	0.00	2	0.4	242	PASS
198	198	100	100	100.0	55317	PASS
199	198	5	9	6.8	3743	PASS
275	198	10	60	25.7	14191	PASS
365	198	1	100	3.0	1679	PASS
441	443	0.01	100	79.8	7023	PASS
442	198	50	100	83.4	46128	PASS
443	442	15	24	19.1	8804	PASS

m/z	Abundance
39.10	1319.0
50.10	4714.0
51.10	18696.0
52.00	923.0
56.00	532.0
57.00	1309.0
63.00	807.0
65.10	436.0
68.00	358.0
69.00	22712.0
74.10	2334.0
75.00	3580.0
76.00	1281.0
77.10	26688.0
78.10	1861.0
79.00	1691.0
80.00	1280.0
81.00	1863.0
82.10	452.0
83.00	443.0
85.00	366.0
86.00	502.0
91.10	426.0
92.00	444.0
93.00	2909.0
98.00	2136.0
99.00	1921.0
101.00	1029.0
103.00	366.0
104.00	609.0
105.00	647.0
107.10	8371.0
108.00	1307.0
110.00	15258.0
111.00	2310.0
116.00	458.0
117.00	6472.0
118.00	478.0
122.00	475.0
123.00	852.0
124.00	363.0
125.00	357.0
127.10	29888.0
128.00	2131.0
129.00	11036.0
130.00	1006.0
134.00	367.0
135.00	1033.0
136.00	339.0
137.10	481.0
141.00	1523.0
142.00	516.0
143.00	318.0
147.00	769.0
148.00	1676.0
149.00	426.0
153.00	449.0
153.90	336.0
155.10	870.0
156.00	1249.0
160.00	510.0
161.00	759.0
165.00	506.0
166.00	441.0
167.00	2810.0
168.00	1705.0
174.00	651.0
175.00	1224.0
176.00	337.0
177.00	550.0
179.00	2232.0
180.00	1595.0
181.00	733.0
185.00	1035.0
186.10	8315.0
187.00	2413.0
188.00	302.0
189.00	556.0
192.00	794.0
193.00	893.0
196.10	1794.0
197.10	357.0
198.00	60104.0
199.00	4180.0
200.00	394.0
203.00	453.0
204.00	2255.0
205.10	3529.0
206.10	15661.0
207.10	2370.0
208.00	625.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37

211.00	555.0
217.00	4063.0
218.00	570.0
221.00	2247.0
221.80	586.0
223.00	949.0
224.10	8637.0
225.10	2180.0
227.10	3385.0
228.00	490.0
229.00	824.0
231.00	305.0
237.00	323.0
242.00	410.0
243.00	450.0
244.10	6379.0
245.10	886.0
246.10	1256.0
255.10	33552.0
256.10	4897.0
257.00	377.0
258.00	1936.0
259.00	322.0
265.10	705.0
273.10	947.0
274.00	2545.0
275.10	14339.0
276.00	1846.0
277.00	1249.0
296.00	3881.0
297.00	545.0
303.10	425.0
315.00	395.0
323.10	1265.0
334.00	695.0
352.10	353.0
354.10	516.0
365.10	1569.0
372.10	562.0
403.00	376.0
421.10	309.0
423.10	2076.0
424.10	562.0
441.10	6074.0
442.10	39592.0
443.10	7754.0
444.10	812.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37

m/z	Abundance
39.10	1321.0
50.10	4405.0
51.10	17848.0
52.10	832.0
56.00	516.0
57.00	1249.0
62.00	301.0
63.00	808.0
65.00	433.0
68.10	348.0
69.00	21584.0
74.10	2184.0
75.00	3587.0
76.10	1226.0
77.10	26584.0
78.10	1606.0
79.00	1598.0
80.00	1243.0
81.00	1836.0
82.00	485.0
83.00	477.0
85.00	488.0
86.00	456.0
91.00	443.0
92.00	456.0
93.00	2945.0
98.00	2294.0
99.00	1846.0
101.00	1107.0
103.00	373.0
104.00	659.0
105.00	646.0
107.00	8257.0
108.00	1326.0
110.00	15249.0
111.00	2269.0
116.00	470.0
117.00	6642.0
118.00	570.0
122.00	525.0
123.00	865.0
124.00	400.0
125.00	375.0
127.10	30064.0
128.00	2242.0
129.00	11505.0
130.00	944.0
134.00	330.0
135.00	950.0
136.00	368.0
137.00	559.0
141.00	1541.0
142.00	450.0
143.10	340.0
146.00	324.0
147.00	886.0
148.00	1794.0
149.00	448.0
153.00	476.0
154.00	378.0
155.00	900.0
156.00	1412.0
157.00	311.0
160.00	514.0
161.00	798.0
165.00	667.0
166.00	461.0
167.00	3278.0
168.00	1728.0
173.00	378.0
174.10	629.0
175.10	1175.0
176.00	412.0
177.00	575.0
179.00	2472.0
180.00	1675.0
181.00	763.0
185.10	1222.0
186.10	9288.0
187.10	2525.0
189.00	572.0
191.10	370.0
192.10	800.0
193.00	903.0
196.00	1703.0
197.10	371.0
198.00	64992.0
199.00	4434.0
203.00	409.0
204.00	2413.0
205.10	4022.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37

206.10	17528.0
207.10	2539.0
208.00	718.0
210.10	307.0
211.00	679.0
216.00	354.0
217.00	4503.0
218.00	557.0
221.10	2704.0
223.00	1087.0
224.10	9731.0
225.10	2367.0
227.00	3839.0
228.00	567.0
229.00	823.0
231.00	383.0
235.00	302.0
237.00	394.0
242.00	484.0
243.10	482.0
244.10	7569.0
245.10	927.0
246.10	1407.0
249.00	329.0
255.10	38408.0
256.00	5525.0
257.00	397.0
258.00	2224.0
259.00	328.0
265.00	916.0
273.10	1097.0
274.00	2952.0
275.10	16696.0
276.10	2101.0
277.00	1516.0
285.00	320.0
293.00	336.0
296.10	4759.0
297.00	637.0
303.00	476.0
315.00	487.0
323.10	1565.0
334.10	1000.0
346.00	330.0
352.10	464.0
353.00	347.0
354.10	514.0
365.00	2050.0
366.00	343.0
372.10	768.0
402.00	320.0
403.10	493.0
421.10	327.0
422.10	380.0
423.10	2750.0
424.10	608.0
441.10	8278.0
442.10	54936.0
443.20	10562.0
444.10	1040.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37

m/z	Abundance
39.00	708.0
50.10	2436.0
51.10	9646.0
52.00	490.0
57.00	678.0
63.00	456.0
69.00	11844.0
74.10	1237.0
75.00	2037.0
76.00	688.0
77.10	14352.0
78.10	996.0
79.00	872.0
80.00	670.0
81.00	980.0
92.00	303.0
93.00	1666.0
98.00	1251.0
99.00	1084.0
101.00	559.0
104.00	347.0
105.00	314.0
107.00	4633.0
108.00	658.0
110.00	8774.0
111.00	1349.0
117.00	3600.0
118.00	303.0
121.90	303.0
123.00	450.0
127.10	17304.0
128.10	1217.0
129.00	6651.0
130.00	601.0
135.00	541.0
141.00	850.0
141.90	309.0
147.00	478.0
148.00	1164.0
155.00	513.0
156.00	821.0
161.00	445.0
165.00	368.0
167.00	1815.0
168.00	1149.0
174.00	436.0
175.00	736.0
177.00	359.0
179.00	1439.0
180.00	1073.0
181.00	496.0
185.00	755.0
186.10	5437.0
187.00	1631.0
189.00	406.0
192.00	575.0
193.00	603.0
196.00	1116.0
198.00	40856.0
199.00	2615.0
204.00	1402.0
205.10	2452.0
206.10	11112.0
207.10	1706.0
208.00	423.0
211.00	407.0
217.00	2857.0
218.00	375.0
221.10	1703.0
221.80	442.0
223.00	756.0
224.10	6189.0
225.00	1464.0
227.00	2551.0
228.00	424.0
229.00	518.0
243.10	344.0
244.10	4886.0
245.10	586.0
246.00	982.0
255.10	24768.0
256.10	3661.0
258.00	1486.0
265.00	620.0
273.10	776.0
274.00	2046.0
275.10	11538.0
276.10	1400.0
277.00	1026.0
296.10	3092.0
297.00	392.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37

303.10	397.0
315.00	348.0
323.10	1148.0
334.10	694.0
352.10	309.0
354.10	348.0
365.10	1418.0
372.10	574.0
403.10	329.0
422.00	307.0
423.10	2288.0
424.10	442.0
441.10	6719.0
442.10	43856.0
443.10	8096.0
444.10	725.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37

m/z	Abundance
207.10	359.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37