

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011421\
 Data File : BM028390.D
 Acq On : 14 Jan 2021 17:30
 Operator : CG/JU
 Sample : PB134123BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010821MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	26	29	37	rVB	10588	14689	1.51%	0.152%
2	4.157	162	165	170	rBV2	1304	1619	0.17%	0.017%
3	7.263	687	693	701	rBV	200379	307681	31.53%	3.185%
4	7.440	716	723	730	rBV	143493	221113	22.66%	2.289%
5	7.640	751	757	766	rVB	198073	316513	32.43%	3.276%
6	8.122	832	839	846	rVB	119054	184378	18.89%	1.908%
7	8.828	951	959	967	rBB	238195	370136	37.92%	3.831%
8	9.298	1032	1039	1047	rBB	185784	306167	31.37%	3.169%
9	10.022	1155	1162	1170	rBB	160386	253017	25.92%	2.619%
10	10.557	1246	1253	1261	rBB	235470	377146	38.64%	3.904%
11	10.945	1312	1319	1326	rBB	158396	263906	27.04%	2.732%
12	11.075	1334	1341	1350	rBB	246985	397821	40.76%	4.118%
13	12.522	1583	1587	1590	rVB	2744	3830	0.39%	0.040%
14	14.157	1859	1865	1871	rBV	428282	547596	56.11%	5.668%
15	14.451	1908	1915	1924	rBV	482233	659857	67.61%	6.830%
16	14.751	1960	1966	1973	rBV	234790	339296	34.76%	3.512%
17	14.927	1990	1996	2009	rBV	202409	289524	29.67%	2.997%
18	15.739	2127	2134	2141	rVB	571936	784575	80.39%	8.121%
19	15.851	2147	2153	2160	rBV	203104	266361	27.29%	2.757%
20	15.974	2170	2174	2178	rVB	4200	5054	0.52%	0.052%
21	16.510	2262	2265	2269	rBV2	1327	1493	0.15%	0.015%
22	17.474	2423	2429	2436	rVB	285085	387429	39.70%	4.010%
23	17.574	2440	2446	2459	rVB	631308	862137	88.34%	8.923%
24	19.474	2765	2769	2775	rVB	5478	6683	0.68%	0.069%
25	19.727	2809	2812	2816	rVB	4136	5075	0.52%	0.053%
26	19.839	2825	2831	2839	rBV	768049	975972	100.00%	10.102%
27	21.592	3124	3129	3135	rBV	324512	399540	40.94%	4.135%
28	23.774	3493	3500	3509	rVB	431154	780952	80.02%	8.083%
29	23.921	3518	3525	3535	rBV2	176773	331946	34.01%	3.436%


Sum of corrected areas: 9661506

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011421\
Data File : BM028390.D
Acq On : 14 Jan 2021 17:30
Operator : CG/JU
Sample : PB134123BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK23

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

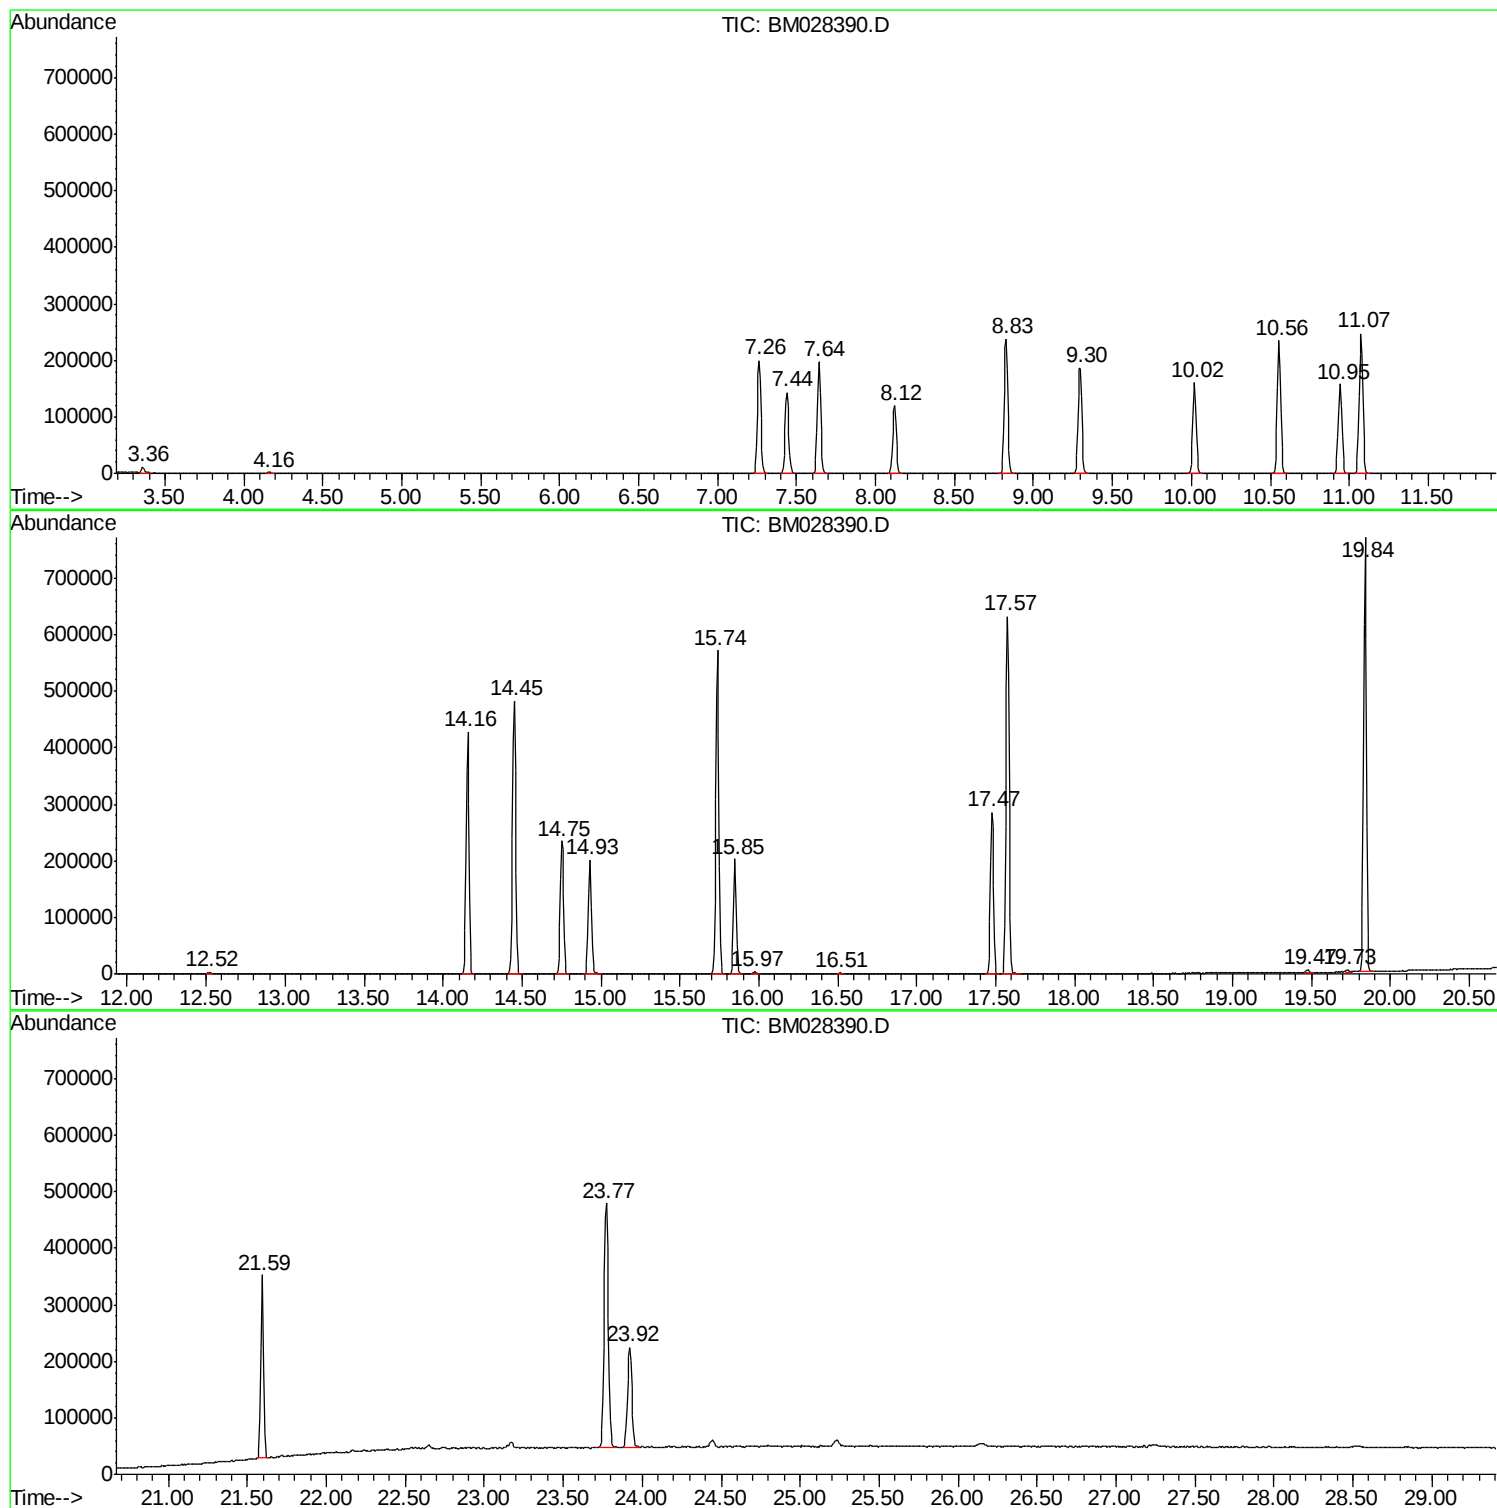

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM011421\
Data File : BM028390.D
Acq On : 14 Jan 2021 17:30
Operator : CG/JU
Sample : PB134123BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK23

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM011421\
Data File : BM028390.D
Acq On : 14 Jan 2021 17:30
Operator : CG/JU
Sample : PB134123BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK23

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc