


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM011421\
 Data File : BM028388.D
 Acq On : 14 Jan 2021 10:14
 Operator : CG/JU
 Sample : DFTPP17
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP17

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010821MA.M
 Title : SVOA CALIBRATION
 Last Update : Thu Jan 14 17:28:01 2021

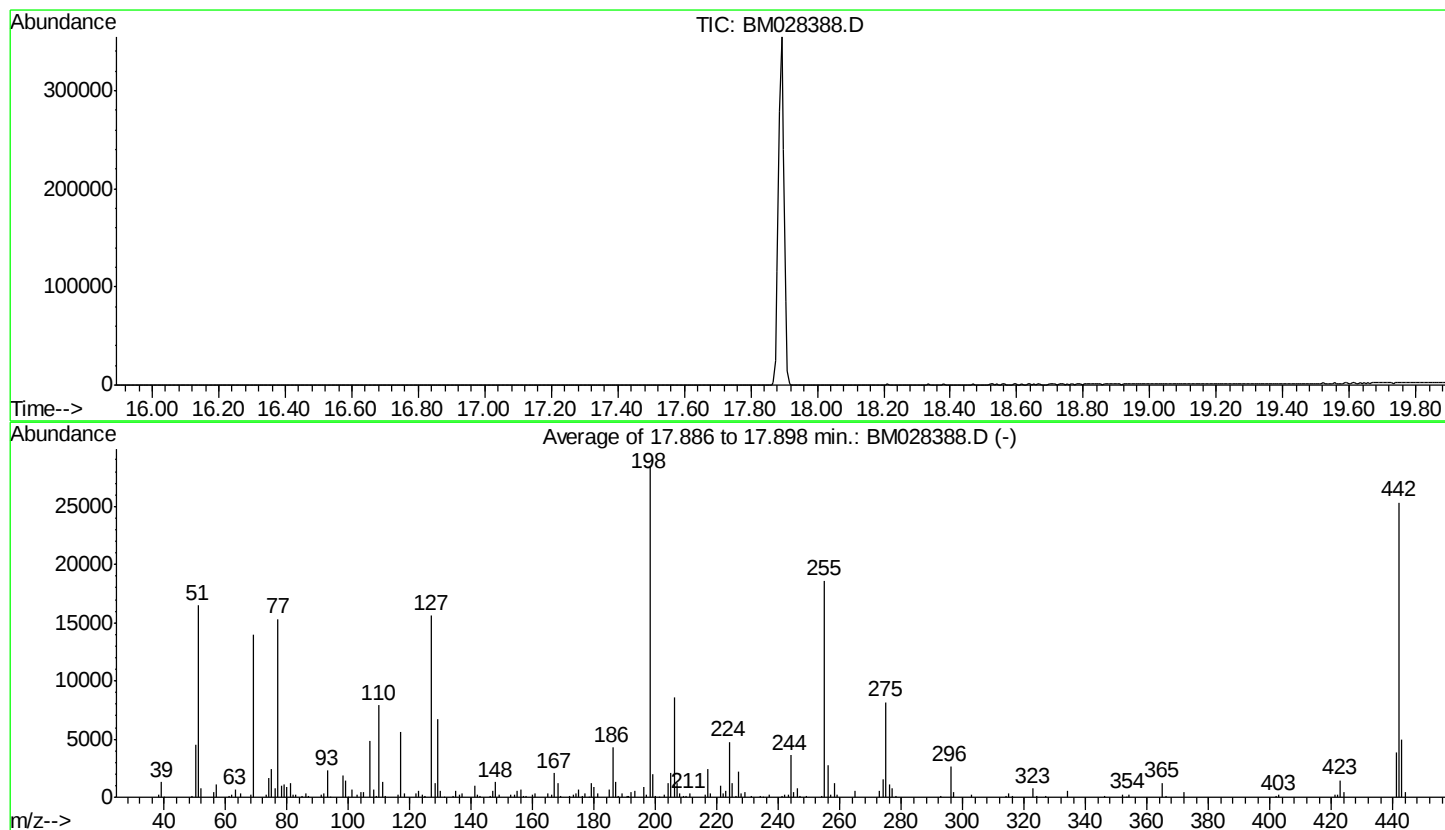

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.7	16457	PASS
68	69	0.00	2	2.0	275	PASS
69	198	0.00	100	48.9	13928	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.7	15579	PASS
197	198	0.00	2	0.7	187	PASS
198	198	100	100	100.0	28506	PASS
199	198	5	9	7.1	2021	PASS
275	198	10	60	28.7	8172	PASS
365	198	1	100	4.4	1255	PASS
441	198	0.01	100	13.4	3833	PASS
442	198	50	100	89.0	25365	PASS
443	442	15	24	19.5	4956	PASS

Scan 2494 (17.857 min): BM028388.D
DFTPP17

m/z	Abundance
44.00	244.0
206.90	201.0

Instrument :
BNA_M
ClientSampleId :
DFTPP17

m/z	Abundance
38.00	251.0
39.10	1467.0
40.00	171.0
44.00	247.0
49.00	202.0
50.10	5128.0
51.10	18328.0
52.00	869.0
56.00	530.0
57.00	1209.0
61.00	175.0
62.00	250.0
63.00	659.0
65.00	284.0
68.00	310.0
69.00	15089.0
73.00	263.0
74.00	1952.0
75.00	2496.0
76.10	847.0
77.10	16920.0
78.00	1142.0
79.00	1181.0
80.00	1016.0
81.00	1288.0
82.00	309.0
82.90	257.0
85.00	206.0
86.00	458.0
86.90	205.0
90.90	277.0
91.90	361.0
93.00	2467.0
98.00	1868.0
99.00	1562.0
101.00	757.0
102.90	227.0
104.00	444.0
105.00	461.0
107.00	5247.0
108.00	712.0
110.00	8241.0
111.00	1293.0
116.00	319.0
117.00	5944.0
118.00	367.0
122.00	367.0
122.90	531.0
124.00	259.0
124.90	214.0
127.00	15846.0
128.00	1258.0
129.00	6800.0
129.90	584.0
133.80	228.0
135.00	615.0
136.00	219.0
137.00	385.0
141.00	989.0
141.90	261.0
142.90	176.0
147.00	570.0
148.00	1357.0
148.90	300.0
152.90	279.0
154.00	208.0
155.00	517.0
156.00	726.0
157.90	185.0
160.00	306.0
160.90	393.0
165.00	292.0
166.00	280.0
167.00	2006.0
168.00	1228.0
169.00	151.0
171.80	153.0
173.00	253.0
174.00	340.0
175.00	676.0
177.00	282.0
178.90	1208.0
180.00	975.0
181.00	351.0
185.00	629.0
186.00	4176.0
187.00	1295.0
187.90	182.0
188.90	279.0
190.90	160.0
192.00	346.0
193.00	534.0

Instrument :
BNA_M
ClientSampleId :
DFTPP17

195.90	734.0
197.10	292.0
198.00	26864.0
198.90	1961.0
202.90	212.0
204.00	1201.0
205.00	1948.0
206.00	7905.0
207.00	1404.0
207.90	410.0
209.00	158.0
211.00	268.0
215.90	192.0
217.00	2310.0
218.00	302.0
221.00	1155.0
221.90	226.0
222.90	509.0
224.00	4262.0
225.00	1099.0
226.00	168.0
227.00	2062.0
228.00	316.0
229.00	406.0
233.90	179.0
237.00	277.0
241.00	167.0
241.90	244.0
243.00	226.0
244.00	3253.0
245.00	513.0
246.00	676.0
247.00	153.0
254.20	182.0
255.00	16384.0
256.00	2668.0
257.00	262.0
258.00	1023.0
258.90	239.0
264.90	449.0
273.00	535.0
274.00	1352.0
275.00	7165.0
276.00	1018.0
276.90	714.0
296.00	2284.0
296.90	373.0
302.90	276.0
315.00	192.0
323.00	639.0
334.00	410.0
353.10	156.0
354.00	202.0
365.00	947.0
372.00	296.0
402.90	186.0
421.00	181.0
421.90	213.0
422.90	1042.0
423.90	386.0
440.90	2771.0
442.00	17448.0
443.00	3469.0
443.90	335.0

Instrument :
BNA_M
ClientSampleId :
DFTPP17

m/z	Abundance
38.00	348.0
39.00	1558.0
43.90	244.0
49.00	204.0
50.10	5379.0
51.10	19720.0
52.10	1020.0
55.90	641.0
57.00	1268.0
61.00	211.0
61.90	265.0
63.00	711.0
65.00	359.0
68.10	318.0
69.00	17152.0
73.00	299.0
74.00	2001.0
75.00	2922.0
76.00	854.0
77.10	18432.0
78.00	1217.0
79.00	1349.0
80.00	1085.0
81.00	1453.0
82.00	282.0
83.00	250.0
85.00	200.0
86.00	452.0
87.00	201.0
91.00	302.0
91.90	424.0
93.00	2673.0
94.00	174.0
98.00	2194.0
99.00	1649.0
100.00	161.0
101.00	890.0
102.90	240.0
103.90	524.0
104.90	486.0
107.00	5584.0
108.00	823.0
109.00	203.0
110.00	9593.0
111.00	1559.0
111.90	228.0
116.00	308.0
117.00	6632.0
118.00	451.0
122.00	427.0
123.00	736.0
124.00	275.0
125.00	284.0
127.00	19112.0
128.00	1508.0
129.00	8226.0
130.00	742.0
131.00	151.0
133.90	219.0
134.90	634.0
136.00	269.0
137.00	423.0
141.00	1206.0
141.90	367.0
142.90	177.0
146.00	260.0
147.00	657.0
147.90	1554.0
149.00	296.0
152.90	304.0
154.00	278.0
155.00	613.0
156.00	765.0
157.00	215.0
159.90	320.0
160.90	482.0
164.90	513.0
165.90	267.0
167.00	2675.0
168.00	1387.0
169.00	198.0
171.90	169.0
173.00	256.0
173.90	440.0
175.00	844.0
176.00	214.0
176.90	367.0
178.00	169.0
178.90	1549.0
180.00	1054.0
181.00	464.0
185.00	738.0

Instrument :
BNA_M
ClientSampleId :
DFTPP17

186.00	5126.0
187.00	1539.0
188.00	198.0
189.00	451.0
191.10	183.0
191.90	543.0
193.00	600.0
195.90	972.0
197.10	271.0
198.00	34696.0
198.90	2494.0
200.00	232.0
201.30	158.0
202.90	268.0
204.00	1404.0
205.00	2501.0
206.00	10493.0
207.00	1524.0
208.00	428.0
208.90	170.0
209.90	183.0
210.90	485.0
216.00	230.0
217.00	2869.0
218.00	368.0
221.00	1227.0
221.90	310.0
223.00	667.0
224.00	5732.0
225.00	1460.0
225.90	195.0
227.00	2598.0
227.90	436.0
229.00	488.0
231.00	226.0
234.00	182.0
235.00	169.0
237.00	218.0
240.90	162.0
242.00	320.0
243.00	280.0
244.00	4478.0
245.00	548.0
246.00	913.0
246.90	216.0
248.90	222.0
254.10	221.0
255.00	22704.0
256.00	3319.0
257.00	248.0
258.00	1439.0
258.90	218.0
265.00	659.0
273.00	672.0
274.00	1852.0
275.00	9753.0
276.00	1263.0
276.90	946.0
278.00	194.0
292.90	202.0
296.00	3120.0
296.90	434.0
303.00	262.0
314.00	181.0
315.00	357.0
316.00	243.0
323.00	898.0
323.90	152.0
327.00	185.0
334.00	772.0
346.00	176.0
352.00	284.0
353.90	302.0
365.00	1580.0
366.00	249.0
372.00	480.0
401.90	247.0
402.90	227.0
421.00	250.0
422.00	295.0
423.00	1788.0
423.90	507.0
441.00	4559.0
442.00	30264.0
443.00	6081.0
443.90	552.0

Instrument :
BNA_M
ClientSampleId :
DFTPP17

m/z	Abundance
38.00	193.0
39.00	839.0
44.00	196.0
50.00	3137.0
51.10	11323.0
52.00	529.0
55.90	285.0
57.00	732.0
63.00	462.0
65.00	200.0
68.00	197.0
69.00	9544.0
73.00	225.0
74.00	1112.0
75.00	1751.0
76.10	554.0
77.10	10656.0
78.00	691.0
79.00	850.0
80.00	636.0
81.00	855.0
82.00	203.0
83.00	171.0
85.90	234.0
90.90	177.0
92.00	225.0
93.00	1698.0
98.00	1409.0
99.00	983.0
101.00	391.0
103.00	170.0
103.90	300.0
105.00	310.0
107.00	3749.0
108.00	522.0
110.00	5825.0
111.00	962.0
116.00	208.0
117.00	4382.0
118.00	287.0
121.90	276.0
123.00	357.0
124.00	174.0
127.00	11780.0
128.00	963.0
129.00	4989.0
129.90	456.0
135.00	442.0
136.00	150.0
136.90	236.0
141.00	800.0
141.90	203.0
147.00	386.0
148.00	1013.0
148.90	175.0
152.90	235.0
154.00	192.0
154.90	416.0
156.00	535.0
157.00	155.0
159.90	174.0
161.00	287.0
164.90	317.0
165.90	167.0
167.00	1544.0
168.00	872.0
171.90	167.0
174.00	290.0
175.00	599.0
176.90	283.0
178.90	1024.0
180.00	782.0
180.90	332.0
185.00	519.0
186.00	3533.0
187.00	1109.0
188.90	224.0
190.90	154.0
191.90	350.0
193.00	475.0
196.00	822.0
198.00	23960.0
198.90	1610.0
203.00	229.0
204.00	981.0
205.00	1826.0
206.00	7235.0
207.00	1209.0
208.00	305.0
211.00	221.0
216.00	162.0
217.00	2161.0

Instrument :
BNA_M
ClientSampleId :
DFTPP17

217.90	272.0
220.90	760.0
221.70	303.0
223.00	357.0
224.00	4216.0
225.00	1103.0
227.00	1997.0
228.00	312.0
228.90	348.0
236.90	206.0
242.00	210.0
243.00	258.0
244.00	3023.0
245.00	389.0
246.00	702.0
255.00	16816.0
256.00	2327.0
257.00	181.0
258.00	1147.0
258.90	155.0
264.90	439.0
272.90	438.0
274.00	1391.0
275.00	7599.0
276.00	953.0
277.00	699.0
278.00	150.0
292.80	168.0
296.00	2425.0
297.00	368.0
303.00	277.0
315.00	295.0
323.00	758.0
324.00	158.0
334.00	487.0
345.90	170.0
351.90	285.0
354.00	261.0
364.90	1238.0
372.00	436.0
401.90	153.0
403.00	246.0
420.90	199.0
421.90	231.0
423.00	1571.0
424.00	397.0
441.00	4170.0
442.00	28384.0
443.00	5319.0
443.90	463.0

Instrument :

BNA_M

ClientSampleId :

DFTPP17