

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011422\
 Data File : BM033741.D
 Acq On : 14 Jan 2022 22:58
 Operator : CG/JU
 Sample : N1124-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WASTE-CLASS-BOILER-PIT

Quant Time: Jan 17 00:28:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 13 07:49:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.972	152	167372	20.000	ng	0.00
21) Naphthalene-d8	10.789	136	701649	20.000	ng	# 0.00
39) Acenaphthene-d10	14.601	164	449610	20.000	ng	0.00
64) Phenanthrene-d10	17.336	188	751674	20.000	ng	0.00
76) Chrysene-d12	21.500	240	621409	20.000	ng	0.00
86) Perylene-d12	23.918	264	689185	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.513	112	1194301	112.538	ng	0.00
7) Phenol-d6	7.125	99	1391605	97.295	ng	0.00
23) Nitrobenzene-d5	9.136	82	1284479	84.544	ng	0.00
42) 2,4,6-Tribromophenol	16.083	330	583447	124.242	ng	0.00
45) 2-Fluorobiphenyl	13.230	172	2393361	69.722	ng	-0.01
79) Terphenyl-d14	19.948	244	2395981	69.403	ng	-0.01
Target Compounds						
						Qvalue
6) Aniline	7.290	93	37996	2.345	ng	# 1
9) Benzaldehyde	7.119	77	291654	32.858	ng	# 1
10) Phenol	7.148	94	41222	2.867	ng	# 1
11) bis(2-Chloroethyl)ether	7.366	93	40232	3.547	ng	# 1
15) Benzyl Alcohol	8.225	79	60575	5.188	ng	# 69
18) Hexachloroethane	9.101	117	716858	142.627	ng	# 1
19) n-Nitroso-di-n-propyla...	8.772	70	289756	31.007	ng	# 66
22) Acetophenone	8.801	105	3587115	190.621	ng	# 52
24) Nitrobenzene	9.189	77	150753	10.435	ng	# 55
25) Isophorone	9.719	82	338576	13.758	ng	# 1
26) 2-Nitrophenol	9.925	139	41172	6.764	ng	# 1
27) 2,4-Dimethylphenol	10.013	122	92571	9.109	ng	# 15
28) bis(2-Chloroethoxy)met...	10.201	93	58890	3.630	ng	# 1
31) Naphthalene	10.836	128	1131075	29.412	ng	# 96
35) Caprolactam	11.719	113	14081	4.563	ng	# 1
37) 2-Methylnaphthalene	12.436	142	391476	15.065	ng	99
38) 1-Methylnaphthalene	12.654	142	232262	9.196	ng	99
71) Phenanthrene	17.377	178	131748	3.063	ng	# 94
75) Fluoranthene	19.389	202	106129	2.350	ng	89
78) Pyrene	19.748	202	108834	2.488	ng	# 94
80) Butylbenzylphthalate	20.642	149	61090	3.126	ng	99
84) Bis(2-ethylhexyl)phtha...	21.418	149	1581912	53.143	ng	98
85) Di-n-octyl phthalate	22.342	149	169740	3.507	ng	# 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011422\
Data File : BM033741.D
Acq On : 14 Jan 2022 22:58
Operator : CG/JU
Sample : N1124-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WASTE-CLASS-BOILER-PIT

Quant Time: Jan 17 00:28:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 13 07:49:01 2022
Response via : Initial Calibration




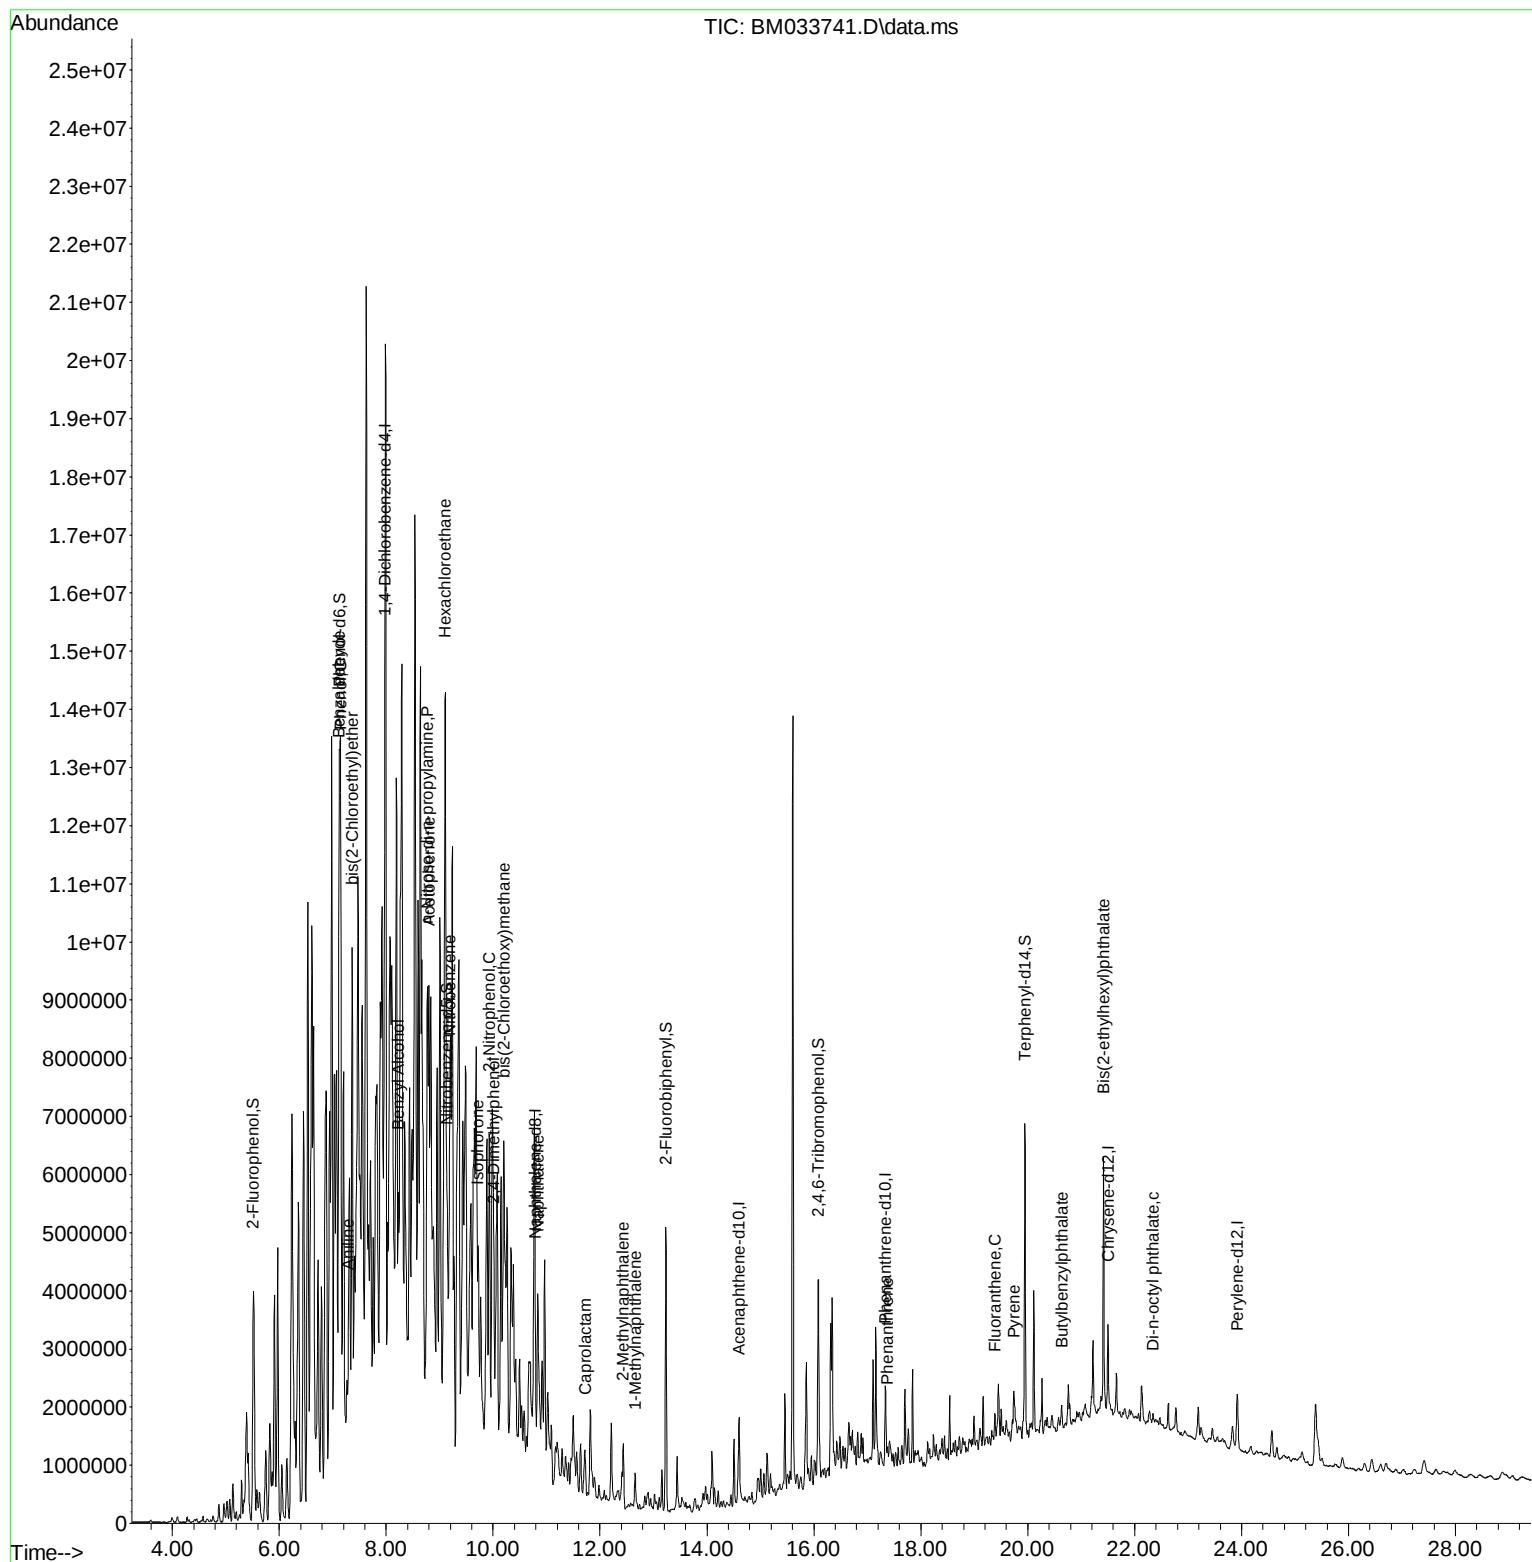


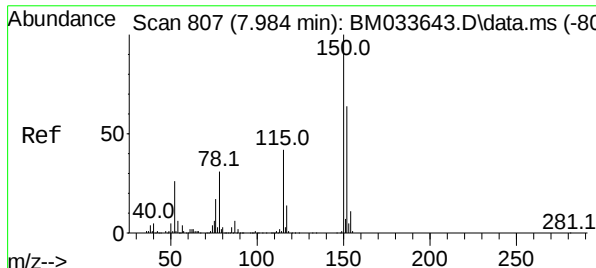

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.972 min Scan# 807
 Delta R.T. -0.000 min
 Lab File: BM033741.D
 Acq: 14 Jan 2022 22:58




Instrument :
 BNA_M
 ClientSampleId :
 WASTE-CLASS-BOILER-PIT


Tgt Ion:	152	Resp:	167372
Ion	Ratio	Lower	Upper
152	100		
150	150.2	128.9	193.3
115	62.7	53.0	79.6

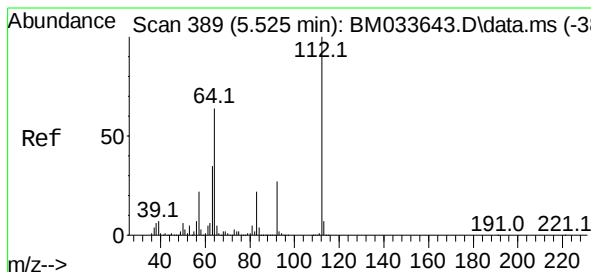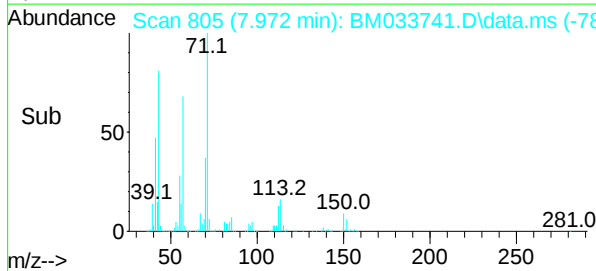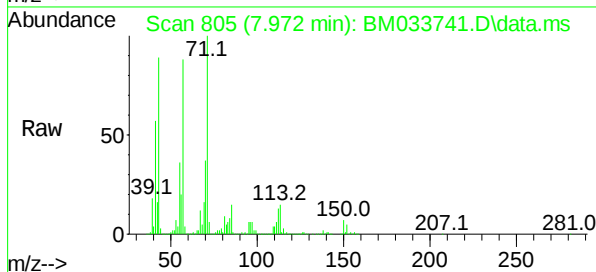

2-Fluorophenol
 Concen: 112.538 ng
 RT: 5.513 min Scan# 387
 Delta R.T. 0.000 min
 Lab File: BM033741.D
 Acq: 14 Jan 2022 22:58

Tgt Ion:	112	Resp:	1194301
Ion	Ratio	Lower	Upper
112	100		
64	59.0	55.5	83.3
63	32.3	31.3	46.9

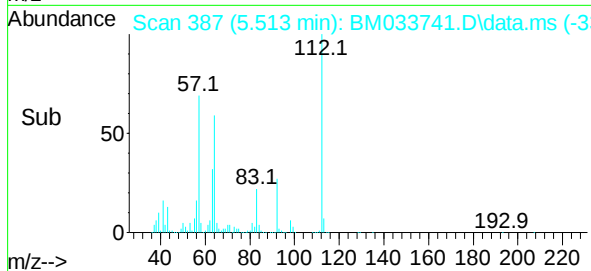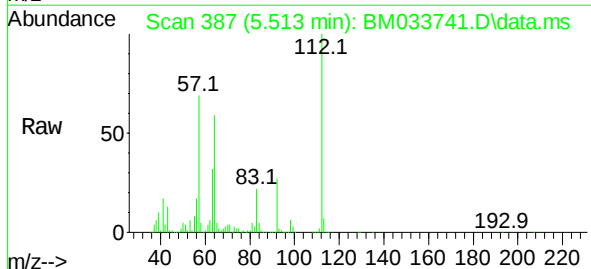

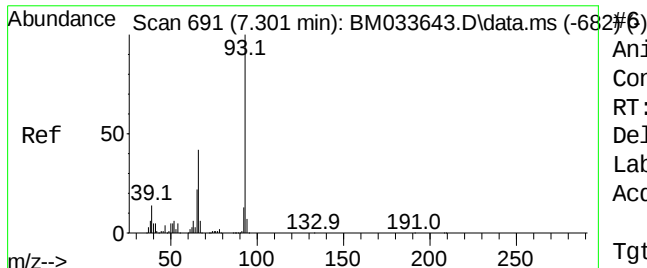

Aniline

Concen: 2.345 ng

RT: 7.290 min Scan#

Delta R.T. 0.000 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58

Instrument :

BNA_M

ClientSampleId :

WASTE-CLASS-BOILER-PIT





Tgt Ion: 93 Resp: 37996

Ion Ratio Lower Upper

93 100

66 69.9 36.0 54.0#

65 158.7 18.2 27.4#

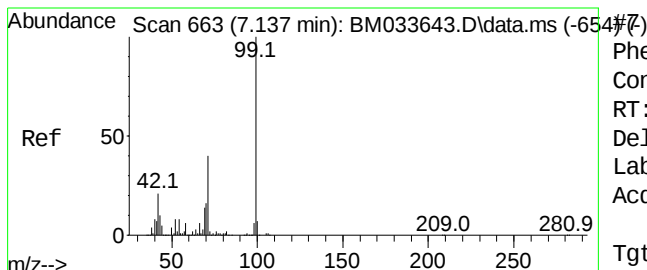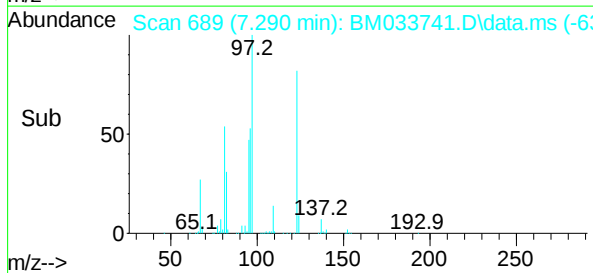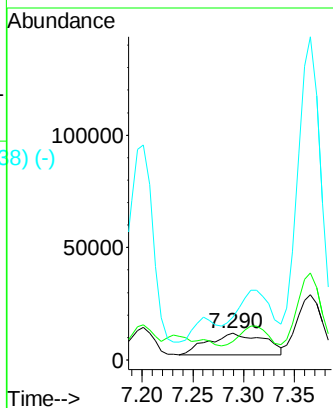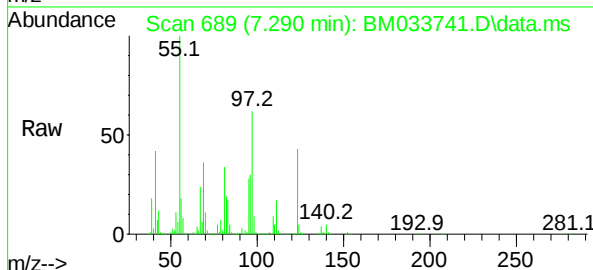

Phenol-d6

Concen: 97.295 ng

RT: 7.125 min Scan# 661

Delta R.T. 0.000 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58




Tgt Ion: 99 Resp: 1391605


Ion Ratio Lower Upper

99 100

42 34.0 20.3 30.5#

71 80.0 34.5 51.7#

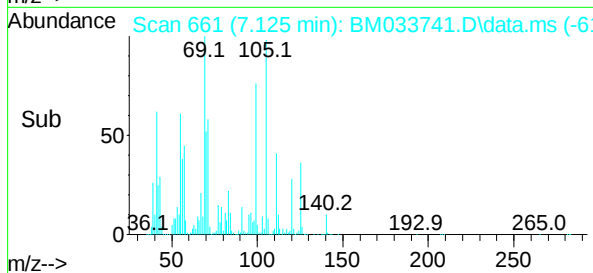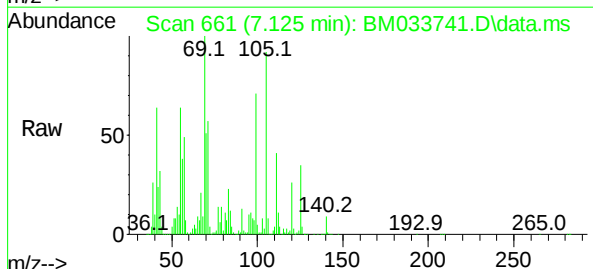

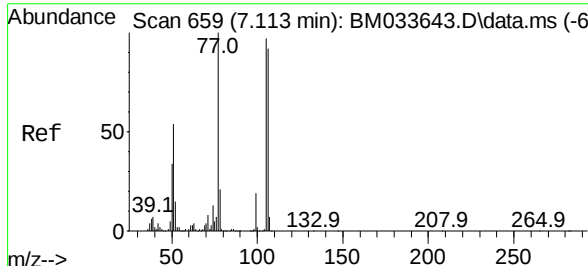

Benzaldehyde

Concen: 32.858 ng

RT: 7.119 min Scan# 659

Delta R.T. 0.024 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58

Instrument :





BNA_M

ClientSampleId :

WASTE-CLASS-BOILER-PIT

Tgt Ion: 77 Resp: 291654

Ion	Ratio	Lower	Upper
77	100		
105	643.7	67.1	107.1#
106	57.5	64.3	104.3#

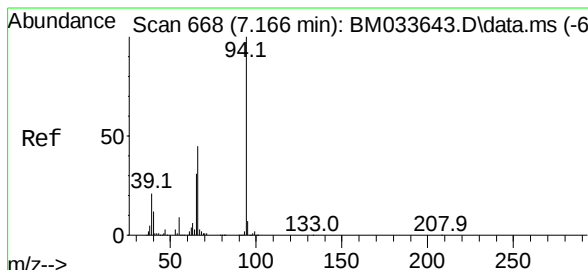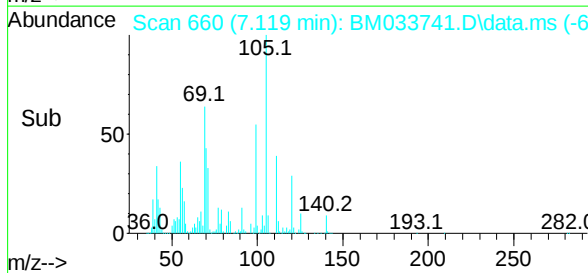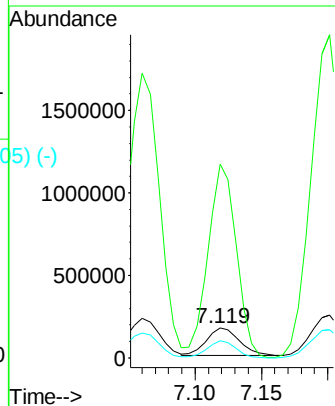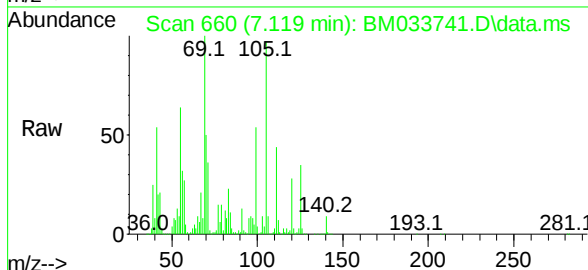

Phenol

Concen: 2.867 ng

RT: 7.148 min Scan# 665




Delta R.T. -0.006 min


Lab File: BM033741.D

Acq: 14 Jan 2022 22:58

Tgt Ion: 94 Resp: 41222

Ion	Ratio	Lower	Upper
94	100		
65	182.5	15.5	55.5#
66	138.9	28.5	68.5#


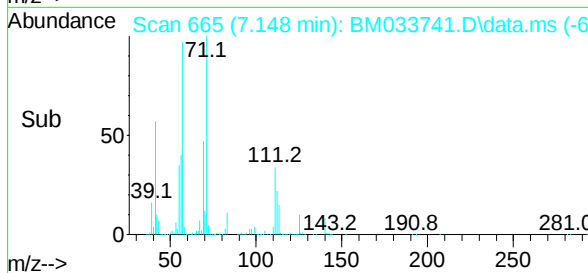
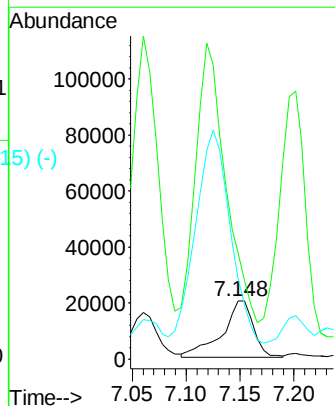
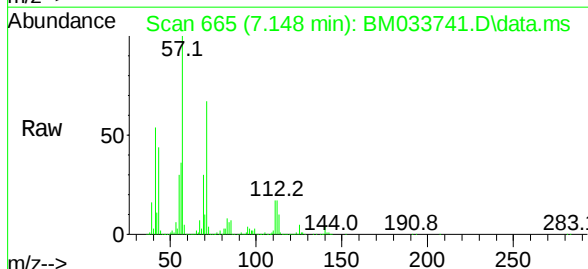


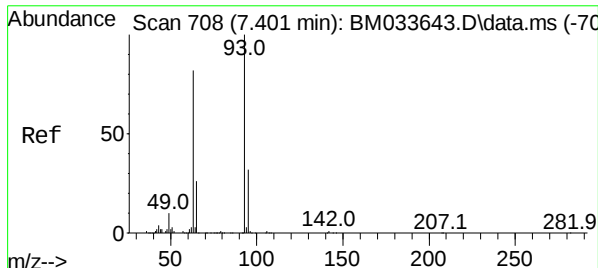

bis(2-Chloroethyl)ether
 Concen: 3.547 ng
 RT: 7.366 min Scan# 708
 Delta R.T. -0.018 min
 Lab File: BM033741.D
 Acq: 14 Jan 2022 22:58




Instrument :
 BNA_M
 ClientSampleId :
 WASTE-CLASS-BOILER-PIT


Tgt Ion: 93 Resp: 40232
 Ion Ratio Lower Upper
 93 100
 63 299.0 67.0 107.0#
 95 1242.8 11.6 51.6#

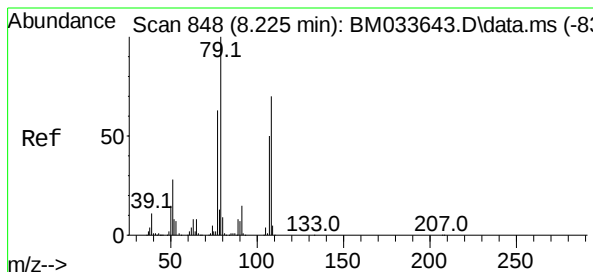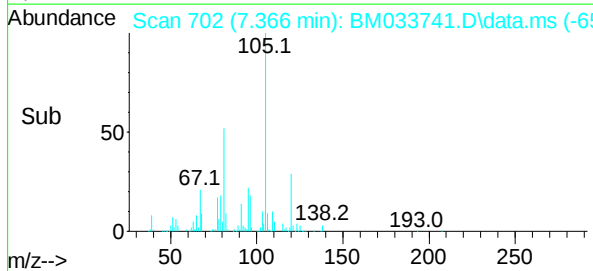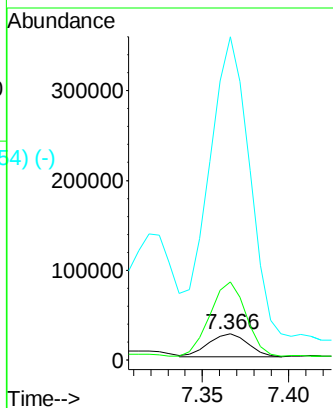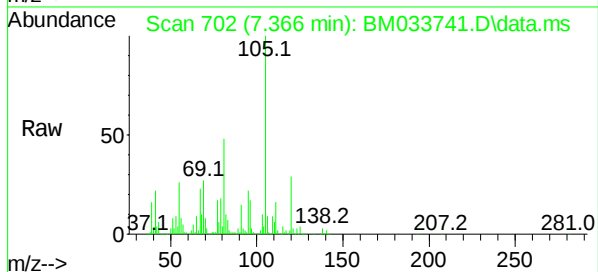

Benzyl Alcohol
 Concen: 5.188 ng
 RT: 8.225 min Scan# 848
 Delta R.T. 0.018 min
 Lab File: BM033741.D
 Acq: 14 Jan 2022 22:58

Tgt Ion: 79 Resp: 60575
 Ion Ratio Lower Upper
 79 100
 108 18.6 51.1 76.7#
 77 63.0 53.8 80.8


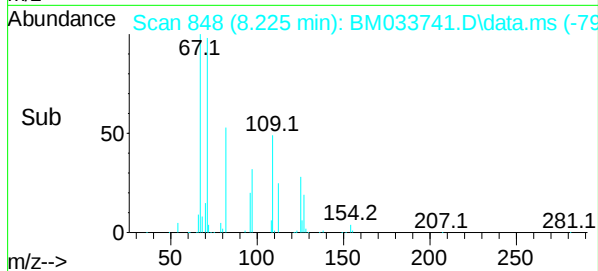

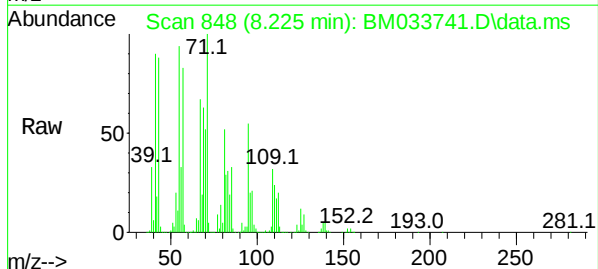


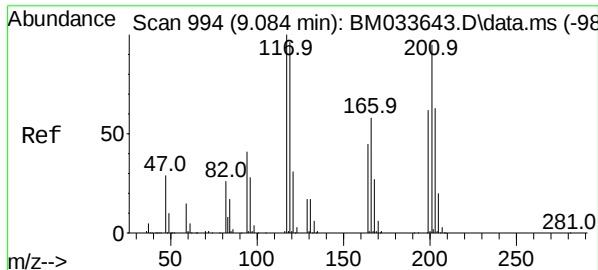

#18
Hexachloroethane
Concen: 142.627 ng
RT: 9.101 min Scan# 941
Delta R.T. 0.035 min
Lab File: BM033741.D
Acq: 14 Jan 2022 22:58




Instrument :
BNA_M
ClientSampleId :
WASTE-CLASS-BOILER-PIT


Tgt Ion:117 Resp: 716858
Ion Ratio Lower Upper
117 100
119 595.9 75.0 112.6#
201 0.0 75.2 112.8#

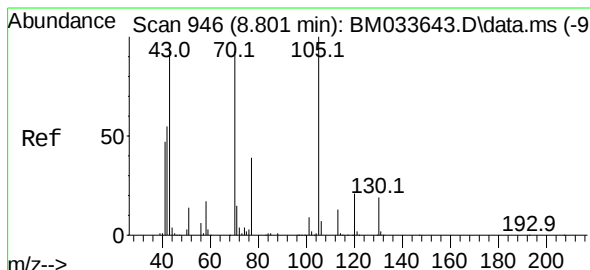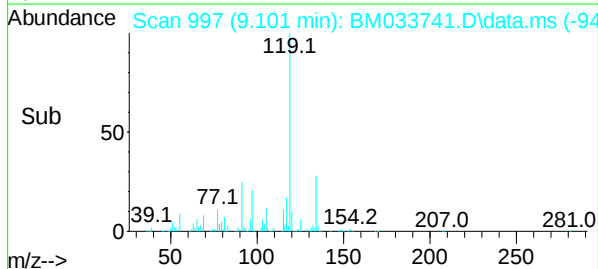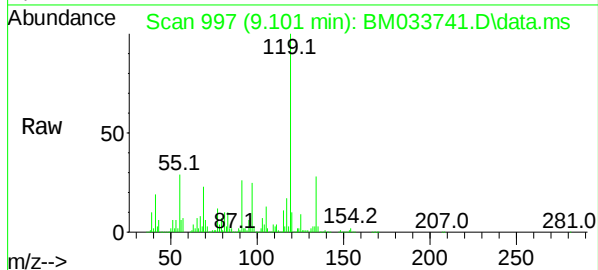

#19
n-Nitroso-di-n-propylamine
Concen: 31.007 ng
RT: 8.772 min Scan# 941
Delta R.T. -0.012 min
Lab File: BM033741.D
Acq: 14 Jan 2022 22:58

Tgt Ion: 70 Resp: 289756
Ion Ratio Lower Upper
70 100
42 94.7 54.1 81.1#
101 0.2 7.8 11.6#
130 0.0 13.9 20.9#


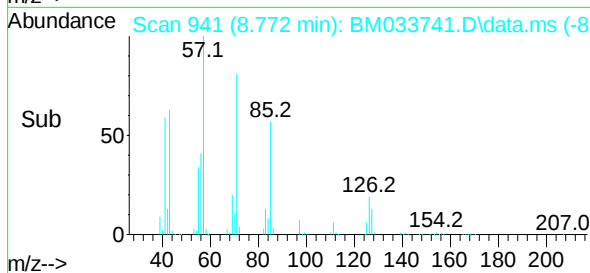
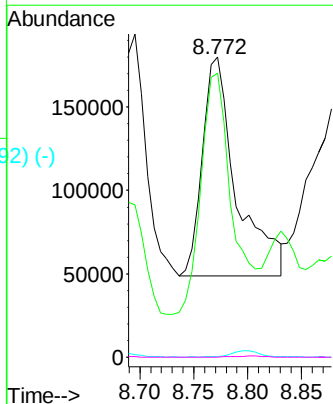
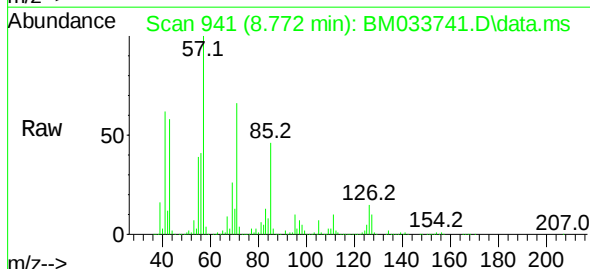


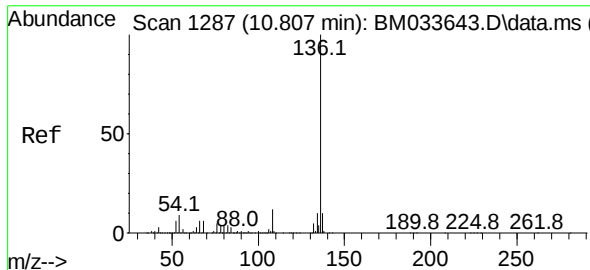

Naphthalene-d8
Concen: 20.000 ng
RT: 10.789 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BM033741.D
Acq: 14 Jan 2022 22:58




Instrument :
BNA_M
ClientSampleId :
WASTE-CLASS-BOILER-PIT


Tgt Ion:	136	Resp:	701649
Ion	Ratio	Lower	Upper
136	100		
137	12.3	8.6	13.0
54	12.5	8.3	12.5#
68	10.2	5.0	7.6#

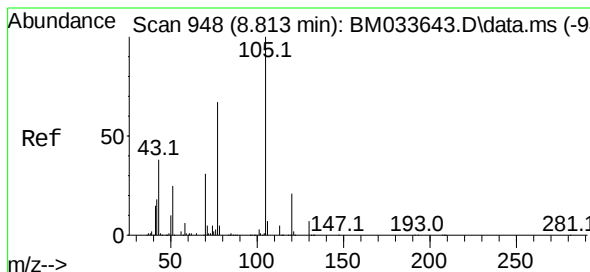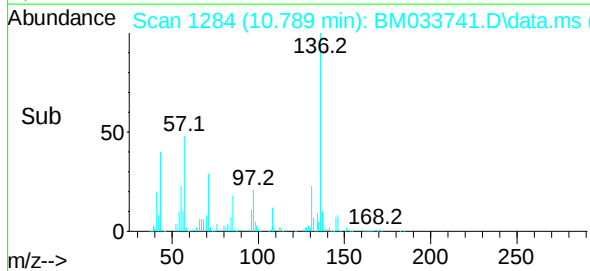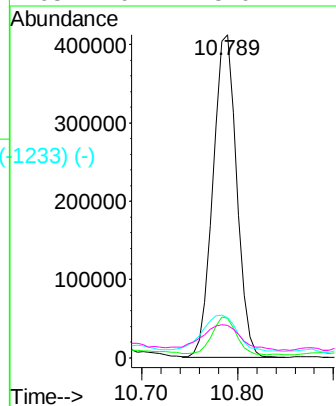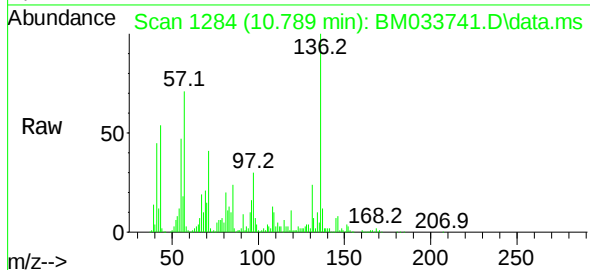

Acetophenone
Concen: 190.621 ng
RT: 8.801 min Scan# 946
Delta R.T. 0.006 min
Lab File: BM033741.D
Acq: 14 Jan 2022 22:58

Tgt Ion:	105	Resp:	3587115
Ion	Ratio	Lower	Upper
105	100		
71	7.2	1.6	2.4#
51	4.5	27.7	41.5#
120	0.3	16.2	24.2#

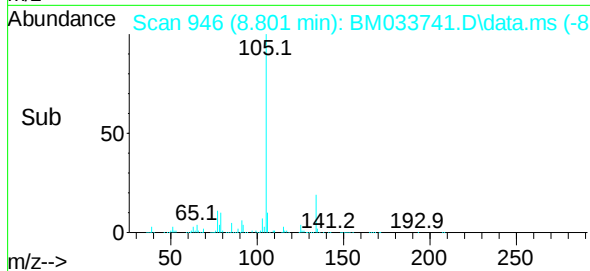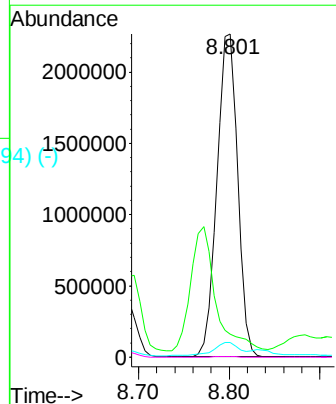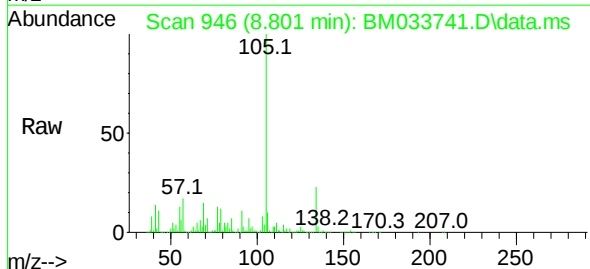

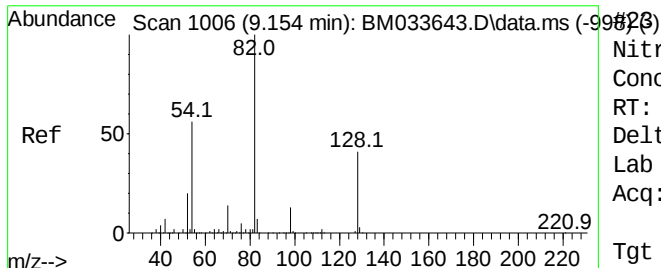

Nitrobenzene-d5

Concen: 84.544 ng

RT: 9.136 min Scan# 1003

Delta R.T. 0.000 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58

Instrument :

BNA_M

ClientSampleId :

WASTE-CLASS-BOILER-PIT





Tgt Ion: 82 Resp: 1284479

Ion Ratio Lower Upper

82 100

128 36.8 28.1 42.1

54 49.1 46.1 69.1

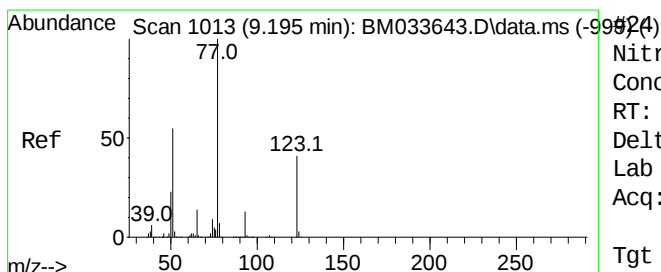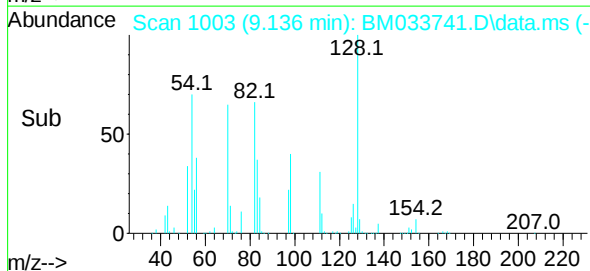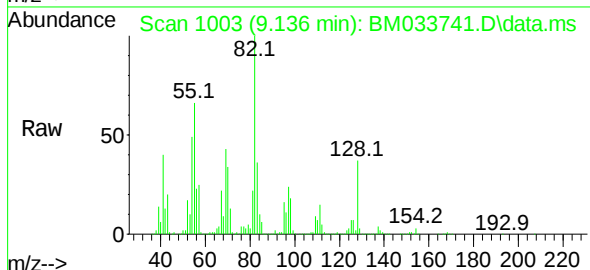

Nitrobenzene

Concen: 10.435 ng

RT: 9.189 min Scan# 1012

Delta R.T. 0.012 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58




Tgt Ion: 77 Resp: 150753


Ion Ratio Lower Upper

77 100

123 30.8 29.8 44.8

65 69.7 11.5 17.3#

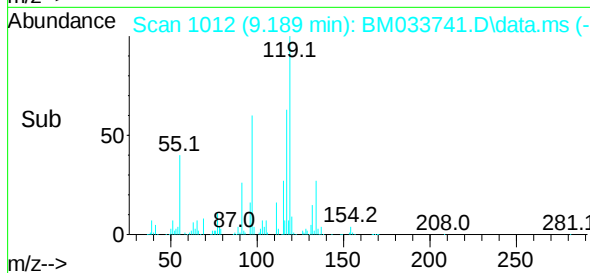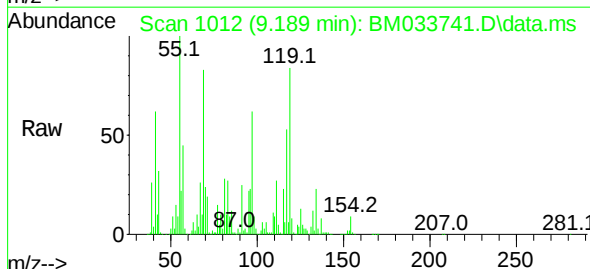

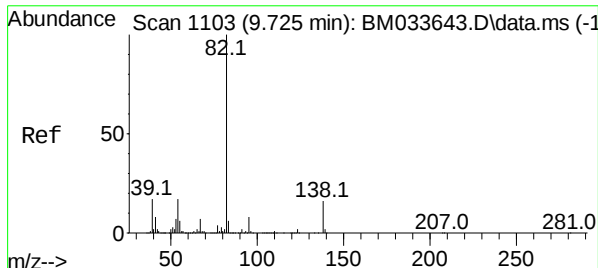

Isophorone

Concen: 13.758 ng

RT: 9.719 min Scan#

Delta R.T. 0.006 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58

Instrument :

BNA_M

ClientSampleId :

WASTE-CLASS-BOILER-PIT





Tgt Ion: 82 Resp: 338576

Ion Ratio Lower Upper

82 100

95 177.4 6.4 9.6#

138 10.3 12.4 18.6#

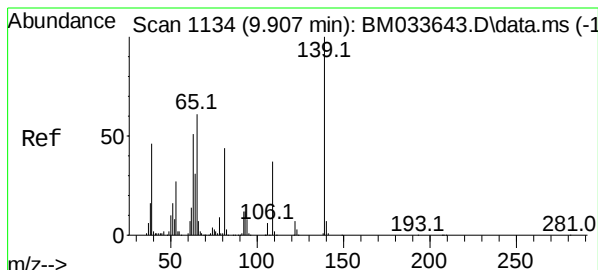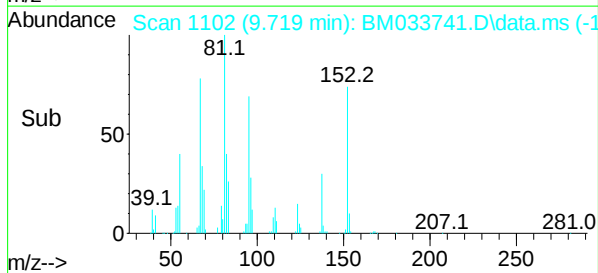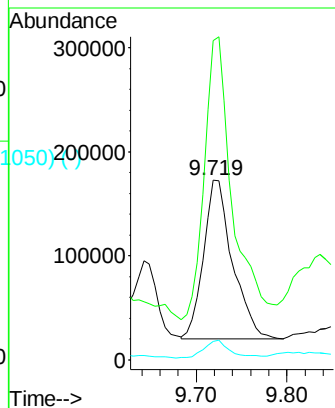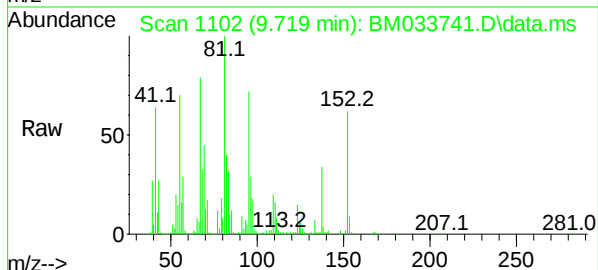

2-Nitrophenol

Concen: 6.764 ng

RT: 9.925 min Scan# 1137

Delta R.T. 0.029 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58




Tgt Ion: 139 Resp: 41172


Ion Ratio Lower Upper

139 100

109 143.1 33.0 49.6#

65 173.4 57.2 85.8#


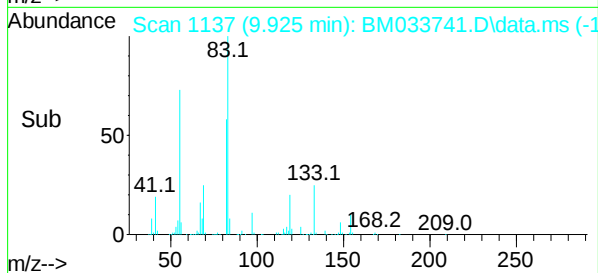
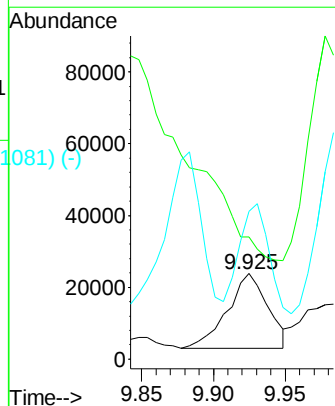
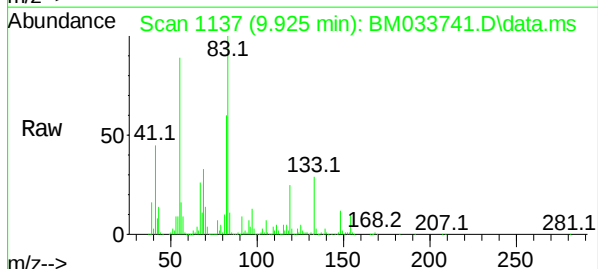


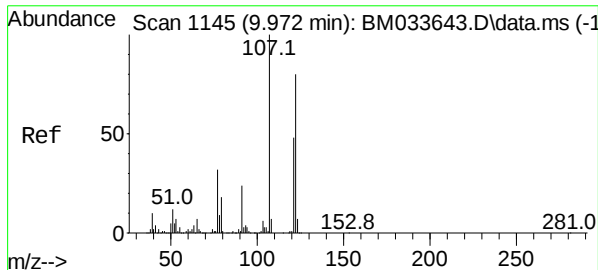

2,4-Dimethylphenol
Concen: 9.109 ng
RT: 10.013 min Scan# 1152
Delta R.T. 0.059 min
Lab File: BM033741.D
Acq: 14 Jan 2022 22:58




Instrument :
BNA_M
ClientSampleId :
WASTE-CLASS-BOILER-PIT


Tgt Ion:122 Resp: 92571
Ion Ratio Lower Upper
122 100
107 250.5 105.3 157.9#
121 100.4 49.7 74.5#

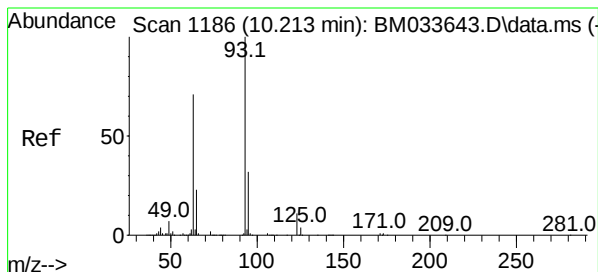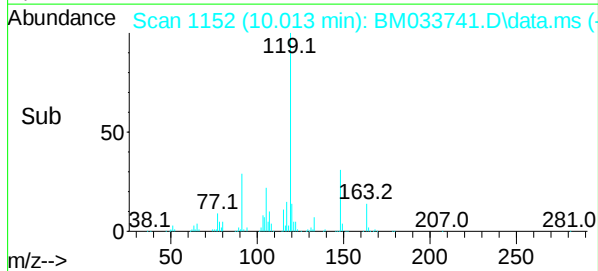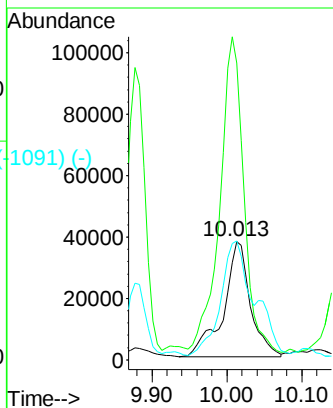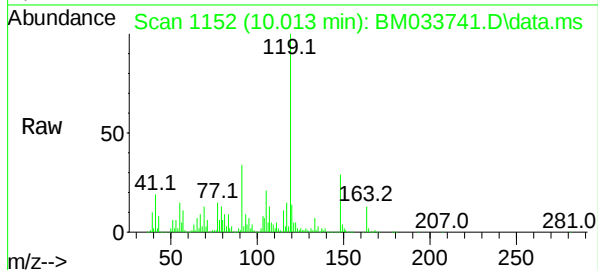

bis(2-Chloroethoxy)methane
Concen: 3.630 ng
RT: 10.201 min Scan# 1184
Delta R.T. 0.012 min
Lab File: BM033741.D
Acq: 14 Jan 2022 22:58

Tgt Ion: 93 Resp: 58890
Ion Ratio Lower Upper
93 100
95 154.2 26.8 40.2#
123 52.8 8.0 12.0#


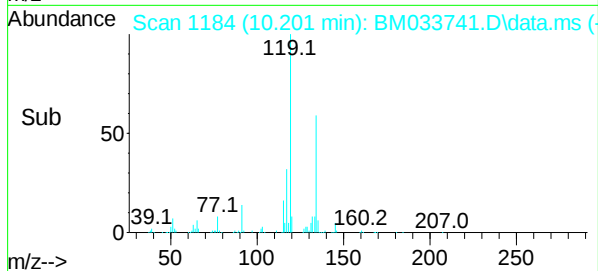

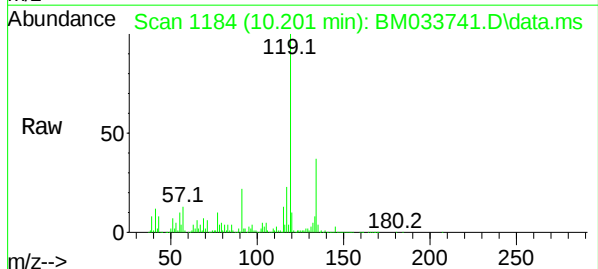


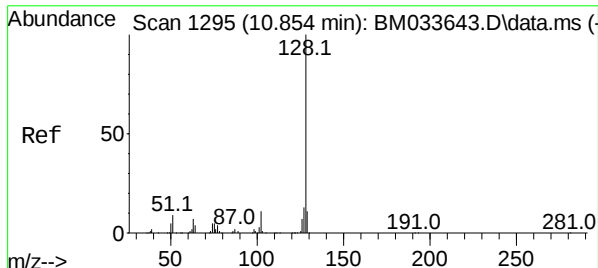

Scan 1295 (10.854 min): BM033643.D\data.ms (-1284) (-)
 Naphthalene
 Concen: 29.412 ng
 RT: 10.836 min Scan# 1284
 Delta R.T. 0.000 min
 Lab File: BM033741.D
 Acq: 14 Jan 2022 22:58




Instrument : BNA_M
 ClientSampleId : BM033741.D
 WASTE-CLASS-BOILER-PIT


Tgt Ion:	128	Resp:	1131075
Ion	Ratio	Lower	Upper
128	100		
129	12.8	8.5	12.7#
127	14.6	10.8	16.2

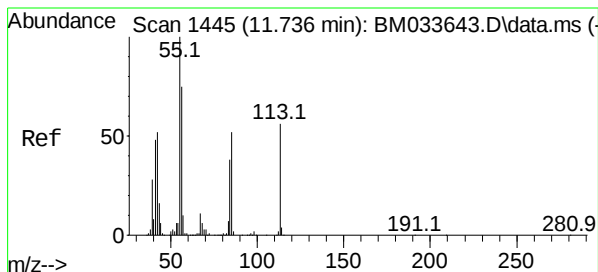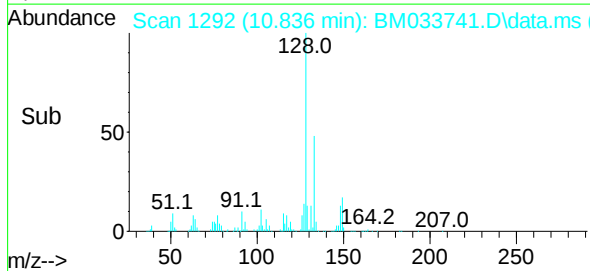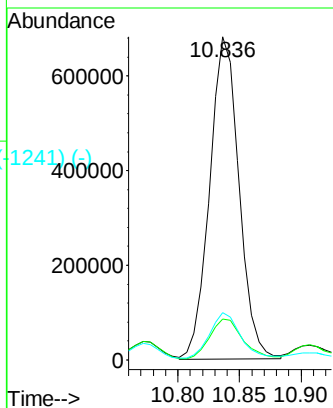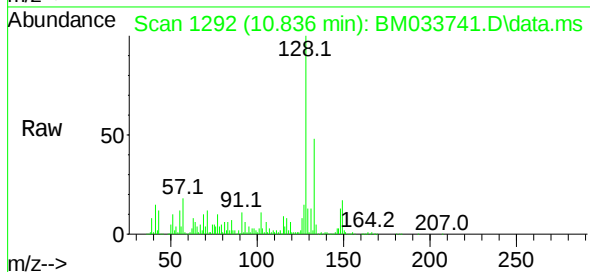

Scan 1445 (11.736 min): BM033643.D\data.ms (-1435) (-)
 Caprolactam
 Concen: 4.563 ng
 RT: 11.719 min Scan# 1442
 Delta R.T. -0.012 min
 Lab File: BM033741.D
 Acq: 14 Jan 2022 22:58

Tgt Ion:	113	Resp:	14081
Ion	Ratio	Lower	Upper
113	100		
55	828.5	183.6	223.6#
56	412.6	143.7	183.7#


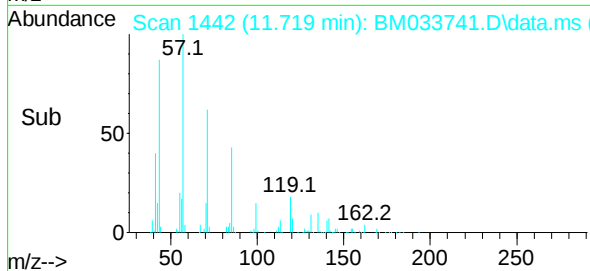

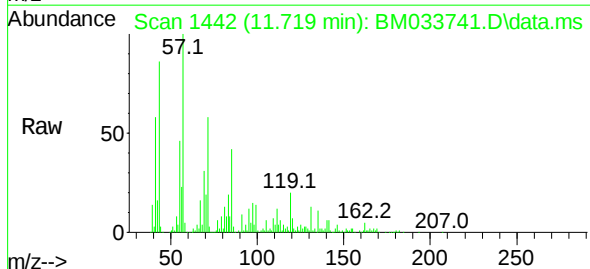


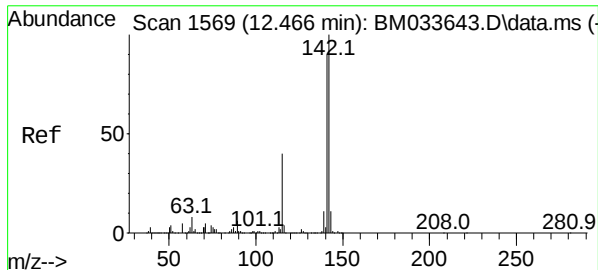

2-Methylnaphthalene
Concen: 15.065 ng
RT: 12.436 min Scan# 1569
Delta R.T. -0.012 min
Lab File: BM033741.D
Acq: 14 Jan 2022 22:58




Instrument :
BNA_M
ClientSampleId :
WASTE-CLASS-BOILER-PIT

Tgt Ion:142 Resp: 391476
Ion Ratio Lower Upper
142 100
141 89.4 72.2 108.2
115 40.0 33.0 49.6

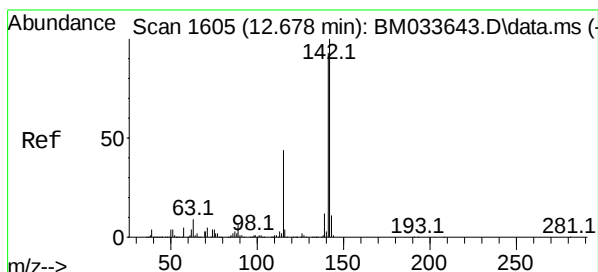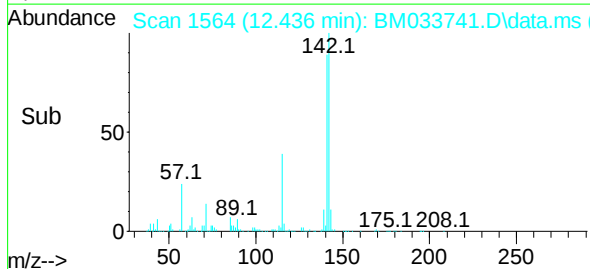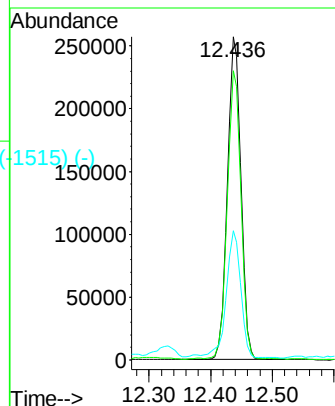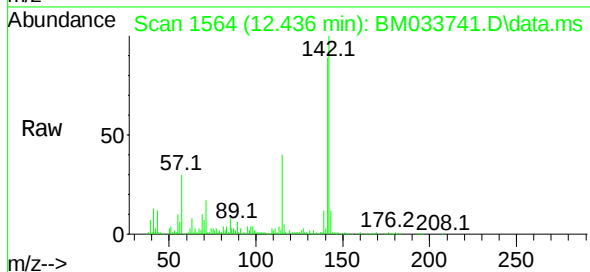

1-Methylnaphthalene
Concen: 9.196 ng
RT: 12.654 min Scan# 1601
Delta R.T. -0.012 min
Lab File: BM033741.D
Acq: 14 Jan 2022 22:58

Tgt Ion:142 Resp: 232262
Ion Ratio Lower Upper
142 100
141 92.8 75.0 112.4
116 5.1 3.5 5.3

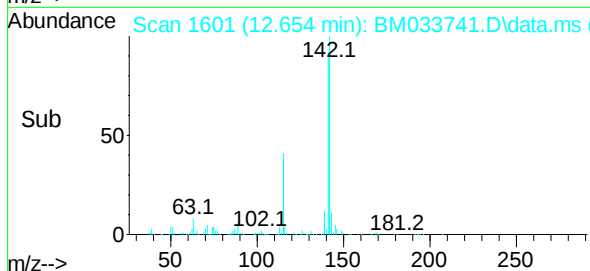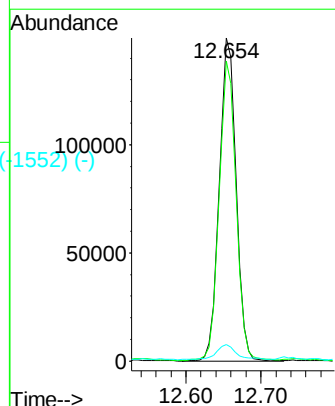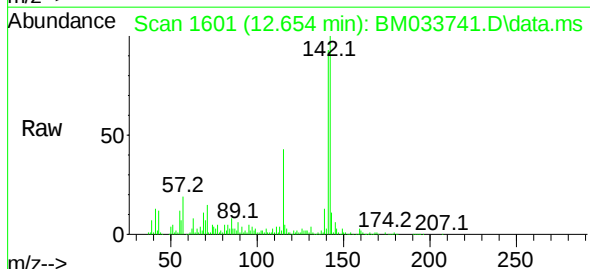

Abundance Scan 1936 (14.624 min): BM033643.D\data.ms (-1539) (-)

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.601 min Scan# 1936

Delta R.T. -0.006 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58

Instrument :

BNA_M

ClientSampleId :

WASTE-CLASS-BOILER-PIT

Tgt Ion:164 Resp: 449610



Ion Ratio Lower Upper

164 100


162 102.4 79.7 119.5

160 44.5 34.2 51.4

Abundance Scan 1932 (14.601 min): BM033741.D\data.ms

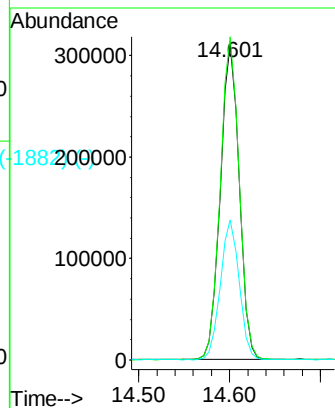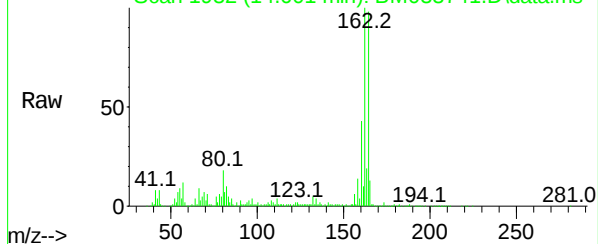

Abundance Scan 1932 (14.601 min): BM033741.D\data.ms (-188200) (-)

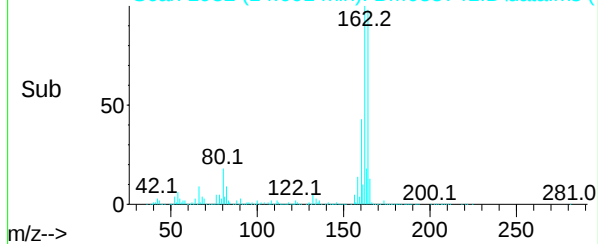

Abundance Scan 2188 (16.107 min): BM033643.D\data.ms (-2140) (-)

2,4,6-Tribromophenol

Concen: 124.242 ng

RT: 16.083 min Scan# 2184

Delta R.T. -0.006 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58

Tgt Ion:330 Resp: 583447



Ion Ratio Lower Upper

330 100


332 97.3 76.5 114.7


141 38.4 35.9 53.9

Abundance Scan 2184 (16.083 min): BM033741.D\data.ms

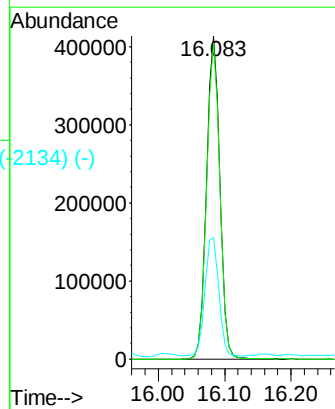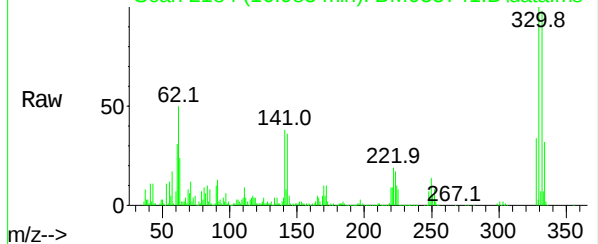

Abundance Scan 2184 (16.083 min): BM033741.D\data.ms (-2134) (-)




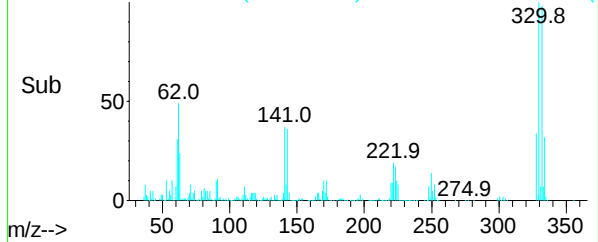


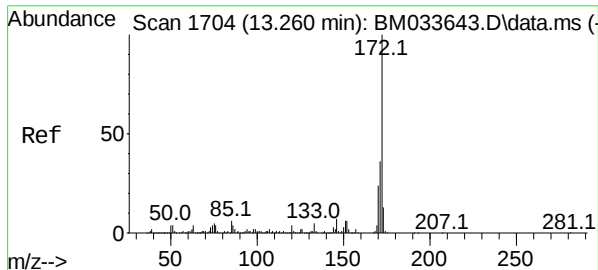

2-Fluorobiphenyl
Concen: 69.722 ng
RT: 13.230 min Scan# 1699
Delta R.T. -0.012 min
Lab File: BM033741.D
Acq: 14 Jan 2022 22:58




Instrument :
BNA_M
ClientSampleId :
WASTE-CLASS-BOILER-PIT


Tgt Ion:172 Resp: 2393361
Ion Ratio Lower Upper
172 100
171 35.9 27.2 40.8
170 23.8 18.7 28.1

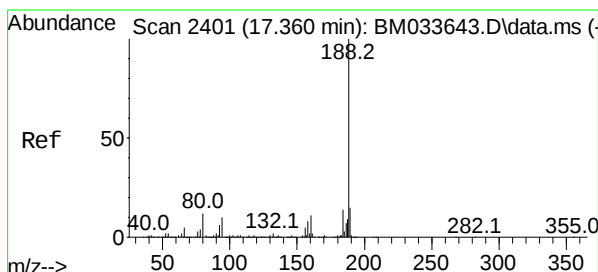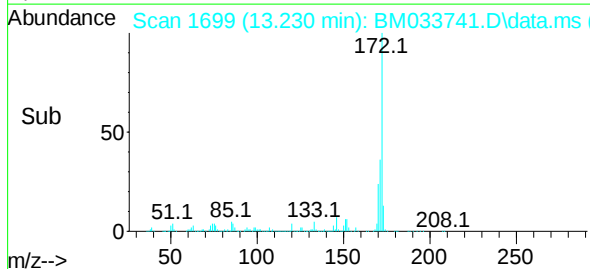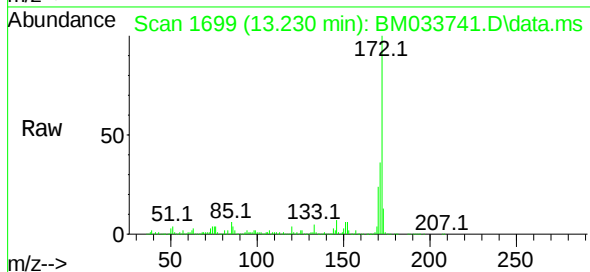

Phenanthrene-d10
Concen: 20.000 ng
RT: 17.336 min Scan# 2397
Delta R.T. -0.006 min
Lab File: BM033741.D
Acq: 14 Jan 2022 22:58

Tgt Ion:188 Resp: 751674
Ion Ratio Lower Upper
188 100
94 9.0 7.5 11.3
80 9.7 8.9 13.3


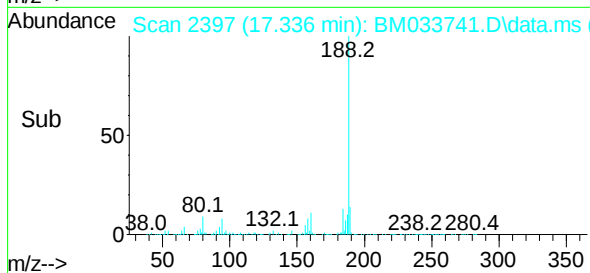

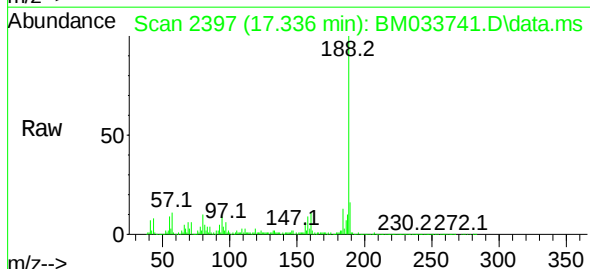


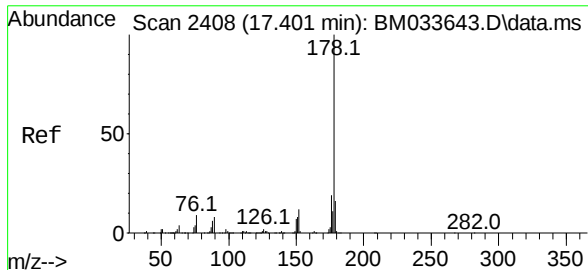

Scan 2408 (17.401 min): BM033643.D\data.ms (-2355) (-)
 Phenanthrene
 Concen: 3.063 ng
 RT: 17.377 min Scan# 2404
 Delta R.T. -0.012 min
 Lab File: BM033741.D
 Acq: 14 Jan 2022 22:58




Instrument :
 BNA_M
 ClientSampleId :
 WASTE-CLASS-BOILER-PIT


Tgt Ion:	178	Resp:	131748
Ion Ratio	Lower	Upper	
178	100		
176	19.8	15.1	22.7
179	19.6	12.0	18.0#

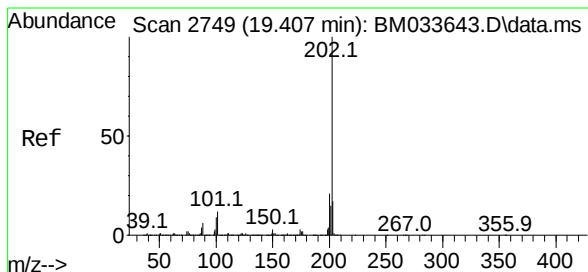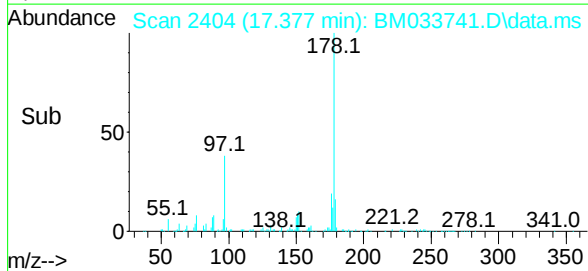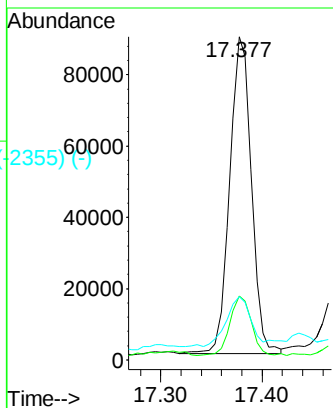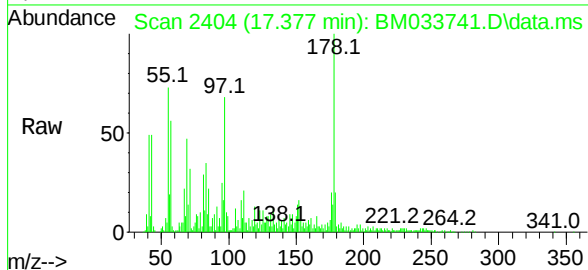

Scan 2749 (19.407 min): BM033643.D\data.ms (-2355) (-)
 Fluoranthene
 Concen: 2.350 ng
 RT: 19.389 min Scan# 2746
 Delta R.T. -0.006 min
 Lab File: BM033741.D
 Acq: 14 Jan 2022 22:58

Tgt Ion:	202	Resp:	106129
Ion Ratio	Lower	Upper	
202	100		
101	11.0	0.0	30.8
203	25.0	0.0	37.2


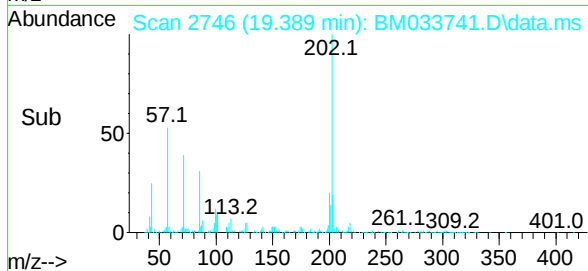

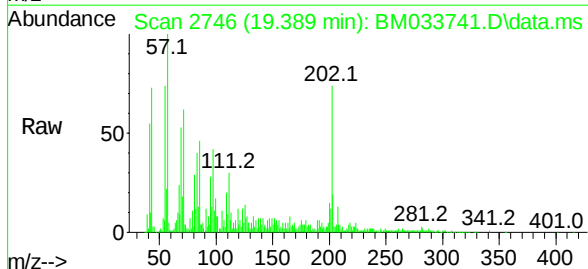


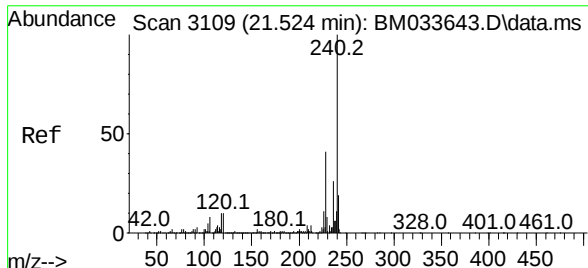

Chrysene-d12
 Concen: 20.000 ng
 RT: 21.500 min Scan# 3109
 Delta R.T. -0.006 min
 Lab File: BM033741.D
 Acq: 14 Jan 2022 22:58




Instrument :
 BNA_M
 ClientSampleId :
 WASTE-CLASS-BOILER-PIT

Tgt Ion:	240	Resp:	621409
Ion	Ratio	Lower	Upper
240	100		
120	10.0	7.8	11.6
236	26.5	20.3	30.5

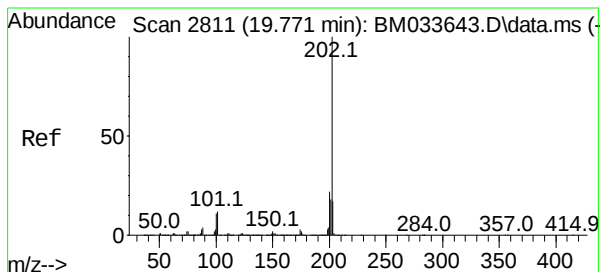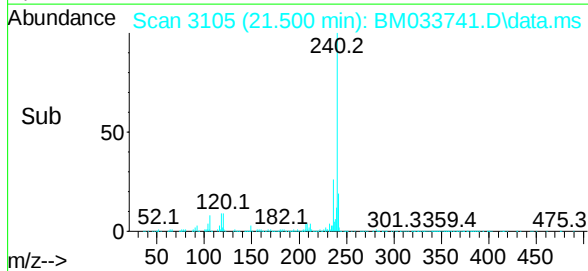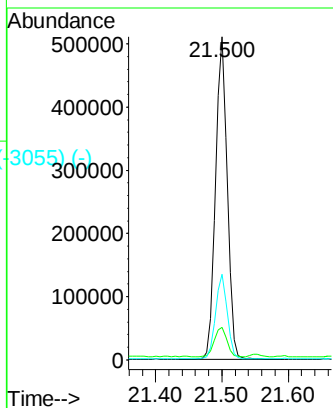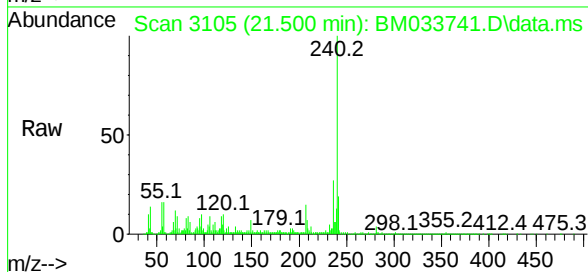


Pyrene
 Concen: 2.488 ng
 RT: 19.748 min Scan# 2807
 Delta R.T. -0.006 min
 Lab File: BM033741.D
 Acq: 14 Jan 2022 22:58

Tgt Ion:	202	Resp:	108834
Ion	Ratio	Lower	Upper
202	100		
200	20.9	16.4	24.6
203	22.7	13.5	20.3#

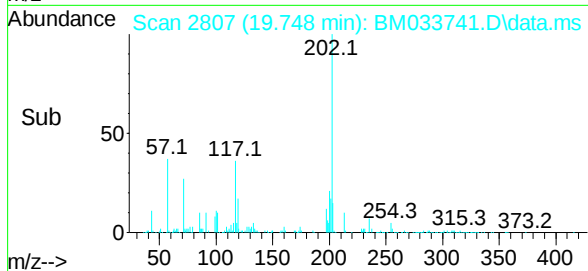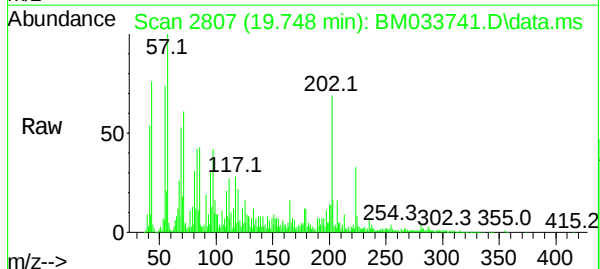

Abundance Scan 2845 (19.971 min): BM033643.D\data.ms (-2879) (-)

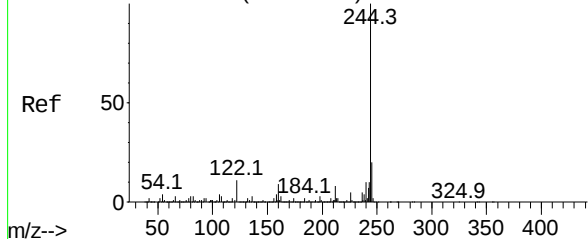

Terphenyl-d14

Concen: 69.403 ng

RT: 19.948 min Scan# 2841

Delta R.T. -0.012 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58

Instrument :

BNA_M

ClientSampleId :

WASTE-CLASS-BOILER-PIT



Tgt Ion:244 Resp: 2395981

Ion Ratio Lower Upper


244 100

212 7.8 5.9 8.9


122 10.1 8.4 12.6

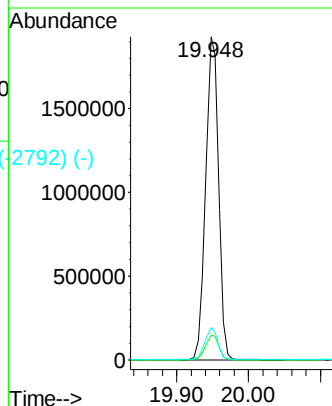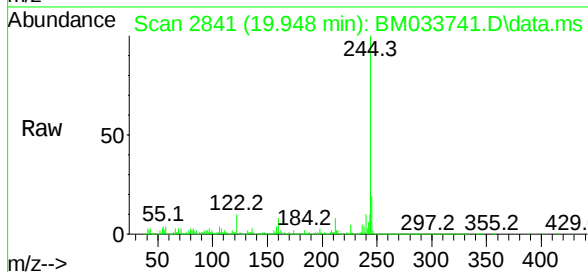

Abundance Scan 2841 (19.948 min): BM033741.D\data.ms (-2792) (-)

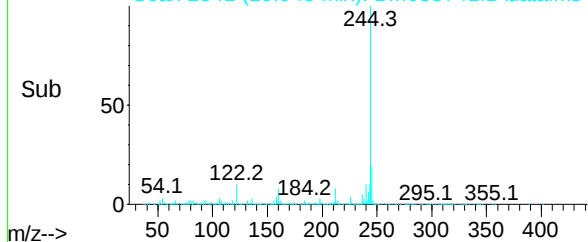

Abundance Scan 2963 (20.665 min): BM033643.D\data.ms (-2960) (-)

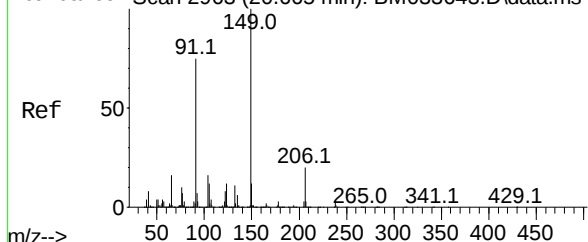

Butylbenzylphthalate

Concen: 3.126 ng

RT: 20.642 min Scan# 2959

Delta R.T. -0.006 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58



Tgt Ion:149 Resp: 61090

Ion Ratio Lower Upper


149 100

91 79.7 63.4 95.0

206 21.6 16.8 25.2

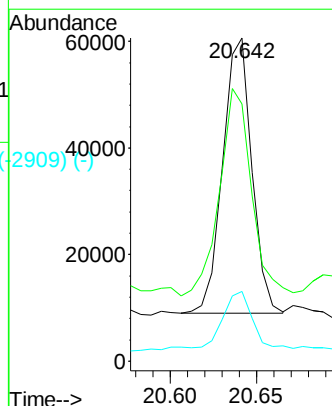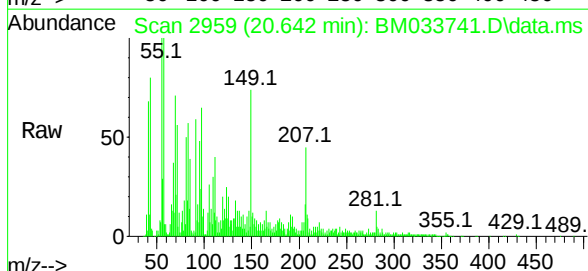

Abundance Scan 2959 (20.642 min): BM033741.D\data.ms (-2909) (-)

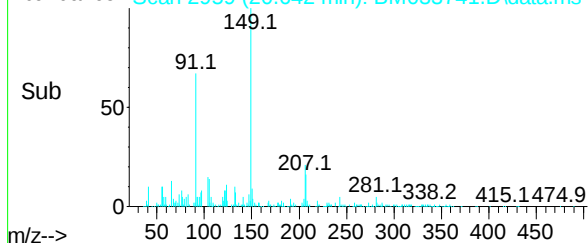

Abundance Scan 3095 (21.442 min): BM033643.D\data.ms (-3089) (-)

Bis(2-ethylhexyl)phthalate

Concen: 53.143 ng

RT: 21.418 min Scan# 3095

Delta R.T. -0.006 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58

Instrument :

BNA_M

ClientSampleId :

WASTE-CLASS-BOILER-PIT

Tgt Ion:149 Resp: 1581912



Ion Ratio Lower Upper

149 100


167 27.6 21.4 32.0

279 4.4 3.0 4.6

Abundance Scan 3091 (21.418 min): BM033741.D\data.ms

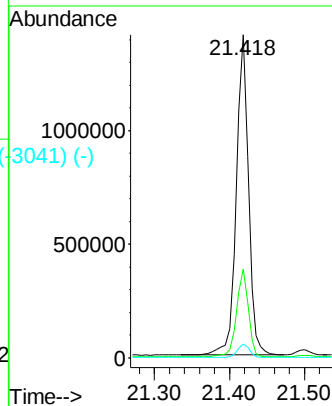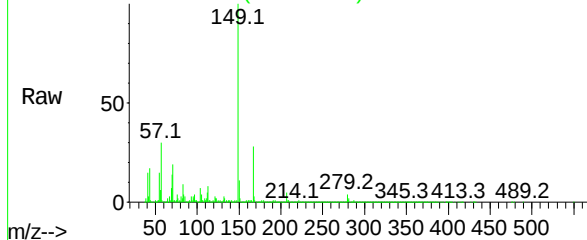

Abundance Scan 3091 (21.418 min): BM033741.D\data.ms (-3041) (-)

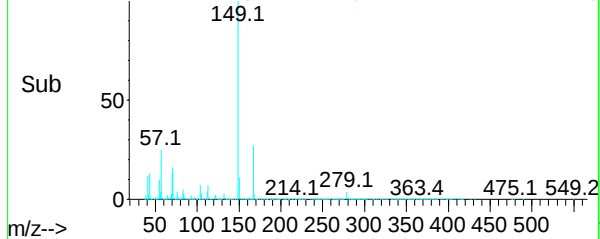

Abundance Scan 3255 (22.383 min): BM033643.D\data.ms (-3245) (-)

Di-n-octyl phthalate

Concen: 3.507 ng

RT: 22.342 min Scan# 3248

Delta R.T. -0.012 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58

Tgt Ion:149 Resp: 169740



Ion Ratio Lower Upper

149 100


167 0.7 1.3 1.9#

43 6.3 10.4 15.6#


Abundance Scan 3248 (22.342 min): BM033741.D\data.ms

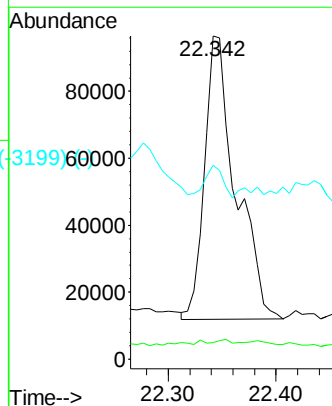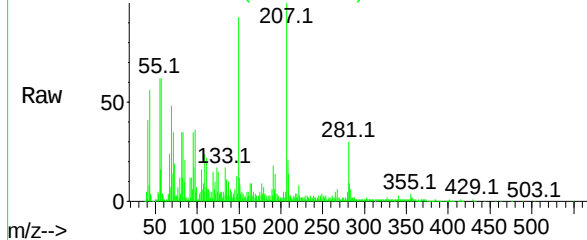

Abundance Scan 3248 (22.342 min): BM033741.D\data.ms (-3199) (-)

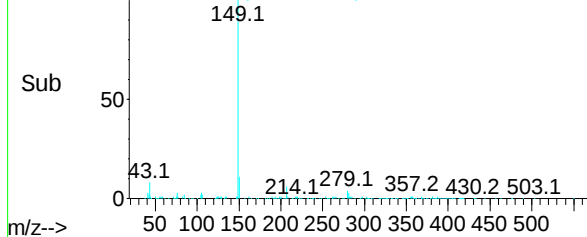

Abundance Scan 3522 (23.953 min): BM033643.D\data.ms (-3522) (-)

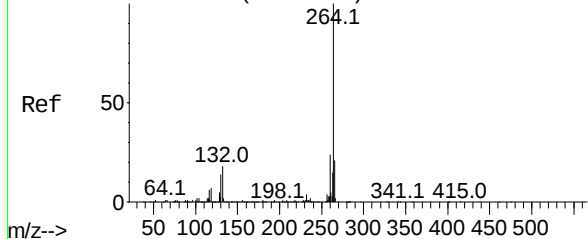

Perylene-d12

Concen: 20.000 ng

RT: 23.918 min Scan#

Delta R.T. -0.012 min

Lab File: BM033741.D

Acq: 14 Jan 2022 22:58

Instrument :

BNA_M

ClientSampleId :

WASTE-CLASS-BOILER-PIT

Tgt Ion:264 Resp: 689185


Ion Ratio Lower Upper

264 100


260 24.4 17.7 26.5

265 22.8 17.7 26.5

Abundance Scan 3516 (23.918 min): BM033741.D\data.ms

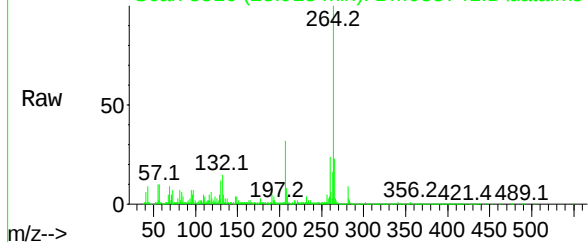

Abundance

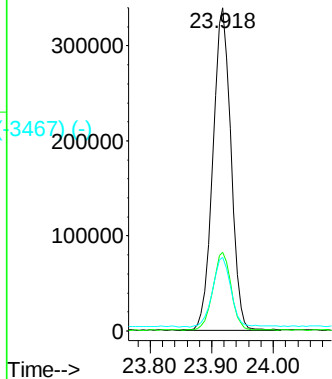

Abundance Scan 3516 (23.918 min): BM033741.D\data.ms (-3467) (-)

