

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011422\
 Data File : BM033726.D
 Acq On : 14 Jan 2022 13:59
 Operator : CG/JU
 Sample : PB142032BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB142032BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.513	379	387	397	rBV	3056627	4425010	54.89%	10.588%
2	7.125	652	661	674	rBV	2951381	4667901	57.90%	11.170%
3	7.966	797	804	811	rVB	577366	909333	11.28%	2.176%
4	9.131	993	1002	1010	rBV	1889901	3115877	38.65%	7.456%
5	10.783	1275	1283	1291	rBV	790627	1336832	16.58%	3.199%
6	13.236	1692	1700	1717	rBV	4949575	7085232	87.88%	16.954%
7	14.607	1926	1933	1950	rBV	1162994	1799250	22.32%	4.305%
8	16.083	2177	2184	2207	rBV	3499508	5066347	62.84%	12.123%
9	17.342	2391	2398	2409	rBV	1349612	1952141	24.21%	4.671%
10	19.953	2836	2842	2853	rBV	6579829	8062241	100.00%	19.292%
11	21.500	3100	3105	3111	rBV	1299666	1641467	20.36%	3.928%
12	23.924	3510	3517	3526	rVB2	817637	1729256	21.45%	4.138%




Sum of corrected areas: 41790887

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011422\
Data File : BM033726.D
Acq On : 14 Jan 2022 13:59
Operator : CG/JU
Sample : PB142032BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142032BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

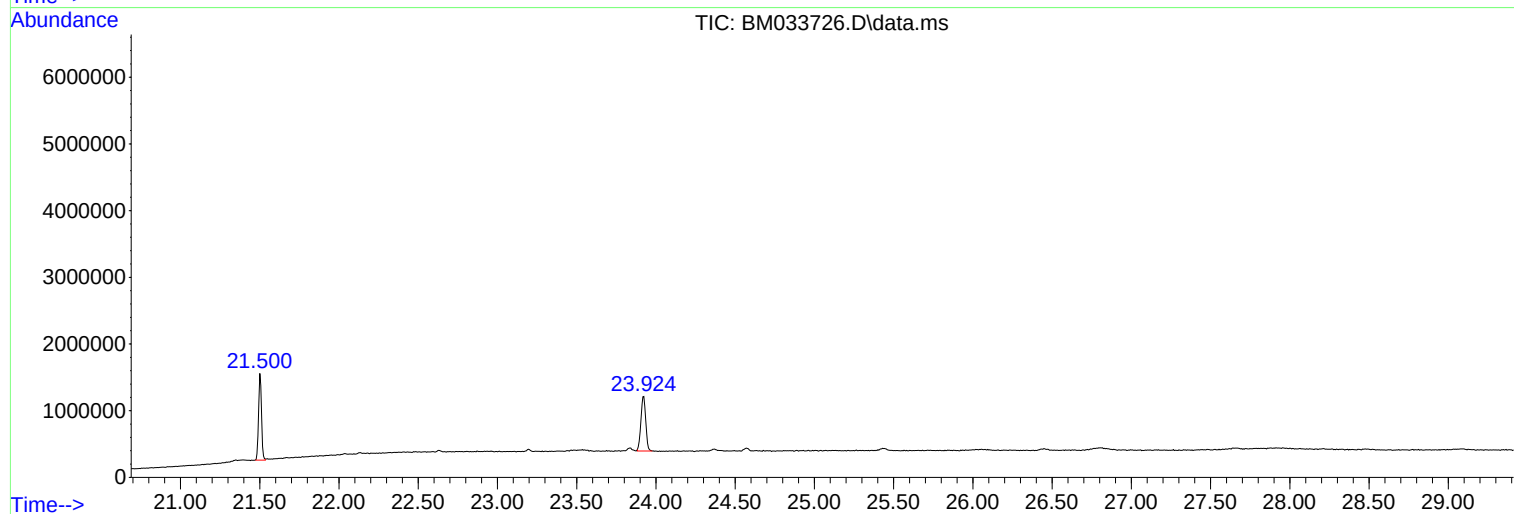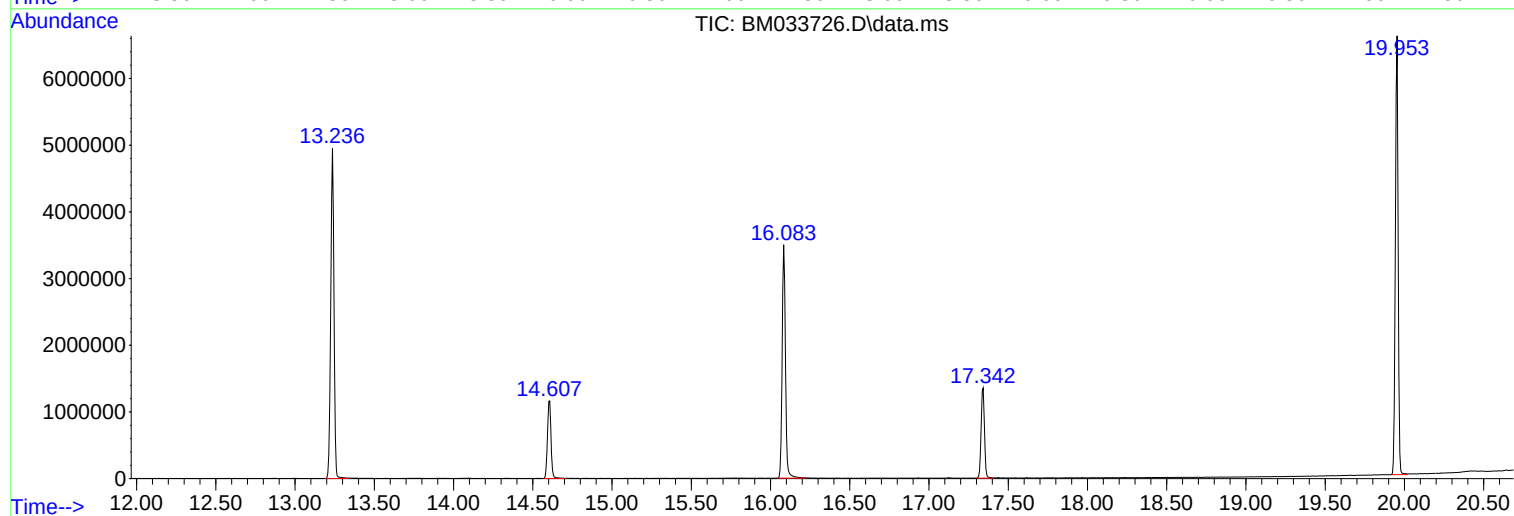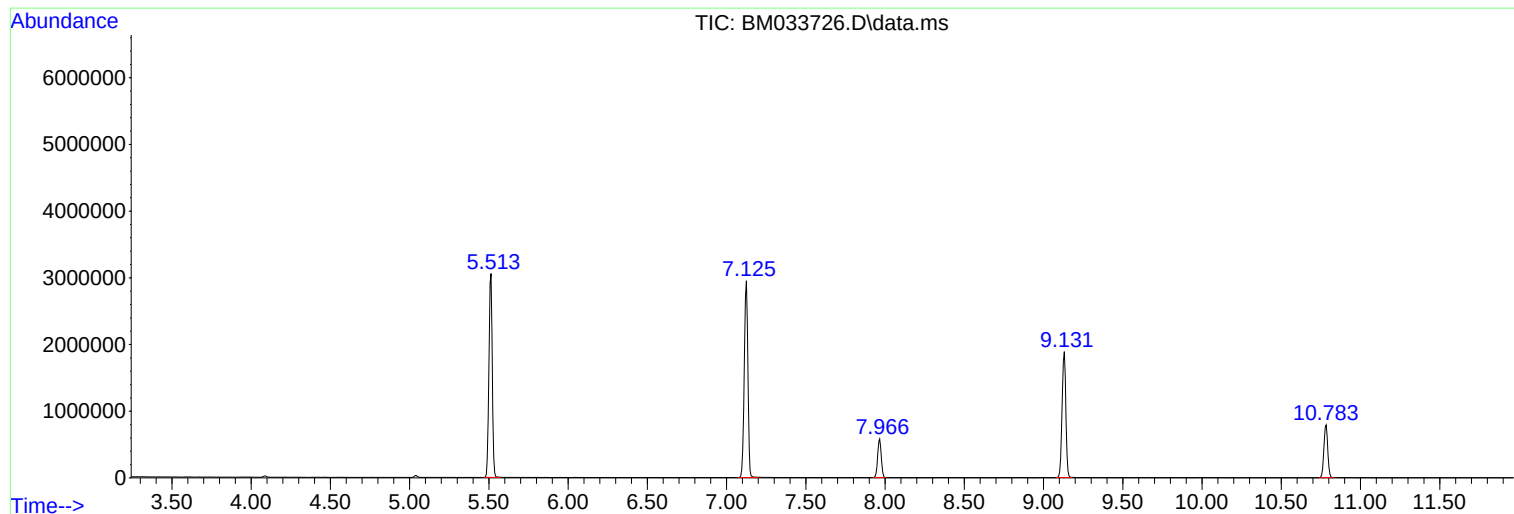

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011422\
Data File : BM033726.D
Acq On : 14 Jan 2022 13:59
Operator : CG/JU
Sample : PB142032BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142032BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011422\
Data File : BM033726.D
Acq On : 14 Jan 2022 13:59
Operator : CG/JU
Sample : PB142032BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142032BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------