

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011425\
 Data File : BM049344.D
 Acq On : 14 Jan 2025 10:05
 Operator : RC/JU
 Sample : PB166010BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK010

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	29	rVB	72407	84503	2.21%	0.191%
2	3.516	86	90	105	rBV	947660	1220428	31.92%	2.757%
3	3.822	138	142	150	rVB2	16435	25330	0.66%	0.057%
4	4.275	215	219	222	rBV6	4811	7337	0.19%	0.017%
5	6.716	627	634	652	rBV	871395	1349282	35.29%	3.048%
6	6.875	654	661	676	rVB	708310	1107307	28.96%	2.502%
7	7.063	687	693	706	rVB	922202	1391578	36.39%	3.144%
8	7.522	765	771	782	rBV	801811	1228792	32.13%	2.776%
9	8.234	885	892	905	rBV	986432	1551098	40.56%	3.504%
10	8.669	957	966	981	rBV	703117	1182723	30.93%	2.672%
11	9.380	1080	1087	1099	rBV	572410	921314	24.09%	2.082%
12	9.916	1171	1178	1197	rBV	894959	1550460	40.55%	3.503%
13	10.286	1232	1241	1252	rBV	995724	1616787	42.28%	3.653%
14	10.427	1257	1265	1292	rBV	663386	1330474	34.79%	3.006%
15	10.727	1312	1316	1318	rBV5	2925	3980	0.10%	0.009%
16	11.010	1362	1364	1372	rVB5	2785	6007	0.16%	0.014%
17	11.592	1458	1463	1464	rBV5	3390	4830	0.13%	0.011%
18	11.892	1509	1514	1525	rVB3	10727	31339	0.82%	0.071%
19	12.116	1549	1552	1556	rVB5	3772	3898	0.10%	0.009%
20	13.586	1794	1802	1811	rBV	1455656	2056460	53.78%	4.646%
21	13.851	1840	1847	1858	rBV	1854164	2619882	68.51%	5.919%
22	13.939	1861	1862	1868	rVB6	2646	3895	0.10%	0.009%
23	14.163	1891	1900	1911	rBV	1489322	2064899	54.00%	4.665%
24	14.392	1931	1939	1970	rBV2	240899	745039	19.48%	1.683%
25	15.033	2045	2048	2053	rVB6	3252	4825	0.13%	0.011%
26	15.162	2063	2070	2085	rBV	2288695	3211268	83.98%	7.255%
27	15.286	2085	2091	2107	rVV	493155	734425	19.21%	1.659%
28	15.404	2108	2111	2115	rVB5	8442	12824	0.34%	0.029%
29	15.739	2163	2168	2171	rBV6	2700	4433	0.12%	0.010%
30	16.439	2284	2287	2292	rBV6	2174	4458	0.12%	0.010%
31	16.580	2308	2311	2314	rBV3	3186	4146	0.11%	0.009%
32	16.698	2328	2331	2337	rVB4	6638	10467	0.27%	0.024%
33	16.804	2345	2349	2352	rBV7	2310	3935	0.10%	0.009%
34	16.915	2361	2368	2377	rBV	1702052	2335077	61.07%	5.276%
35	17.015	2378	2385	2399	rVB	2330452	3366921	88.05%	7.607%
36	17.139	2404	2406	2410	rVB5	3516	4794	0.13%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011425\
 Data File : BM049344.D
 Acq On : 14 Jan 2025 10:05
 Operator : RC/JU
 Sample : PB166010BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK010

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

37	17.656	2493	2494	2499	rVB5	3912	4903	0.13%	0.011%
38	17.839	2520	2525	2527	rBV4	11339	17992	0.47%	0.041%
39	18.056	2558	2562	2564	rBV4	2879	3855	0.10%	0.009%
40	18.880	2698	2702	2709	rVB3	23680	31789	0.83%	0.072%
41	18.950	2709	2714	2719	rBV	22824	34650	0.91%	0.078%
42	19.133	2741	2745	2751	rBV7	10949	19357	0.51%	0.044%
43	19.315	2771	2776	2787	rBV	2941885	3823885	100.00%	8.639%
44	20.356	2951	2953	2958	rVB3	26541	25311	0.66%	0.057%
45	21.144	3081	3087	3096	rBV	1711611	2347942	61.40%	5.305%
46	23.738	3520	3528	3542	rVB	1704172	3584607	93.74%	8.099%
47	23.927	3552	3560	3578	rVB	1055567	2561758	66.99%	5.788%




Sum of corrected areas: 44261264

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011425\
Data File : BM049344.D
Acq On : 14 Jan 2025 10:05
Operator : RC/JU
Sample : PB166010BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK010

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

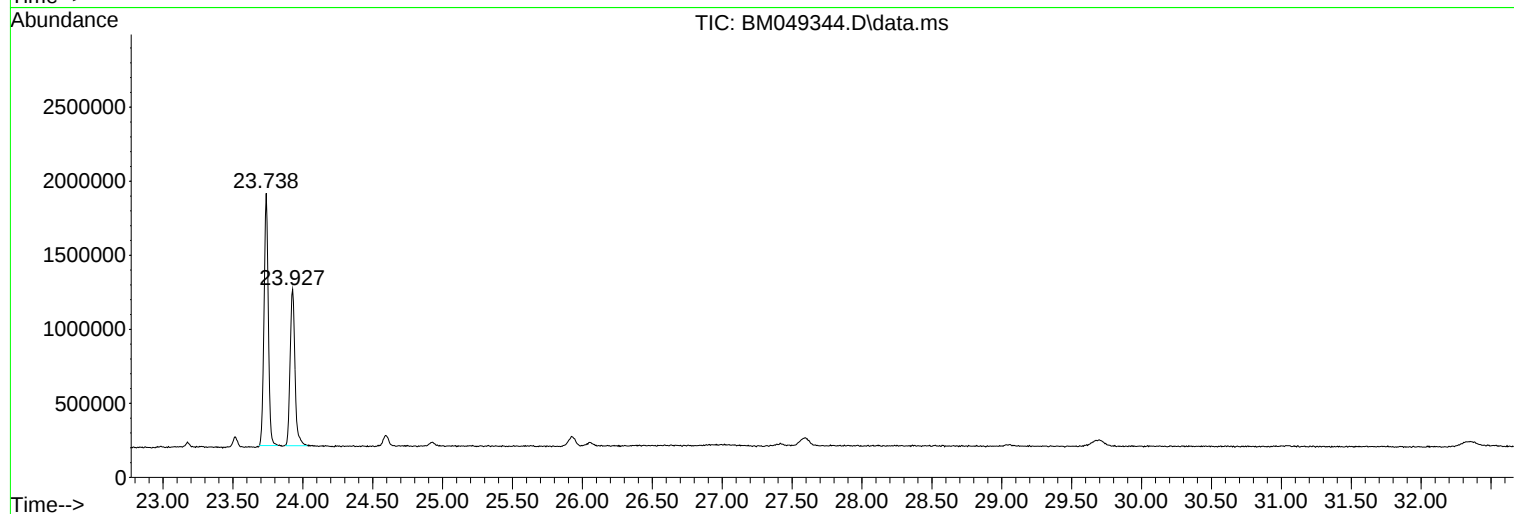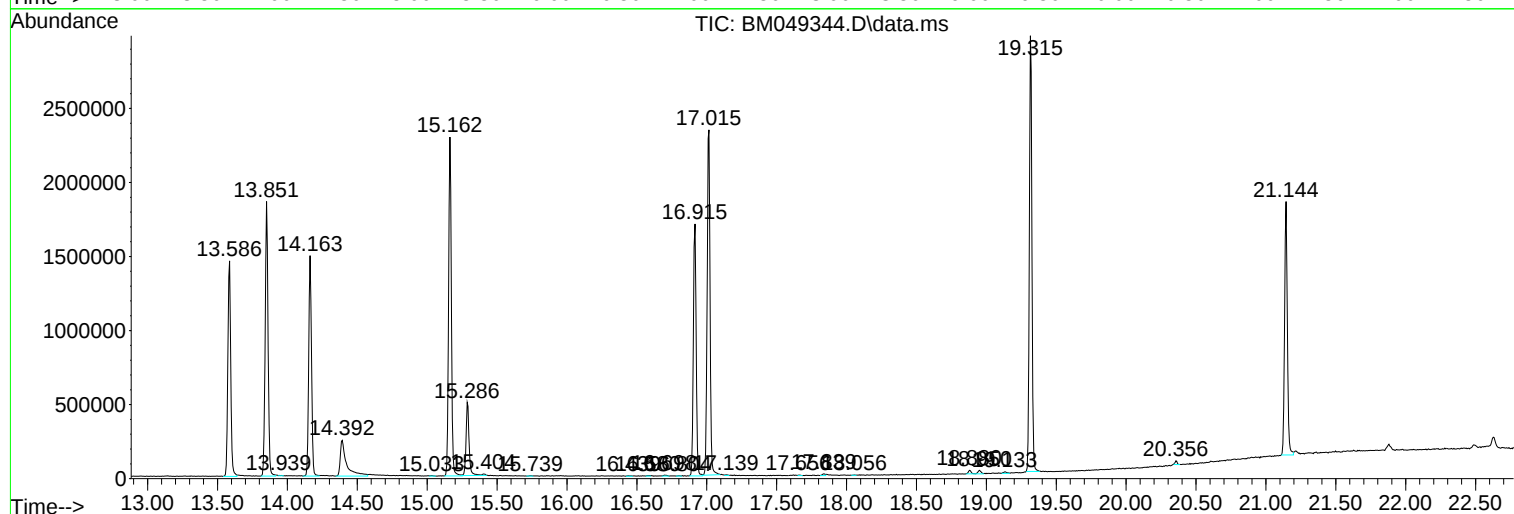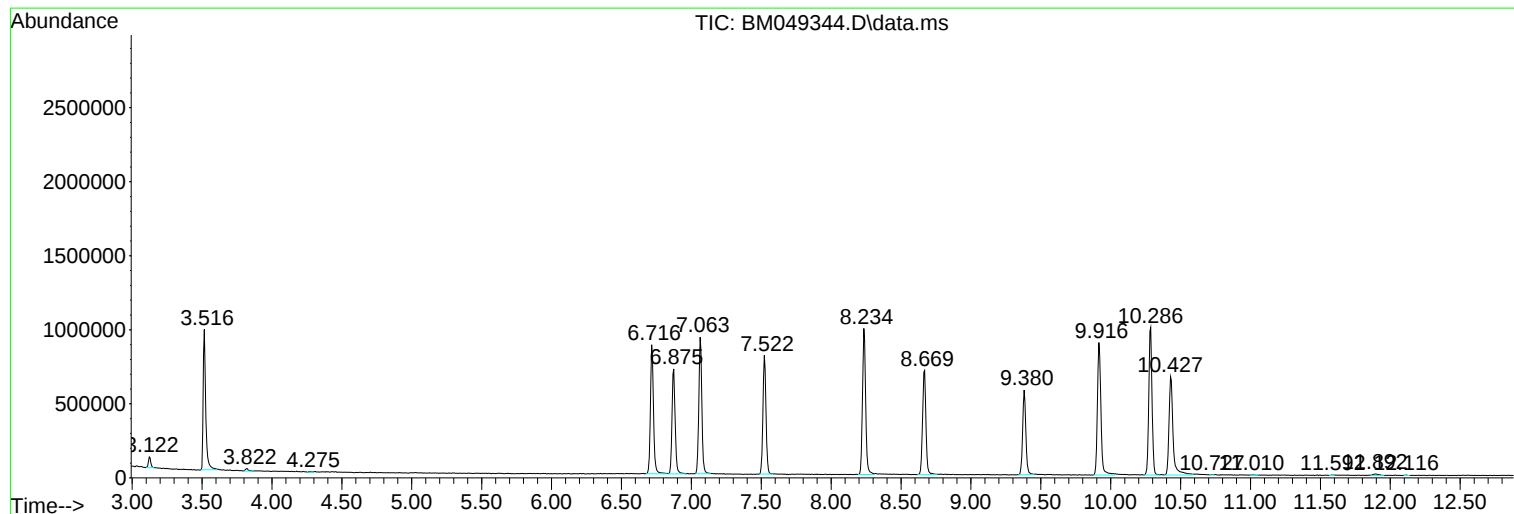

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011425\
Data File : BM049344.D
Acq On : 14 Jan 2025 10:05
Operator : RC/JU
Sample : PB166010BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK010

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011425\
Data File : BM049344.D
Acq On : 14 Jan 2025 10:05
Operator : RC/JU
Sample : PB166010BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK010

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc