

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011425\
 Data File : BM049345.D
 Acq On : 14 Jan 2025 10:44
 Operator : RC/JU
 Sample : Q1006-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM049345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.822	139	142	148	rVB2	12646	15969	0.78%	0.155%
2	4.540	262	264	267	rBV3	3769	3147	0.15%	0.031%
3	4.934	329	331	335	rVB5	4079	4844	0.24%	0.047%
4	6.687	627	629	633	rBV4	2562	3124	0.15%	0.030%
5	6.945	671	673	676	rBV3	3034	2098	0.10%	0.020%
6	6.981	678	679	682	rVB3	2431	2142	0.10%	0.021%
7	7.034	684	688	690	rBV5	3293	3754	0.18%	0.036%
8	7.093	696	698	701	rVB4	2197	2056	0.10%	0.020%
9	7.410	751	752	755	rVB3	2695	2532	0.12%	0.025%
10	7.440	755	757	762	rVB6	3840	4914	0.24%	0.048%
11	7.522	762	771	786	rBV	651834	1062010	51.79%	10.294%
12	7.692	797	800	801	rBV3	2291	2064	0.10%	0.020%
13	7.816	819	821	823	rVB2	2979	2655	0.13%	0.026%
14	7.940	840	842	844	rBV3	2182	2993	0.15%	0.029%
15	7.975	846	848	851	rVV4	3423	2267	0.11%	0.022%
16	8.734	975	977	980	rVB4	3428	2212	0.11%	0.021%
17	8.792	983	987	988	rBV3	1926	2328	0.11%	0.023%
18	9.634	1126	1130	1134	rBV5	2214	3004	0.15%	0.029%
19	9.822	1159	1162	1165	rVB4	2006	2631	0.13%	0.026%
20	9.851	1165	1167	1170	rBV2	3145	3225	0.16%	0.031%
21	10.139	1214	1216	1220	rVB5	2143	2531	0.12%	0.025%
22	10.286	1233	1241	1254	rBV	772127	1366364	66.64%	13.244%
23	10.422	1261	1264	1267	rVB5	4059	3860	0.19%	0.037%
24	10.916	1345	1348	1350	rVV4	1922	2121	0.10%	0.021%
25	10.933	1350	1351	1354	rVB3	2644	2421	0.12%	0.023%
26	11.086	1374	1377	1378	rVB3	3165	2405	0.12%	0.023%
27	11.245	1402	1404	1406	rBV3	1743	2125	0.10%	0.021%
28	11.492	1443	1446	1449	rVV6	2346	3129	0.15%	0.030%
29	11.733	1485	1487	1492	rVB5	2336	3152	0.15%	0.031%
30	11.775	1492	1494	1496	rBV2	2552	2495	0.12%	0.024%
31	11.810	1496	1500	1501	rVV4	2189	2774	0.14%	0.027%
32	11.910	1514	1517	1520	rVB4	2257	2580	0.13%	0.025%
33	12.133	1553	1555	1558	rVB4	2012	2412	0.12%	0.023%
34	12.180	1558	1563	1567	rBV7	2216	4237	0.21%	0.041%
35	12.492	1613	1616	1619	rBV4	1663	2503	0.12%	0.024%
36	12.680	1645	1648	1652	rVB6	2309	3496	0.17%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011425\
 Data File : BM049345.D
 Acq On : 14 Jan 2025 10:44
 Operator : RC/JU
 Sample : Q1006-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
 Title : SVOA CALIBRATION

37	12.857	1675	1678	1681	rBV5	1784	2186	0.11%	0.021%
38	12.939	1689	1692	1696	rBV5	1600	2709	0.13%	0.026%
39	12.998	1701	1702	1707	rVB5	2152	2832	0.14%	0.027%
40	13.098	1718	1719	1724	rBV4	1468	2334	0.11%	0.023%
41	13.492	1783	1786	1789	rBV3	2194	2389	0.12%	0.023%
42	13.592	1800	1803	1806	rBV4	2149	2674	0.13%	0.026%
43	13.621	1806	1808	1812	rVV5	2082	2859	0.14%	0.028%
44	13.733	1824	1827	1831	rVB5	2184	2728	0.13%	0.026%
45	13.780	1834	1835	1838	rVB3	2920	2428	0.12%	0.024%
46	13.880	1847	1852	1854	rBV6	2520	3025	0.15%	0.029%
47	14.098	1886	1889	1893	rBV5	1729	2289	0.11%	0.022%
48	14.163	1893	1900	1914	rBV	1255018	1860322	90.73%	18.032%
49	14.645	1979	1982	1989	rVB9	1809	3450	0.17%	0.033%
50	14.727	1993	1996	1998	rVB2	2280	2144	0.10%	0.021%
51	14.904	2022	2026	2027	rBV3	2027	2062	0.10%	0.020%
52	14.974	2035	2038	2042	rBV5	2216	3753	0.18%	0.036%
53	15.021	2042	2046	2048	rVV4	1990	2554	0.12%	0.025%
54	15.104	2056	2060	2061	rBV4	1971	2132	0.10%	0.021%
55	15.763	2169	2172	2174	rBV4	2191	2674	0.13%	0.026%
56	15.839	2181	2185	2186	rBV3	2729	2261	0.11%	0.022%
57	15.945	2198	2203	2204	rBV5	1923	2722	0.13%	0.026%
58	16.410	2278	2282	2285	rBV6	1633	2362	0.12%	0.023%
59	16.451	2285	2289	2290	rVB4	2684	2506	0.12%	0.024%
60	16.533	2301	2303	2305	rBV3	2090	2150	0.10%	0.021%
61	16.568	2307	2309	2313	rVB4	1696	2060	0.10%	0.020%
62	16.604	2313	2315	2318	rBV4	1693	2291	0.11%	0.022%
63	16.704	2327	2332	2336	rBV5	4940	8046	0.39%	0.078%
64	16.845	2352	2356	2358	rBV4	2247	2183	0.11%	0.021%
65	16.915	2359	2368	2384	rBV	1348101	2050473	100.00%	19.875%
66	17.186	2411	2414	2416	rBV4	2036	2302	0.11%	0.022%
67	17.239	2421	2423	2426	rVB4	2937	3027	0.15%	0.029%
68	17.786	2512	2516	2519	rBV6	2712	4190	0.20%	0.041%
69	17.874	2524	2531	2532	rVV5	3403	6333	0.31%	0.061%
70	17.909	2535	2537	2538	rVB	3347	2304	0.11%	0.022%
71	18.351	2607	2612	2613	rBV5	2861	3224	0.16%	0.031%
72	18.362	2613	2614	2620	rVB6	2677	2671	0.13%	0.026%
73	18.439	2623	2627	2628	rBV4	2997	3816	0.19%	0.037%
74	19.109	2739	2741	2743	rBV2	2749	3046	0.15%	0.030%
75	21.145	3081	3087	3096	rBV	1429100	1931464	94.20%	18.721%
76	23.927	3552	3560	3575	rBV2	759301	1831326	89.31%	17.751%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011425\
Data File : BM049345.D
Acq On : 14 Jan 2025 10:44
Operator : RC/JU
Sample : Q1006-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 10316875

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011425\
Data File : BM049345.D
Acq On : 14 Jan 2025 10:44
Operator : RC/JU
Sample : Q1006-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

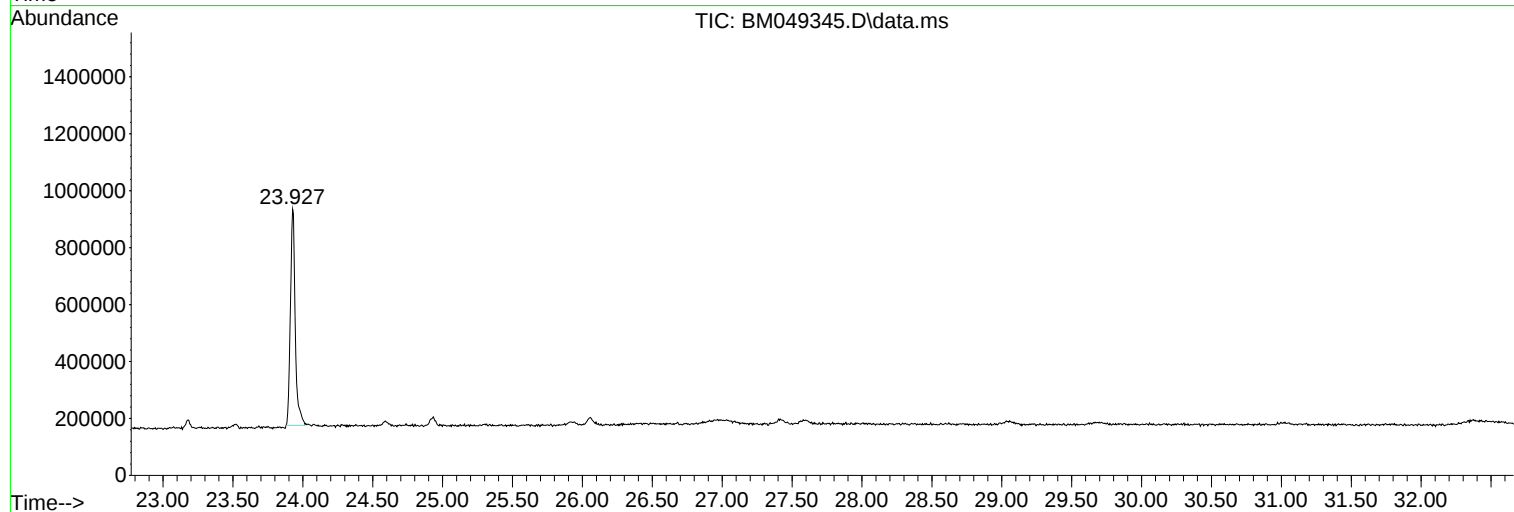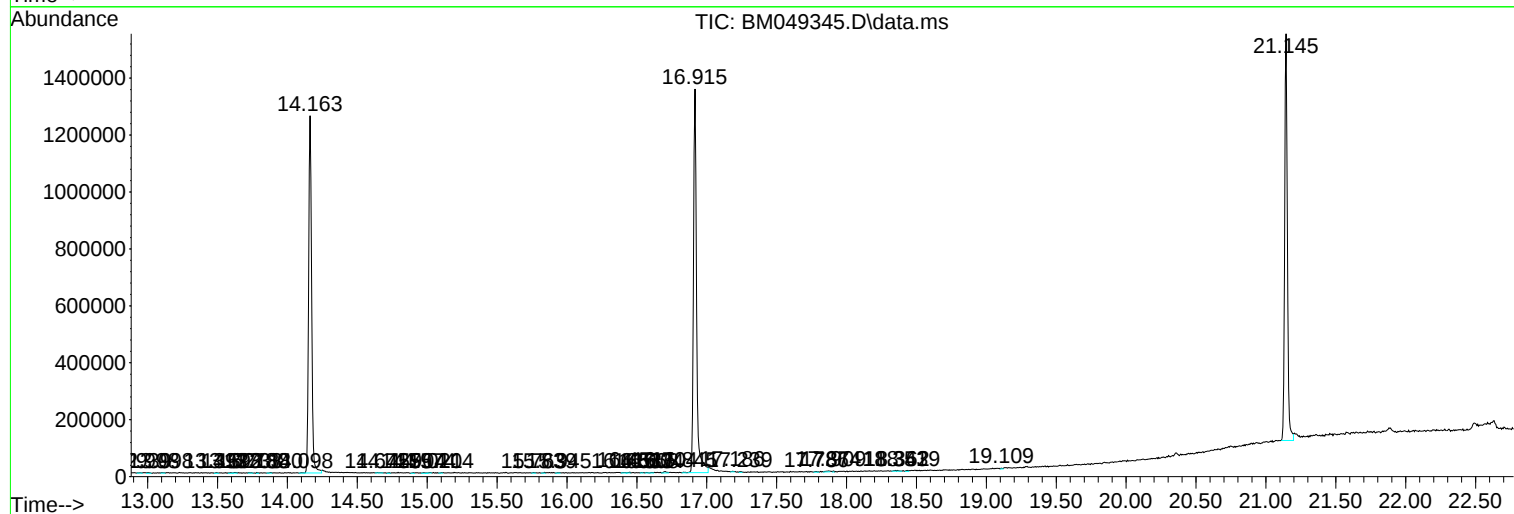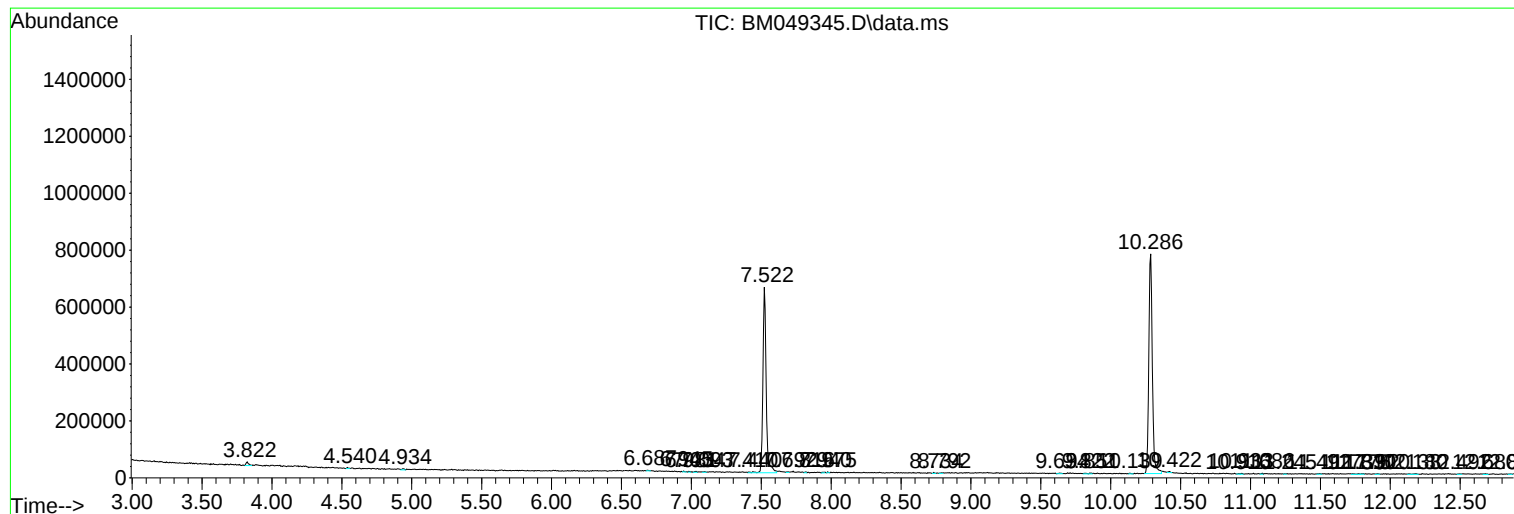

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011425\
Data File : BM049345.D
Acq On : 14 Jan 2025 10:44
Operator : RC/JU
Sample : Q1006-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011425\
Data File : BM049345.D
Acq On : 14 Jan 2025 10:44
Operator : RC/JU
Sample : Q1006-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM011325.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc