
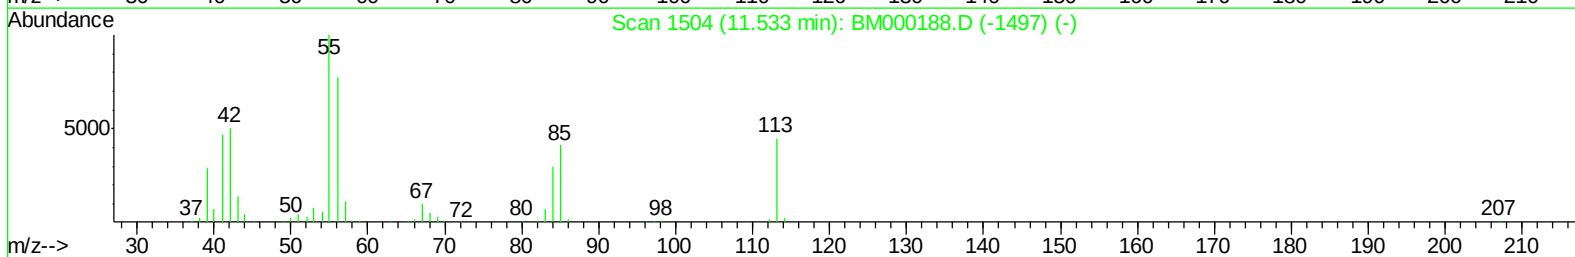
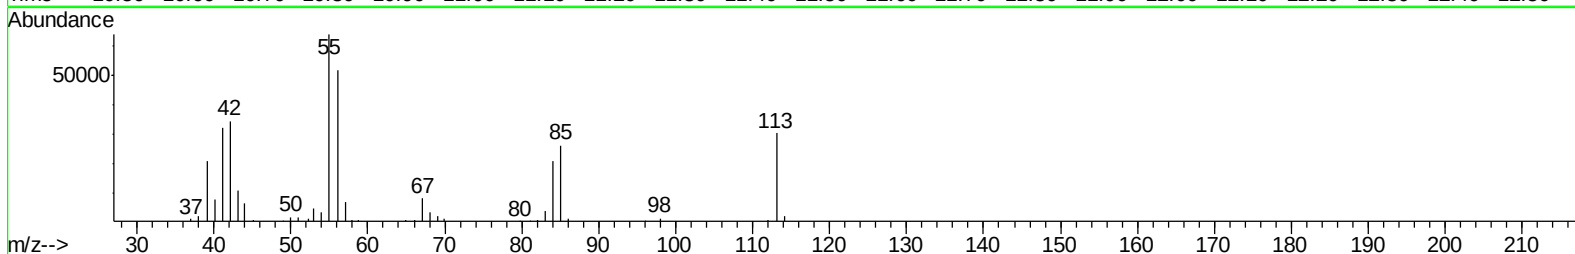


Data Path : Z:\HPCHEM1\BNA_M\Data\BM011515\
Data File : BM000198.D
Acq On : 15 Jan 2015 10:19
Operator : TP/IZ
Sample : SSTD02031
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jan 16 02:30:11 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 14 12:47:10 2015
Response via : Initial Calibration

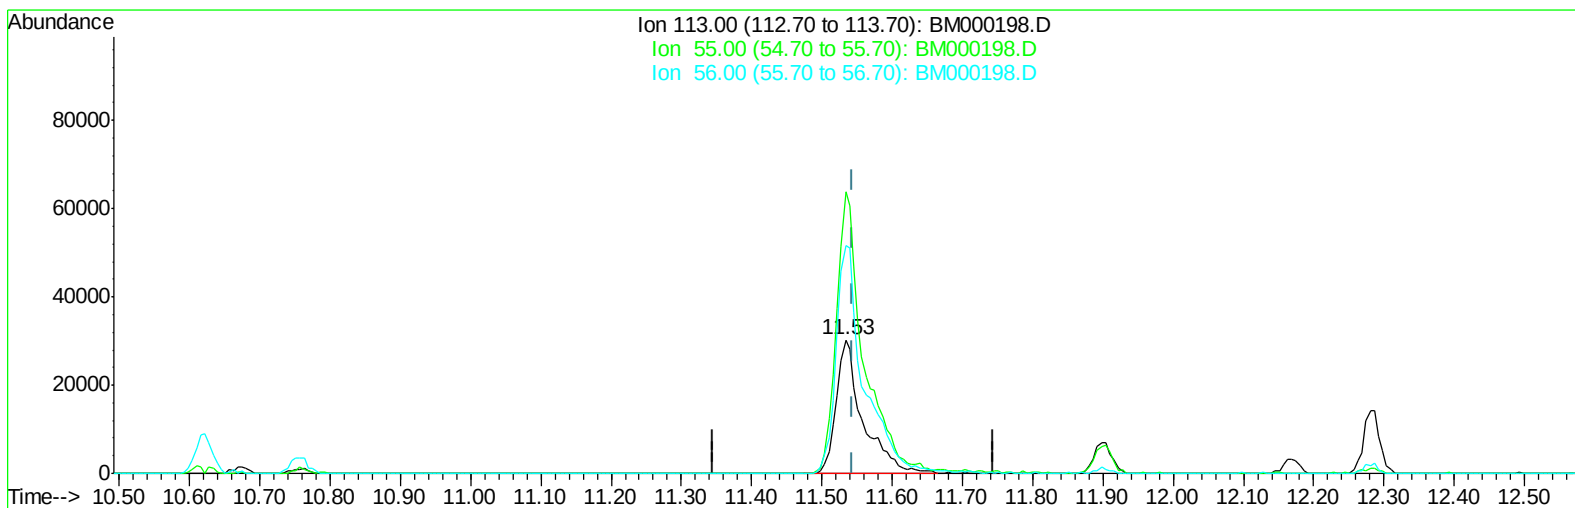

TIC: BM000198.D

(32) Caprolactam

11.533min (-0.012) 18.52ng/ul m

response 79568

Ion	Exp%	Act%
113.00	100	100
55.00	195.70	211.06
56.00	157.90	171.08
0.00	0.00	0.00