

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011515\
 Data File : BM000201.D
 Acq On : 15 Jan 2015 15:44
 Operator : TP/IZ
 Sample : G1063-01RX
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AJ7RX

Quant Time: Jan 16 02:41:51 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 16 02:28:09 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	140831	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	567489	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	383513	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	784120	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	902203	20.00	ng/ul	0.00
83) Perylene-d12	23.69	264	863526	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	2806	1.16	ng/uL	0.00
5) Phenol-d5	6.99	99	39341	3.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	115735	15.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	105117	12.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	65580	6.96	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	60457	15.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	64524	16.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	121361	13.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	3162	0.31	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	481635	17.03	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	511711	15.10	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	11026	2.40	ng/ul	0.00
57) Fluorene-d10	15.46	176	431944	17.78	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	55521	14.94	ng/ul	0.00
70) Anthracene-d10	17.30	188	668468	18.44	ng/ul	0.00
76) Pyrene-d10	19.60	212	787056	18.91	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.54	264	706236	18.02	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.35	88	3939	1.17	ng/uL	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011515\
Data File : BM000201.D
Acq On : 15 Jan 2015 15:44
Operator : TP/IZ
Sample : G1063-01RX
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AJ7RX

Quant Time: Jan 16 02:41:51 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 16 02:28:09 2015
Response via : Initial Calibration

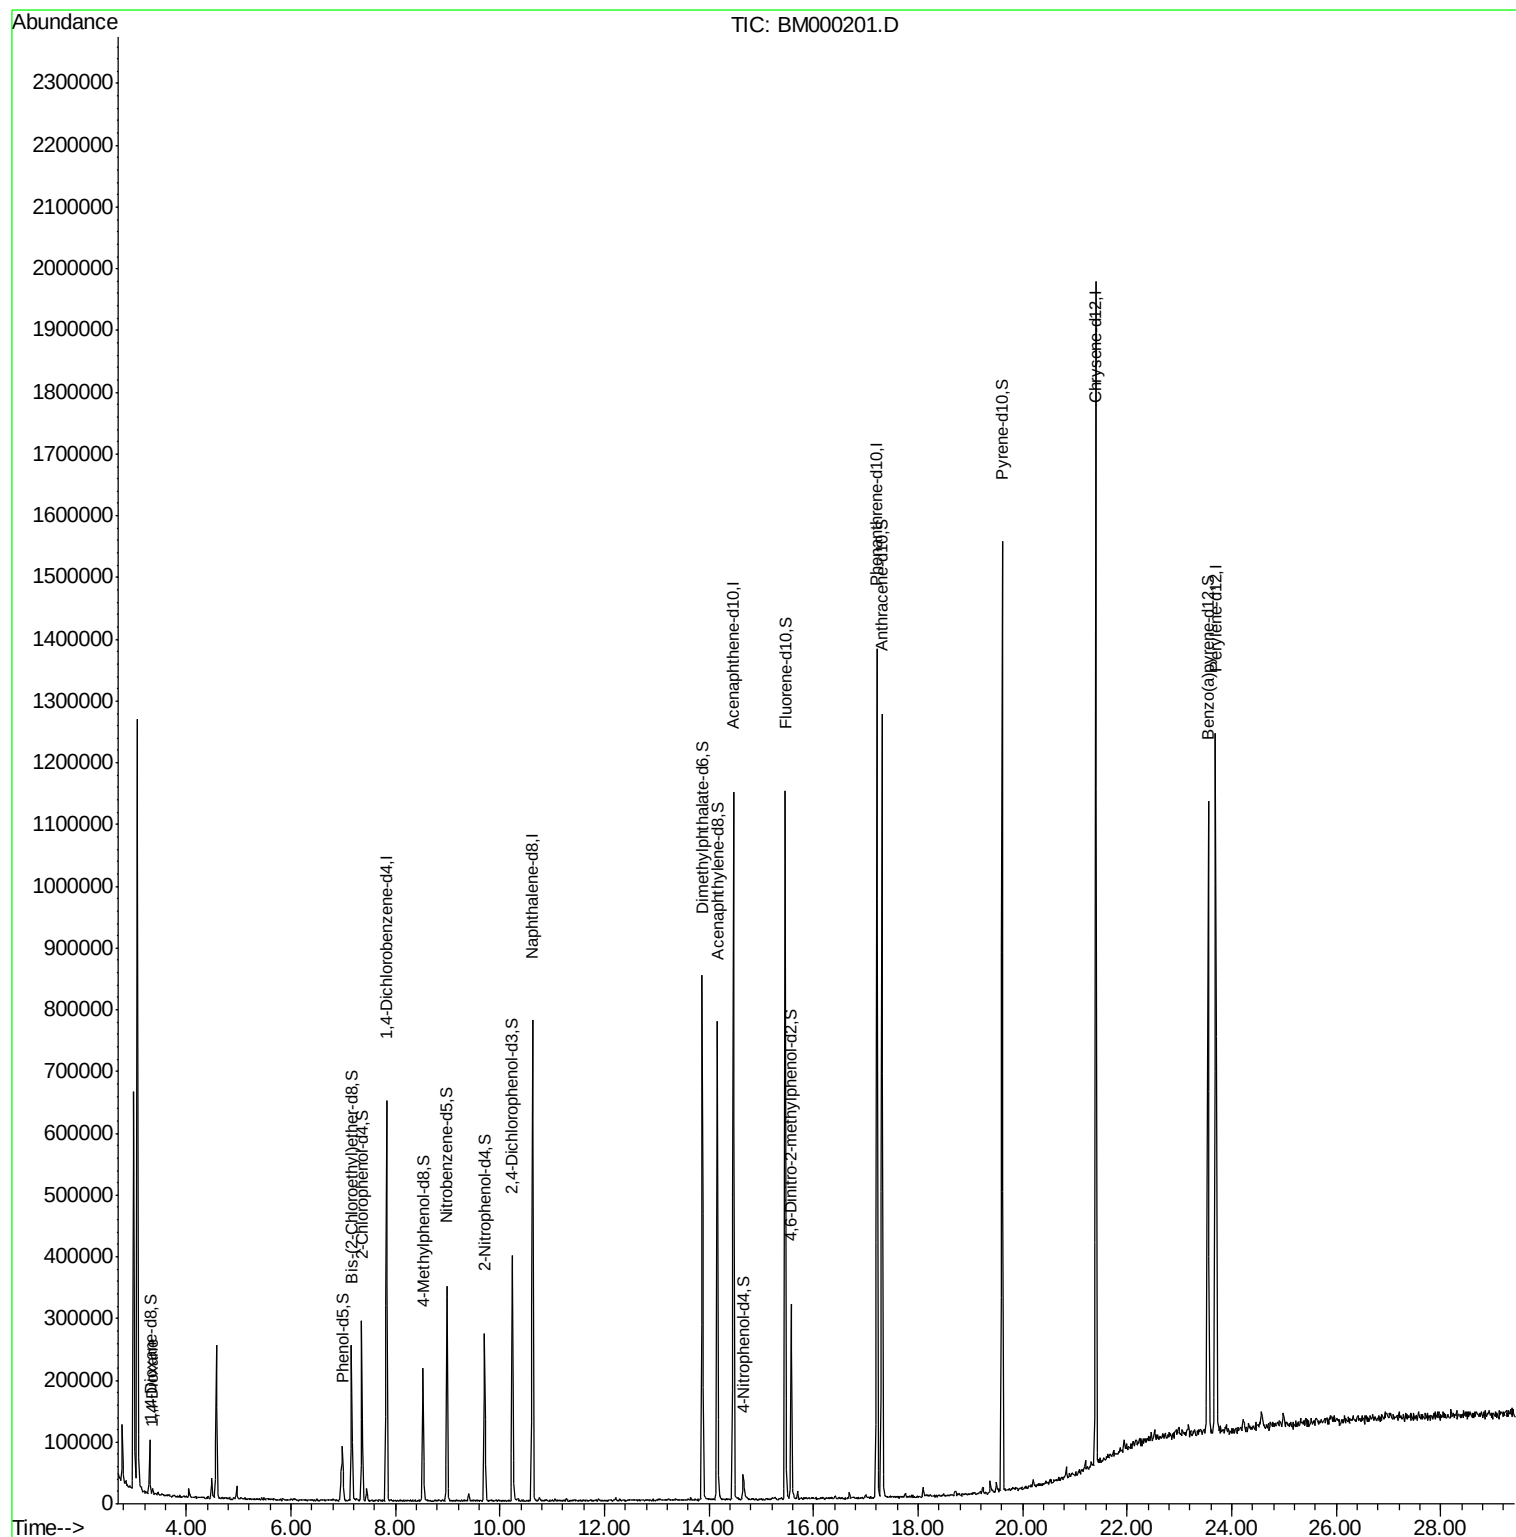

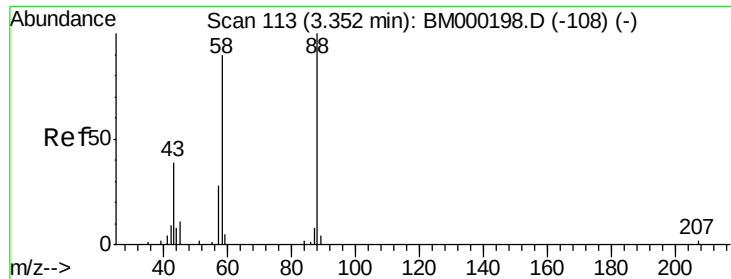

#2

1,4-Dioxane

Concen: 1.17 ng/uL

RT: 3.35 min Scan# 113

Delta R.T. 0.00 min

Lab File: BM000201.D

Acq: 15 Jan 2015 15:44

Instrument :

BNA_M

ClientSampleId :

C0AJ7RX


Tgt Ion: 88 Resp: 3939

Ion Ratio Lower Upper

88 100

43 42.9 34.9 52.3

58 76.8 67.3 100.9

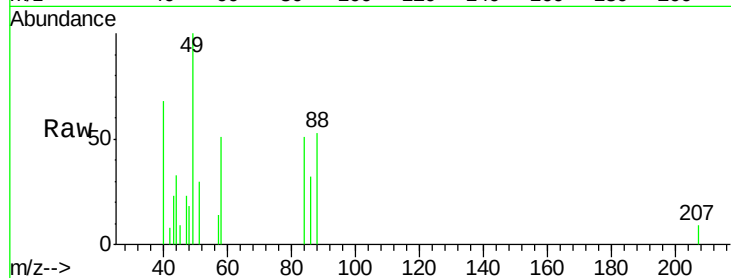

Abundance Ion 88.00 (87.70 to 88.70): BM000201.D (-28) (-)

Ion 43.00 (42.70 to 43.70): BM000201.D (-28) (-)

Ion 58.00 (57.70 to 58.70): BM000201.D (-28) (-)

