

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011515\
 Data File : BM000216.D
 Acq On : 16 Jan 2015 01:14
 Operator : TP/IZ
 Sample : G1065-03RX
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE3RX

Quant Time: Jan 16 04:41:50 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 16 04:15:33 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	138912	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	567646	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	396284	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	811972	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	925602	20.00	ng/ul	0.00
83) Perylene-d12	23.69	264	881374	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	2424	1.01	ng/uL	0.00
5) Phenol-d5	6.99	99	60992	5.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	179403	24.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	167120	19.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	106502	11.46	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	95199	24.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	106234	26.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	182004	20.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	259	0.03	ng/ul	0.01
43) Dimethylphthalate-d6	13.87	166	748344	25.60	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	837023	23.90	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	18352	3.86	ng/ul	0.00
57) Fluorene-d10	15.46	176	648298	25.83	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	87987	22.87	ng/ul	0.00
70) Anthracene-d10	17.30	188	1004680	26.76	ng/ul	0.00
76) Pyrene-d10	19.60	212	1138785	26.67	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.54	264	1017439	25.43	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.87	165	5673	1.09	ng/ul#	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011515\
Data File : BM000216.D
Acq On : 16 Jan 2015 01:14
Operator : TP/IZ
Sample : G1065-03RX
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE3RX

Quant Time: Jan 16 04:41:50 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 16 04:15:33 2015
Response via : Initial Calibration

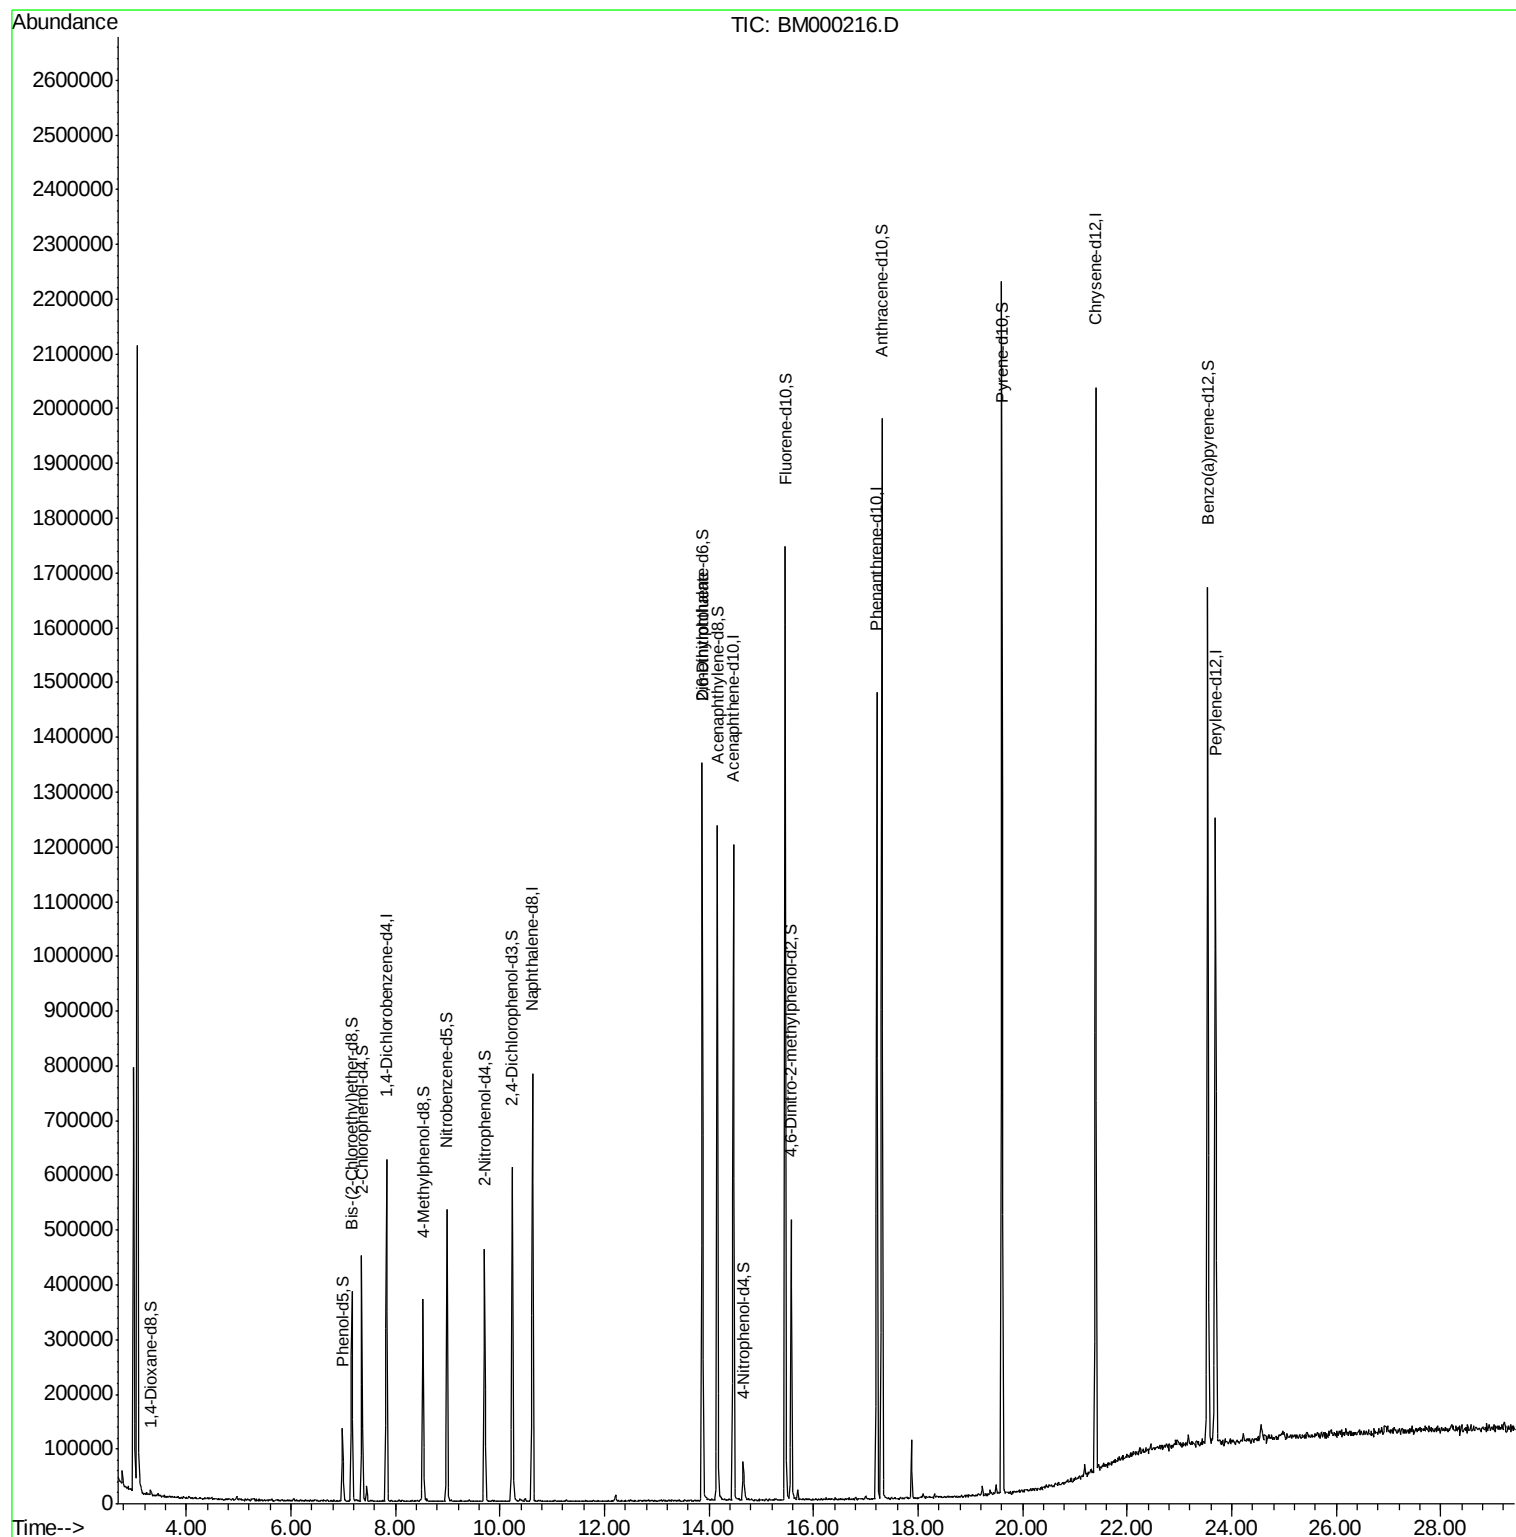

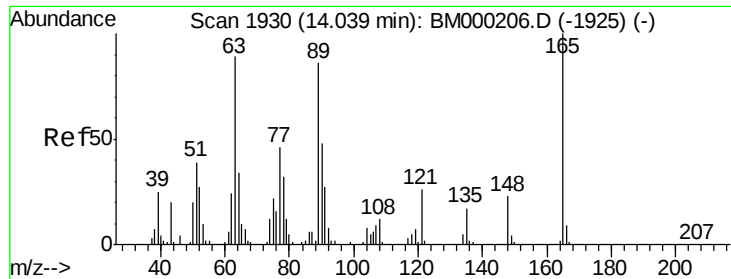

#45

2,6-Dinitrotoluene

Concen: 1.09 ng/ul

RT: 13.87 min Scan# 1901

Delta R.T. -0.17 min

Lab File: BM000216.D


Acq: 16 Jan 2015 01:14

Instrument :

BNA_M

ClientSampleId :

C0AE3RX

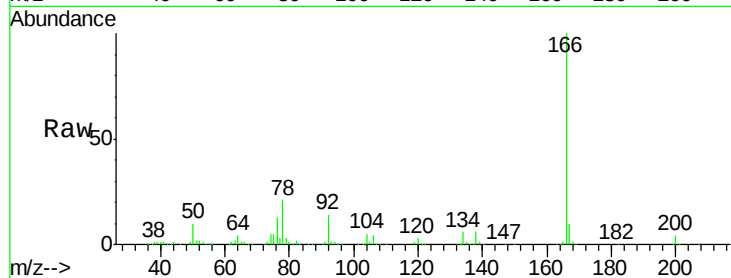

Tgt Ion:	165	Resp:	5673
Ion	Ratio	Lower	Upper
165	100		
89	0.0	54.4	81.6#
121	36.2	18.6	28.0#

