

Data Path : Z:\HPCHEM1\BNA_M\Data\BM011515\
 Data File : BM000226.D
 Acq On : 16 Jan 2015 07:45
 Operator : TP/IZ
 Sample : PB81361BL
 Misc : SBLK96
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK96

Quant Time: Jan 16 10:35:18 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 14 12:47:10 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	140646	20.00	ng/ul	-0.03
18) Naphthalene-d8	10.62	136	584424	20.00	ng/ul	-0.03
35) Acenaphthene-d10	14.46	164	404526	20.00	ng/ul	-0.02
61) Phenanthrene-d10	17.20	188	829478	20.00	ng/ul	-0.02
75) Chrysene-d12	21.39	240	949669	20.00	ng/ul	-0.02
83) Perylene-d12	23.68	264	847281	20.00	ng/ul	-0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	13340	5.50	ng/uL	-0.01
5) Phenol-d5	6.99	99	316298	26.73	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	7.16	67	212718	28.44	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.36	132	240797	27.76	ng/ul	-0.02
13) 4-Methylphenol-d8	8.52	113	241733	25.68	ng/ul	-0.02
19) Nitrobenzene-d5	8.98	128	112606	27.86	ng/ul	-0.03
22) 2-Nitrophenol-d4	9.70	143	120188	29.13	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.23	165	231832	25.43	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.75	131	122700	11.86	ng/ul	-0.03
43) Dimethylphthalate-d6	13.87	166	802401	26.89	ng/ul	-0.02
46) Acenaphthylene-d8	14.16	160	966440	27.04	ng/ul	-0.02
51) 4-Nitrophenol-d4	14.65	143	108926	22.43	ng/ul	-0.01
57) Fluorene-d10	15.46	176	697835	27.24	ng/ul	-0.02
62) 4,6-Dinitro-2-methylphenol	15.57	200	101585	25.84	ng/ul	-0.02
70) Anthracene-d10	17.30	188	1068923	27.87	ng/ul	-0.01
76) Pyrene-d10	19.60	212	1187467	27.11	ng/ul	-0.02
87) Benzo(a)pyrene-d12	23.53	264	1073607	27.92	ng/ul	-0.04


Target Compounds					Qvalue
45) 2,6-Dinitrotoluene	13.87	165	5479	1.03 ng/ul#	32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM011515\
Data File : BM000226.D
Acq On : 16 Jan 2015 07:45
Operator : TP/IZ
Sample : PB81361BL
Misc : SBLK96
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK96

Quant Time: Jan 16 10:35:18 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 14 12:47:10 2015
Response via : Initial Calibration

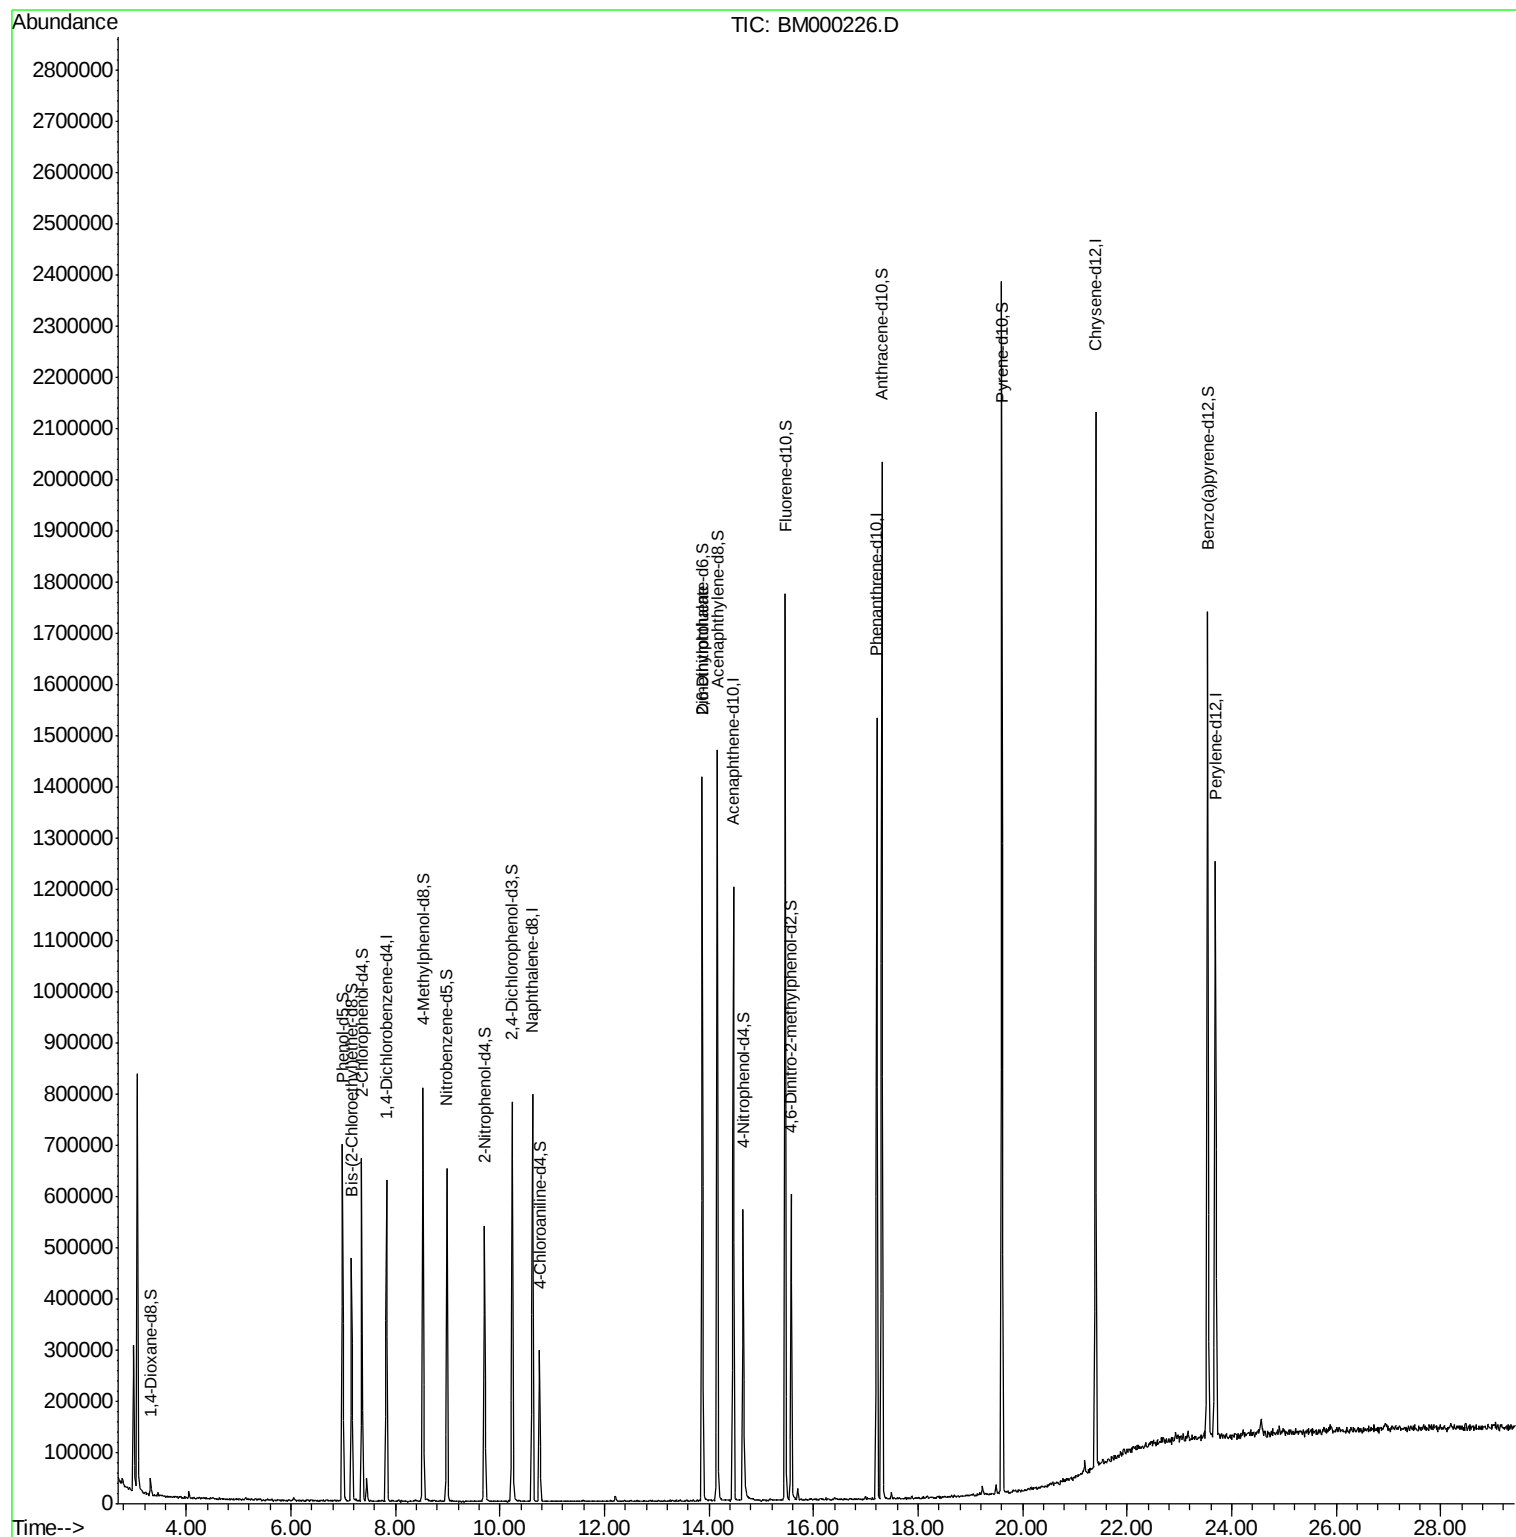

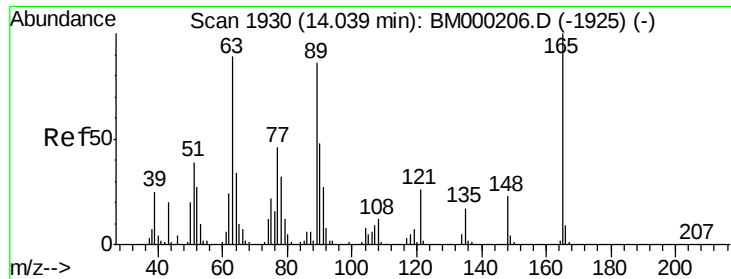

#45

2,6-Dinitrotoluene

Concen: 1.03 ng/ul

RT: 13.87 min Scan# 1901

Delta R.T. -0.19 min

Lab File: BM000226.D


Acq: 16 Jan 2015 07:45

Instrument :

BNA_M

ClientSampleId :

SBLK96

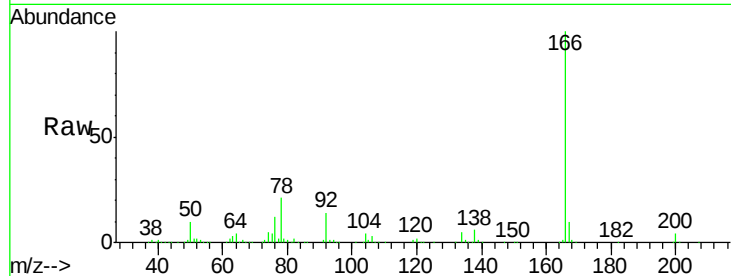

Tgt Ion:	165	Resp:	5479
Ion Ratio	Lower	Upper	
165	100		
89	0.0	54.4	81.6#
121	32.8	18.6	28.0#

