

(QT Reviewed)


```
Data Path   : Z:\HPCHEM1\BNA_M\Data\BM011515\  
Data File  : BM000205.D  
Acq On     : 15 Jan 2015   18:07  
Operator   : TP/IZ  
Sample     : G1063-05RX  
Misc       :  
ALS Vial   : 9      Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
C0AN1RX

Manual Integrations

TEJASKUMAR
1/16/2015 6:24:05 PM

Quant Time: Jan 16 12:17:28 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 14 12:47:10 2015
Response via : Initial Calibration

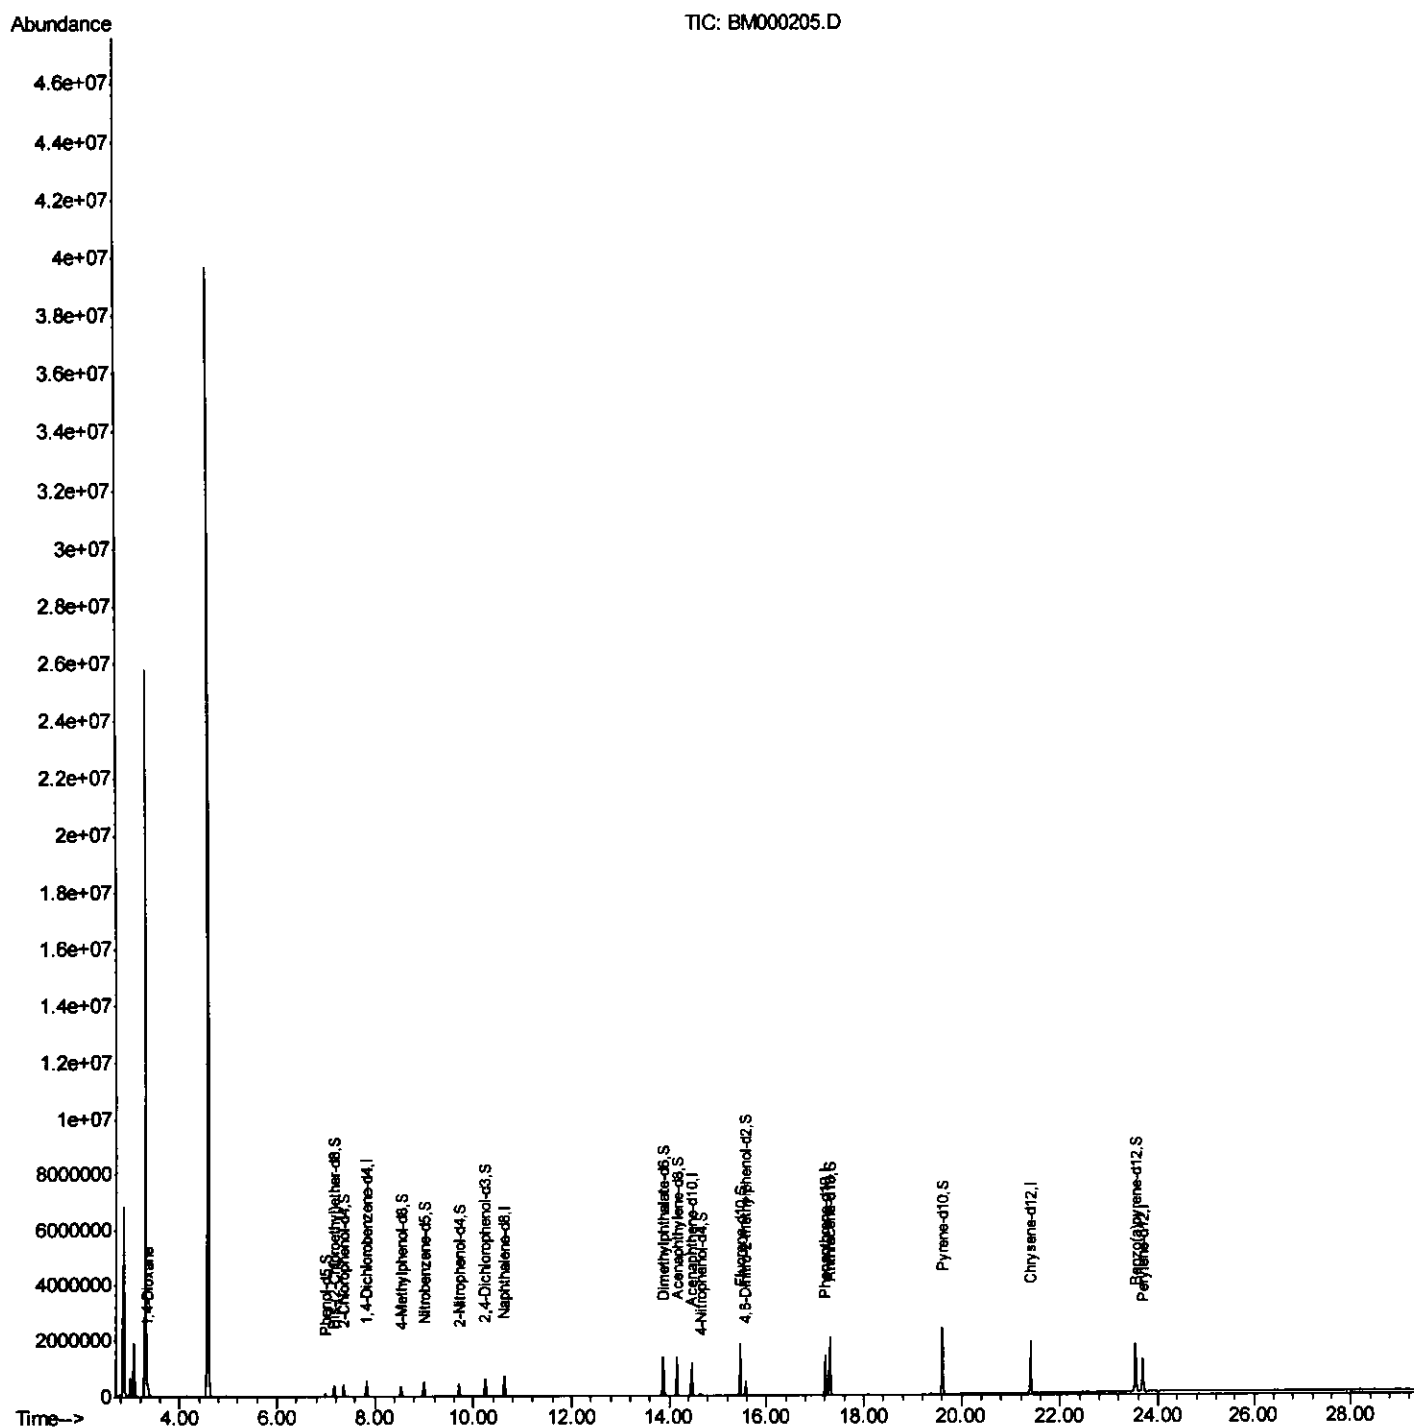

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM011515\
Data File : BM000205.D
Acq On : 15 Jan 2015 18:07
Operator : TP/IZ
Sample : G1063-05RX
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Jan 16 12:15:33 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 14 12:47:10 2015
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
COAN1RX

Manual Integrations
APPROVED

TEJASKUMAR
1/16/2015 6:24:05 PM

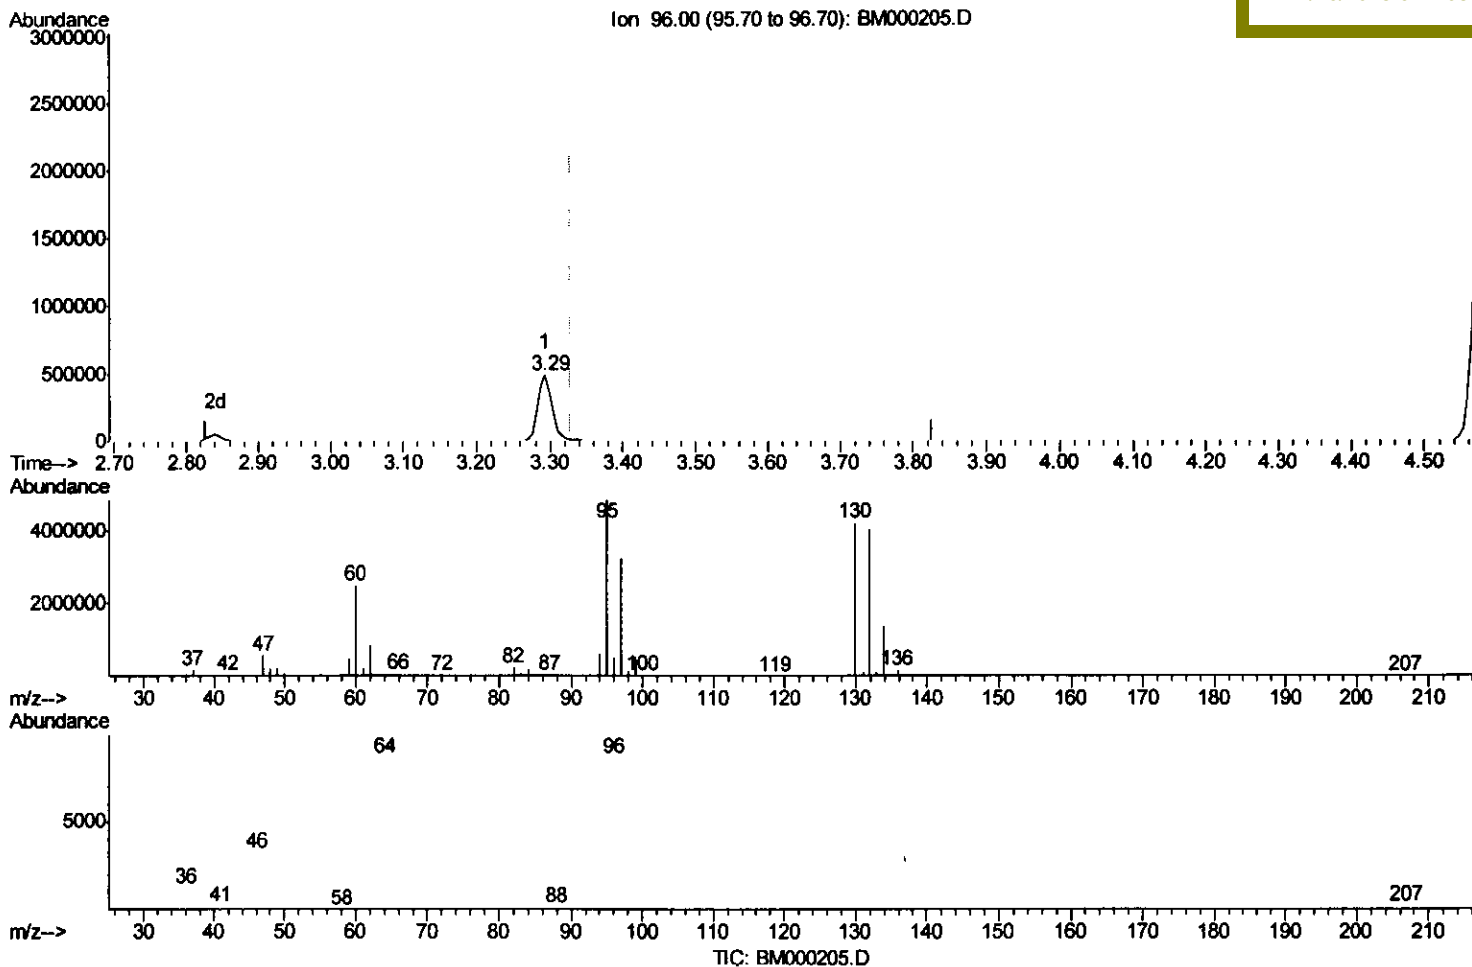

(3) 1,4-Dioxane-d8 (S)

3.293min (-0.034) 285.31ng/uL

response 659807

Ion	Exp%	Act%
96.00	100	100
64.00	82.60	0.06#
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM011515\
 Data File : BM000205.D
 Acq On : 15 Jan 2015 18:07
 Operator : TP/IZ
 Sample : G1063-05RX
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAN1RX

Manual Integrations
 APPROVED

TEJASKUMAR
 1/16/2015 6:24:05 PM

Quant Time: Jan 16 12:15:33 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 14 12:47:10 2015
 Response via : Initial Calibration

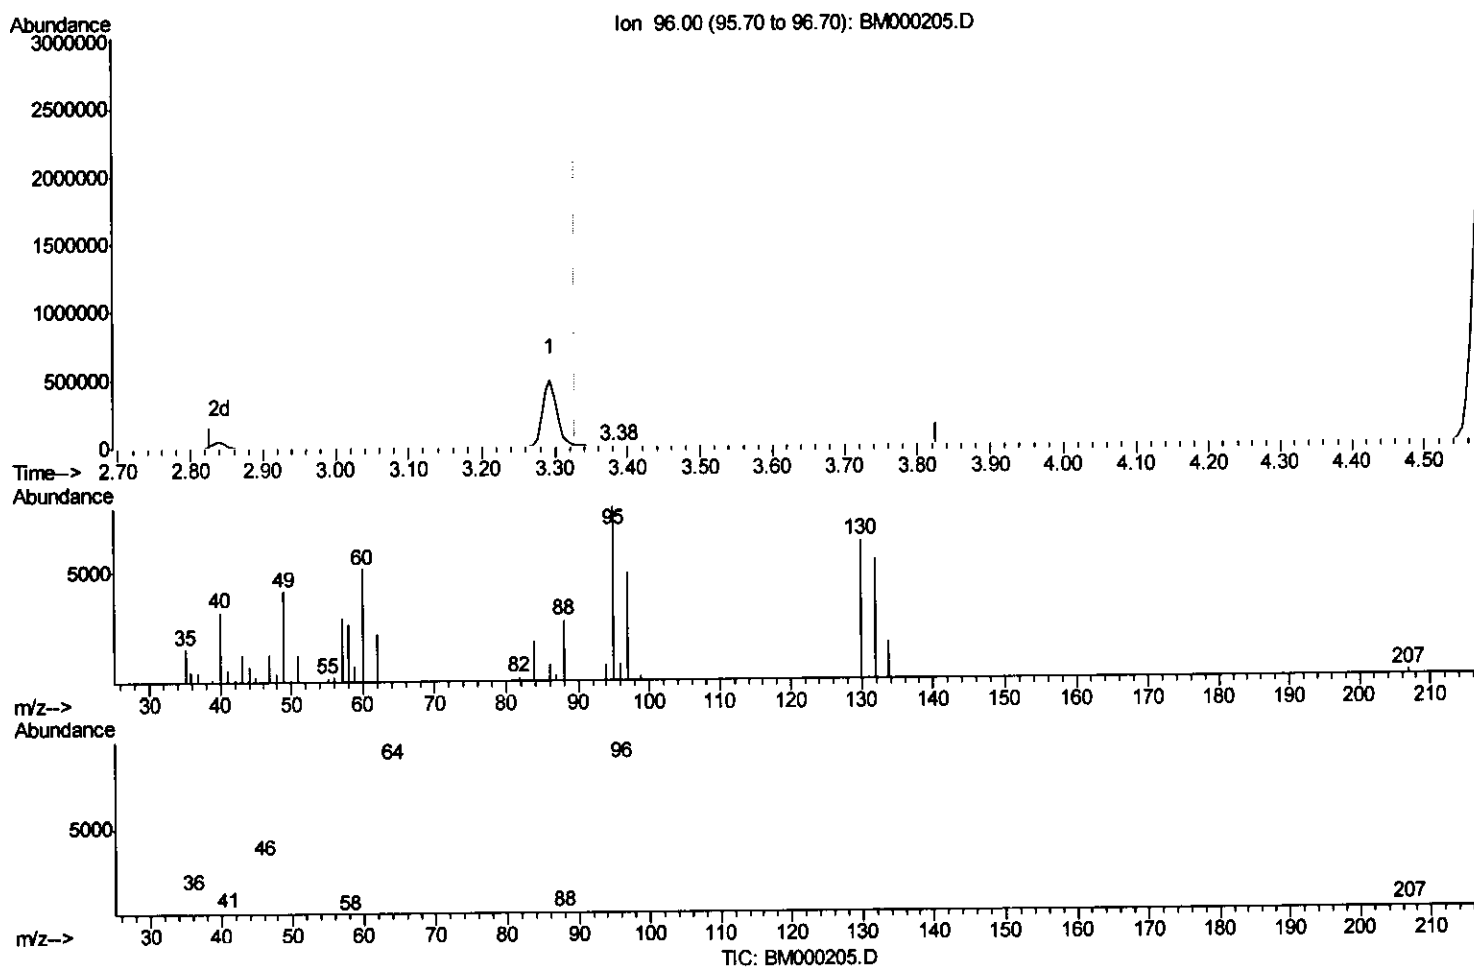

(3) 1,4-Dioxane-d8 (S)

3.381min (+0.054) 0.34ng/uL m

response 777

Ion	Exp%	Act%
96.00	100	100
64.00	82.60	51.22#
34.00	0.00	0.00
0.00	0.00	0.00

T.P
 1/20/15

Data Path : Z:\HPCHEM1\BNA_M\Data\BM011515\
 Data File : BM000205.D
 Acq On : 15 Jan 2015 18:07
 Operator : TP/IZ
 Sample : G1063-05RX
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAN1RX

Quant Time: Jan 16 12:17:28 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 14 12:47:10 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

TEJASKUMAR
 1/16/2015 6:24:05 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	134087	20.00	ng/ul	-0.03
18) Naphthalene-d8	10.62	136	534515	20.00	ng/ul	-0.02
35) Acenaphthene-d10	14.46	164	370755	20.00	ng/ul	-0.02
61) Phenanthrene-d10	17.20	188	759981	20.00	ng/ul	-0.02
75) Chrysene-d12	21.39	240	852851	20.00	ng/ul	-0.02
83) Perylene-d12	23.69	264	832373	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.38	96	777m	0.34	ng/uL	0.05
5) Phenol-d5	6.99	99	66791	5.92	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	7.16	67	176415	24.74	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.36	132	163438	19.76	ng/ul	-0.01
13) 4-Methylphenol-d8	8.52	113	112558	12.54	ng/ul	-0.02
19) Nitrobenzene-d5	8.98	128	96578	26.13	ng/ul	-0.03
22) 2-Nitrophenol-d4	9.70	143	103147	27.33	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.24	165	192392	23.08	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.76	131	436	0.05	ng/ul	-0.02
43) Dimethylphthalate-d6	13.87	166	772932	28.27	ng/ul	-0.02
46) Acenaphthylene-d8	14.16	160	897600	27.40	ng/ul	-0.02
51) 4-Nitrophenol-d4	14.65	143	20133	4.52	ng/ul	-0.01
57) Fluorene-d10	15.46	176	673695	28.69	ng/ul	-0.02
62) 4,6-Dinitro-2-methylphenol	15.57	200	94142	26.14	ng/ul	-0.02
70) Anthracene-d10	17.30	188	1062272	30.23	ng/ul	-0.01
76) Pyrene-d10	19.60	212	1173693	29.83	ng/ul	-0.02
87) Benzo(a)pyrene-d12	23.54	264	1123256	29.73	ng/ul	-0.03

TP
 1/20/15

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.35	88	119676	37.34	ng/uL	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed