

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011515\
 Data File : BM000199.D
 Acq On : 15 Jan 2015 10:55
 Operator : TP/IZ
 Sample : G1063-09DL 2X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AN8DL

Manual Integrations
 APPROVED

TEJASKUMAR
 1/16/2015 6:24:16 PM

Quant Time: Jan 16 03:31:34 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 16 02:28:02 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	135472	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	551297	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	376384	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	758410	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	862980	20.00	ng/ul	0.00
83) Perylene-d12	23.69	264	816023	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.34	96	3014m	1.29	ng/uL	0.02
5) Phenol-d5	6.99	99	31091	2.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	84683	11.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	80983	9.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	49712	5.48	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	42612	11.18	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	46402	11.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	86080	10.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	4962	0.51	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	330721	11.91	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	357018	10.74	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	8103m	1.79	ng/ul	0.00
57) Fluorene-d10	15.46	176	291674	12.24	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	34735	9.66	ng/ul	0.00
70) Anthracene-d10	17.30	188	474131	13.52	ng/ul	0.00
76) Pyrene-d10	19.60	212	553965	13.92	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.53	264	521256	14.07	ng/ul	0.00

Target Compounds					Qvalue
2) 1,4-Dioxane	3.35	88	45618	14.09	ng/uL 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011515\
Data File : BM000199.D
Acq On : 15 Jan 2015 10:55
Operator : TP/IZ
Sample : G1063-09DL 2X
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AN8DL

Manual Integrations
APPROVED

TEJASKUMAR
1/16/2015 6:24:16 PM

Quant Time: Jan 16 03:31:34 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 16 02:28:02 2015
Response via : Initial Calibration

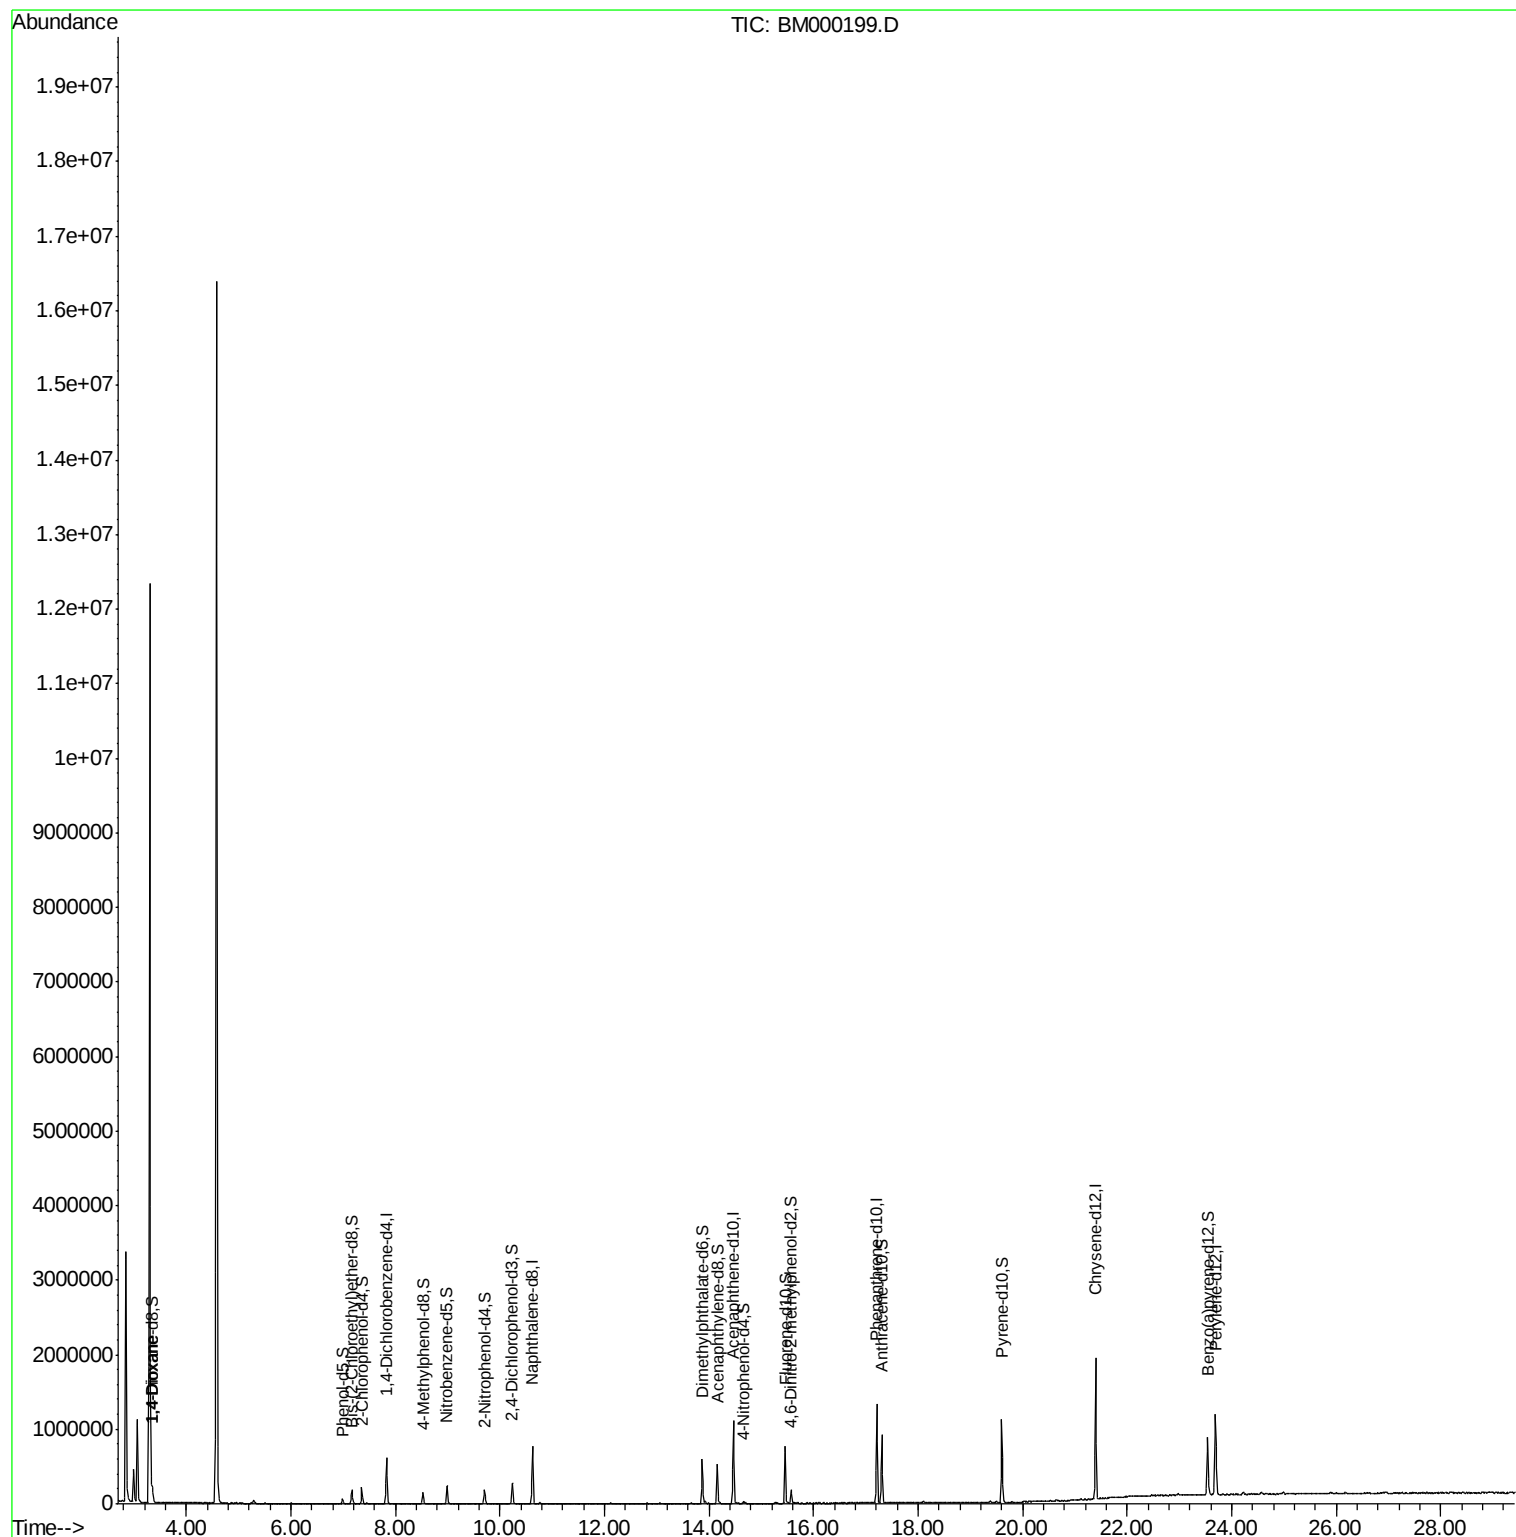

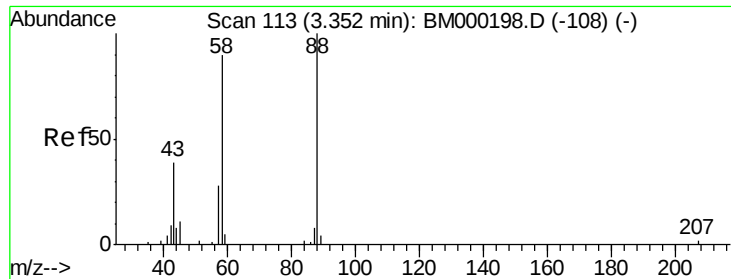

#2
 1,4-Dioxane
 Concen: 14.09 ng/uL
 RT: 3.35 min Scan# 113
 Delta R.T. 0.00 min
 Lab File: BM000199.D
 Acq: 15 Jan 2015 10:55

Instrument :
 BNA_M
 ClientSampleId :
 C0AN8DL

Tgt Ion	Ratio	Lower	Upper
88	100		
43	40.4	34.9	52.3
58	89.7	67.3	100.9

Manual Integrations
 APPROVED

TEJASKUMAR
 1/16/2015 6:24:16 PM

