

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011515\
 Data File : BM000211.D
 Acq On : 15 Jan 2015 22:16
 Operator : TP/IZ
 Sample : G1063-11RX
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AP3RX

Manual Integrations
 APPROVED

TEJASKUMAR
 1/16/2015 6:24:39 PM

Quant Time: Jan 16 04:31:16 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 16 04:15:33 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	136371	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	559090	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	386299	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	786261	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	902611	20.00	ng/ul	0.00
83) Perylene-d12	23.69	264	855300	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	3747m	1.59	ng/uL	0.00
5) Phenol-d5	6.99	99	49133	4.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	144003	19.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	134229	15.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	85657	9.39	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	77886	20.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	82357	20.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	153217	17.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	204	0.02	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	714542	25.08	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	793124	23.24	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	16340	3.52	ng/ul	0.00
57) Fluorene-d10	15.46	176	618397	25.28	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	83722	22.47	ng/ul	0.00
70) Anthracene-d10	17.30	188	995393	27.38	ng/ul	0.00
76) Pyrene-d10	19.60	212	1146034	27.52	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.54	264	1085006	27.95	ng/ul	0.00

Target Compounds					Qvalue
2) 1,4-Dioxane	3.35	88	54846	16.82 ng/uL	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011515\
Data File : BM000211.D
Acq On : 15 Jan 2015 22:16
Operator : TP/IZ
Sample : G1063-11RX
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AP3RX

Manual Integrations
APPROVED

TEJASKUMAR
1/16/2015 6:24:39 PM

Quant Time: Jan 16 04:31:16 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 16 04:15:33 2015
Response via : Initial Calibration

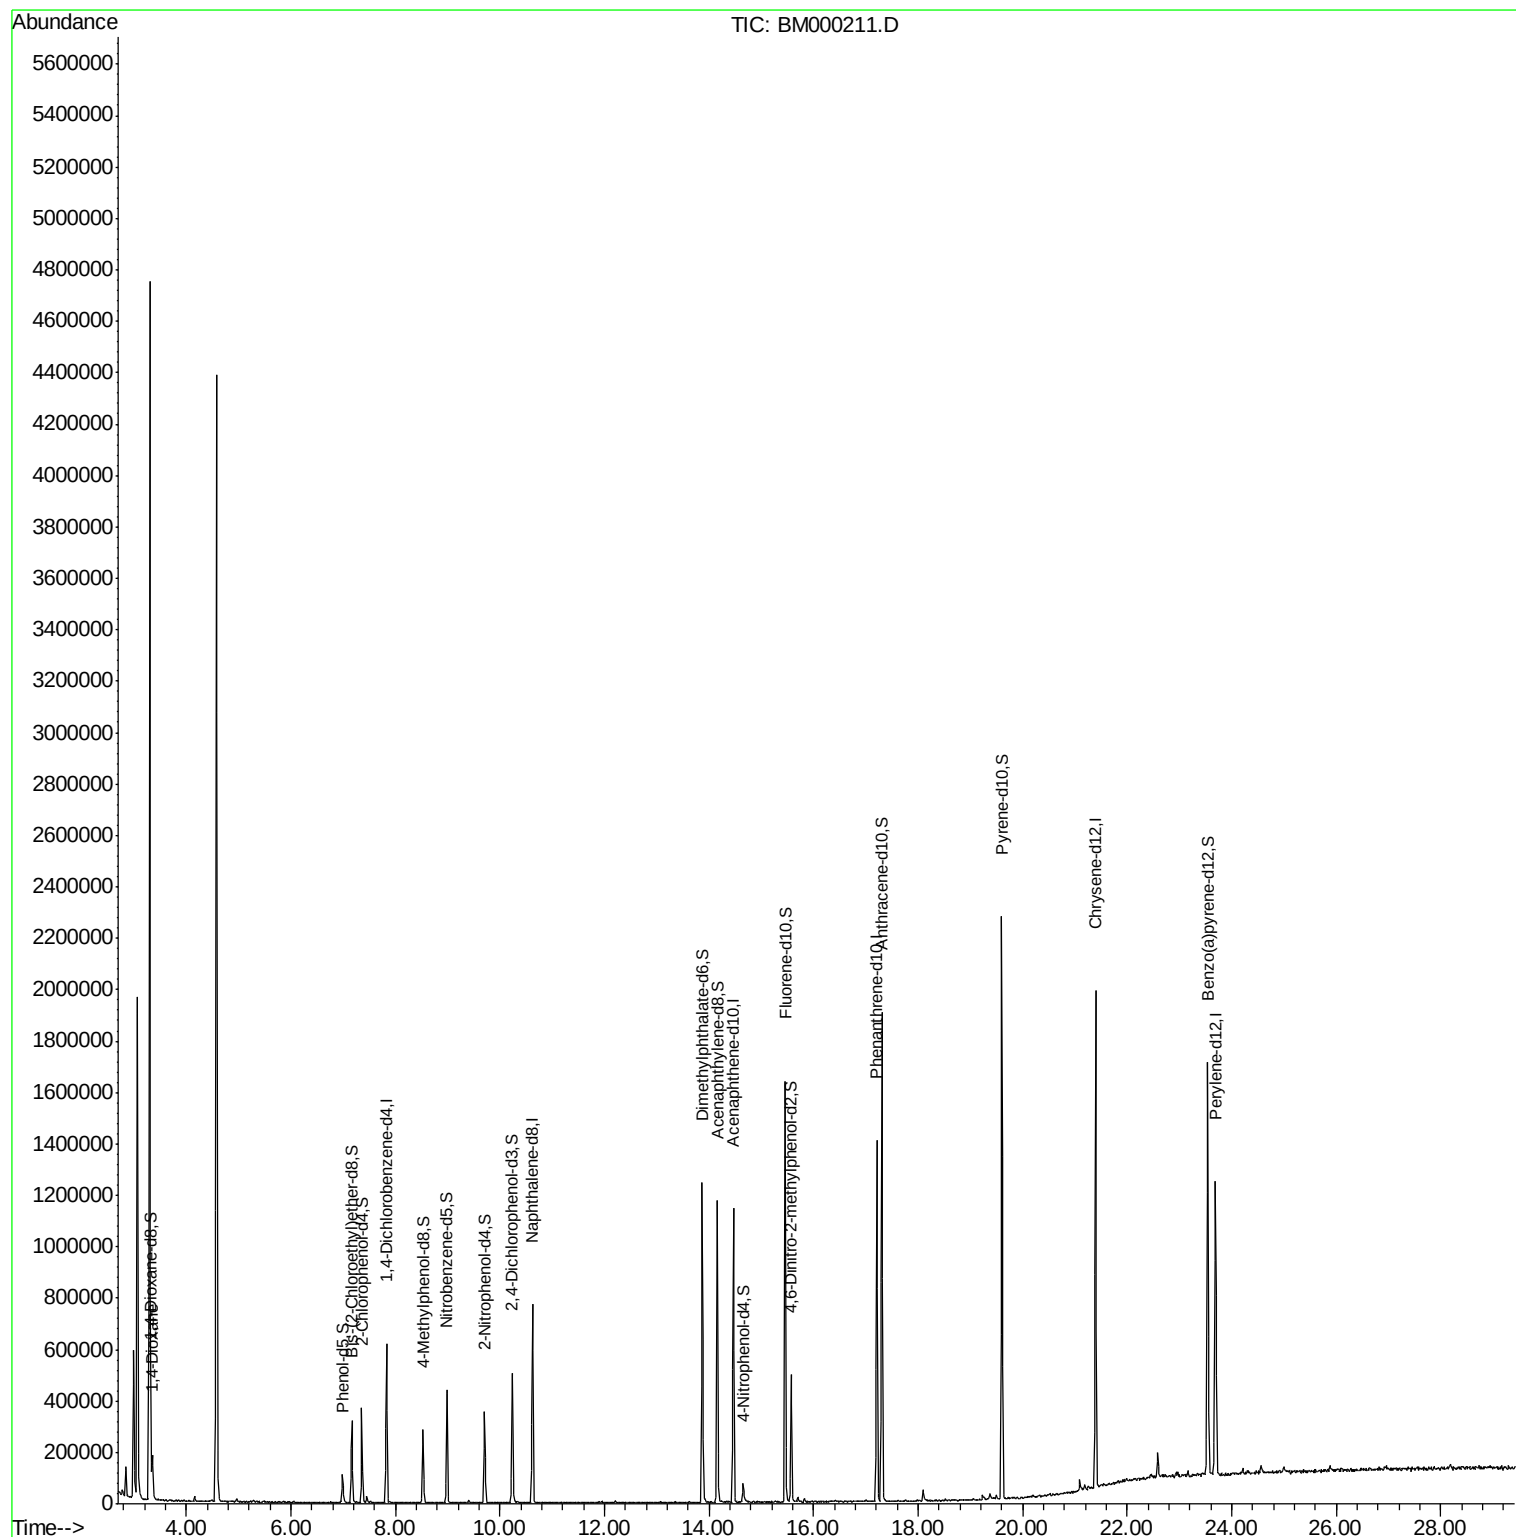

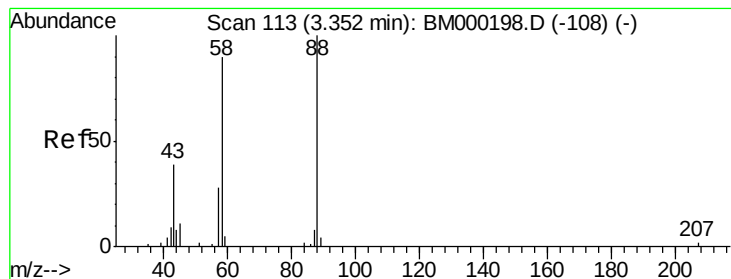

#2

1,4-Dioxane

Concen: 16.82 ng/uL

RT: 3.35 min Scan# 113

Delta R.T. 0.00 min

Lab File: BM000211.D


Acq: 15 Jan 2015 22:16

Instrument :

BNA_M

ClientSampleId :

C0AP3RX

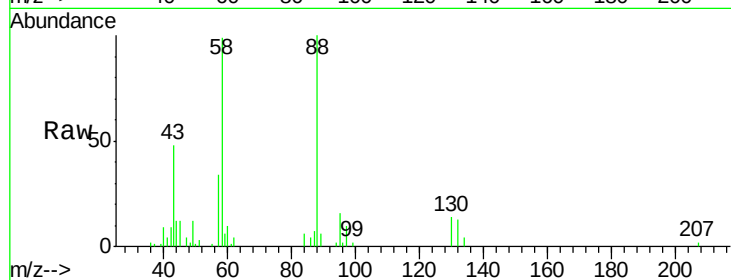

Tgt Ion: 88 Resp: 54846

Ion Ratio Lower Upper

88 100

43 45.1 34.9 52.3

58 93.2 67.3 100.9

Manual Integrations

APPROVED

TEJASKUMAR

1/16/2015 6:24:39 PM

