

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011515\
 Data File : BM000221.D
 Acq On : 16 Jan 2015 04:12
 Operator : TP/IZ
 Sample : G1066-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AR0

Quant Time: Jan 16 04:58:45 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 16 04:15:33 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	157024	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	669302	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	465993	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	919808	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	1005221	20.00	ng/ul	0.00
83) Perylene-d12	23.69	264	977386	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	7001	2.59	ng/uL	0.00
5) Phenol-d5	6.99	99	213834	16.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	139724	16.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	157766	16.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	166456	15.84	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	75034	16.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	82550	17.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	158063	15.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	196573	16.60	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	569338	16.57	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	682348	16.57	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	75622	13.52	ng/ul	0.00
57) Fluorene-d10	15.46	176	492318	16.68	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	69928	16.04	ng/ul	0.00
70) Anthracene-d10	17.30	188	754080	17.73	ng/ul	0.00
76) Pyrene-d10	19.60	212	825759	17.81	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.54	264	783451	17.66	ng/ul	0.00


Target Compounds						Qvalue
6) Phenol	7.02	94	19308	1.39	ng/ul	95
44) Dimethylphthalate	13.92	163	92376	2.70	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011515\
Data File : BM000221.D
Acq On : 16 Jan 2015 04:12
Operator : TP/IZ
Sample : G1066-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AR0

Quant Time: Jan 16 04:58:45 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 16 04:15:33 2015
Response via : Initial Calibration

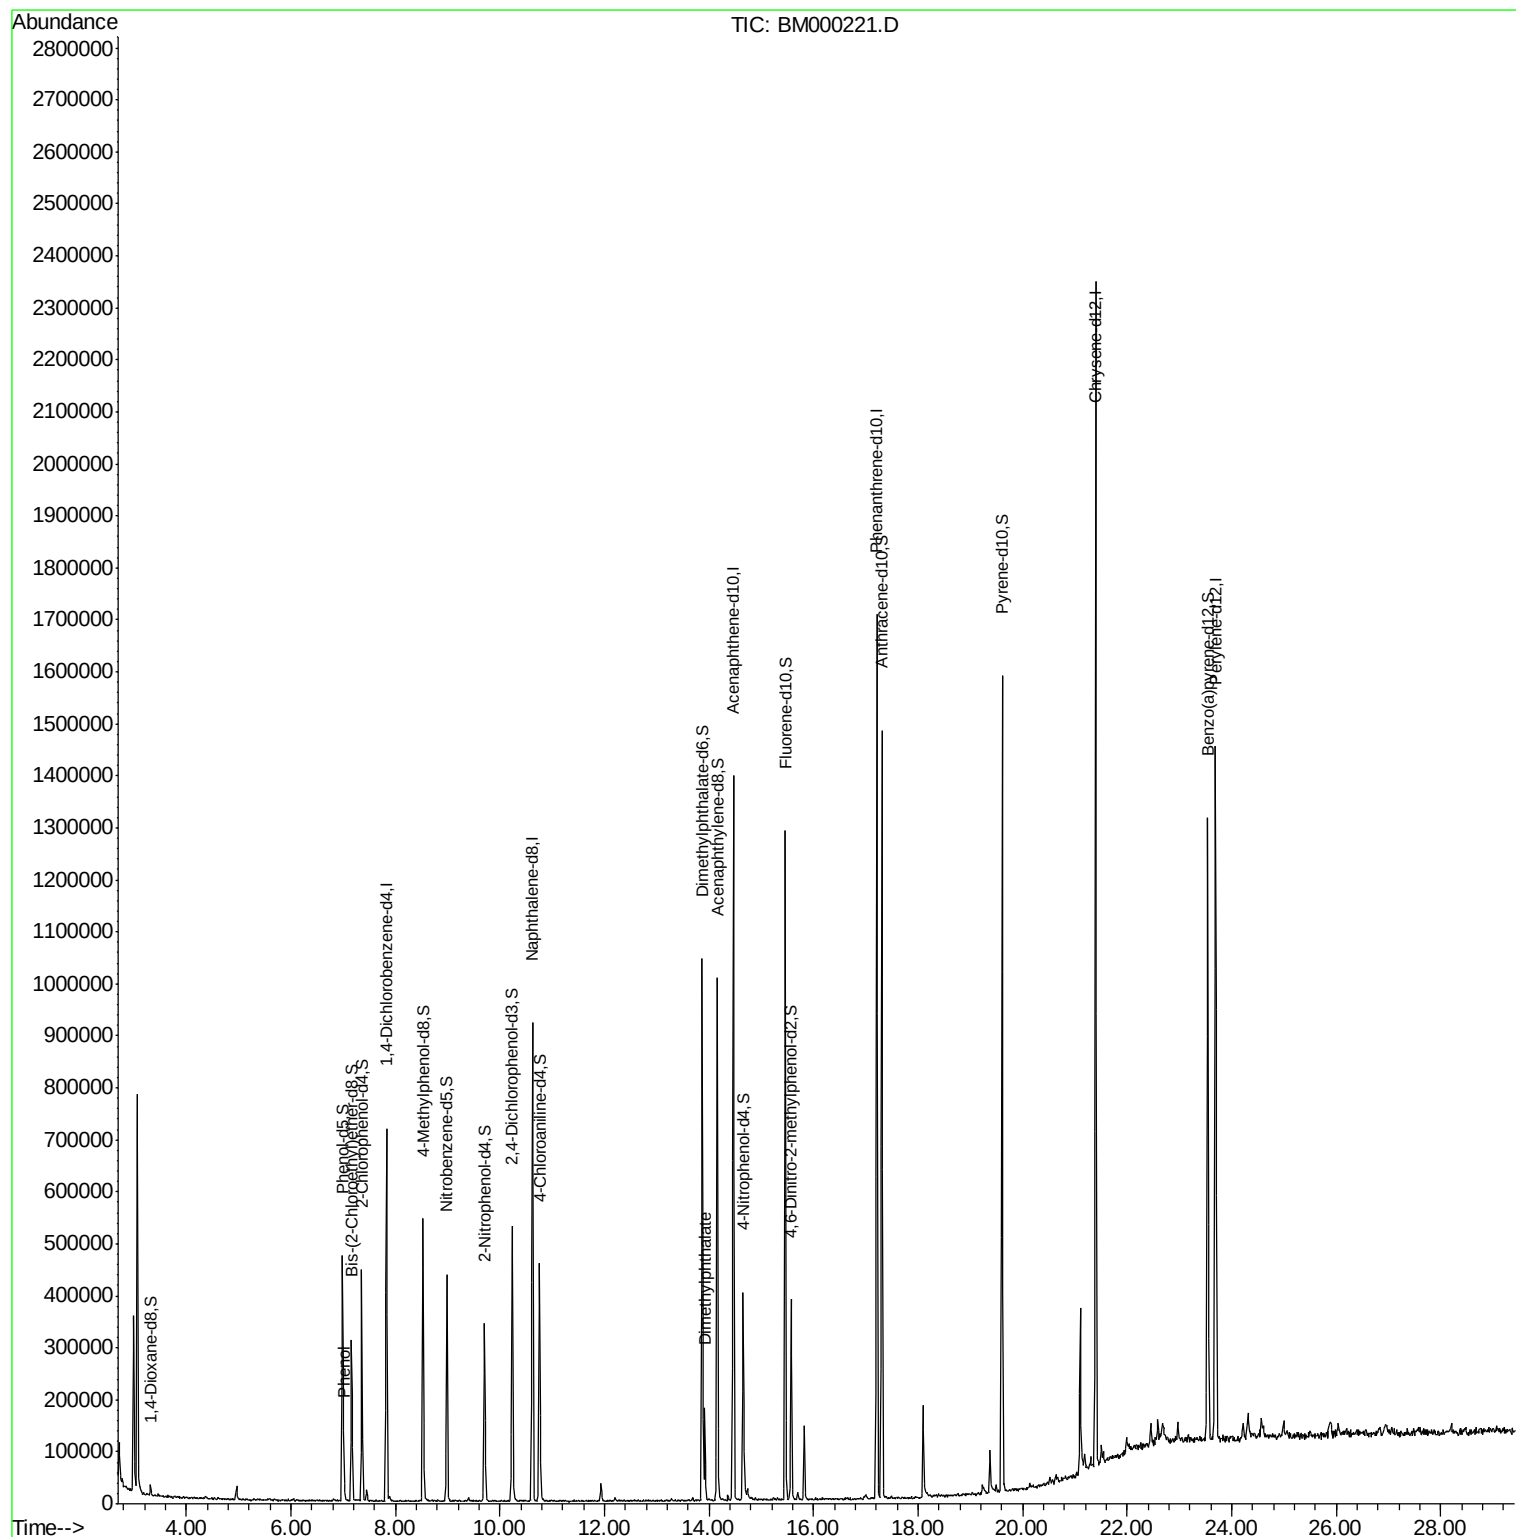

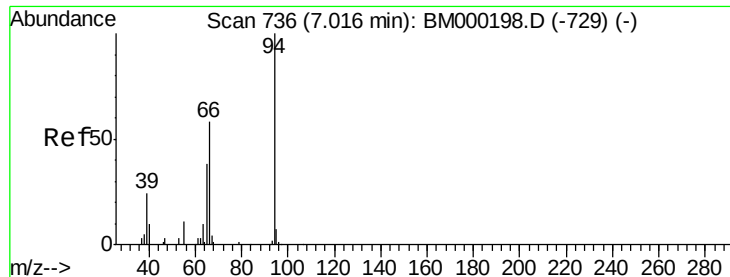

#6

Phenol

Concen: 1.39 ng/ul

RT: 7.02 min Scan# 736

Delta R.T. 0.00 min

Lab File: BM000221.D

Acq: 16 Jan 2015 04:12

Instrument :

BNA_M

ClientSampleId :

C0AR0





Tgt Ion: 94 Resp: 19308

Ion Ratio Lower Upper

94 100

65 29.9 27.4 41.0

66 55.6 42.5 63.7

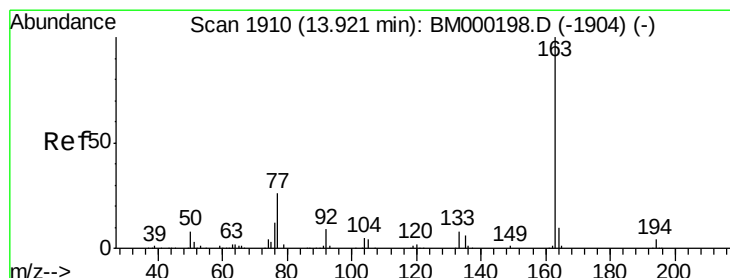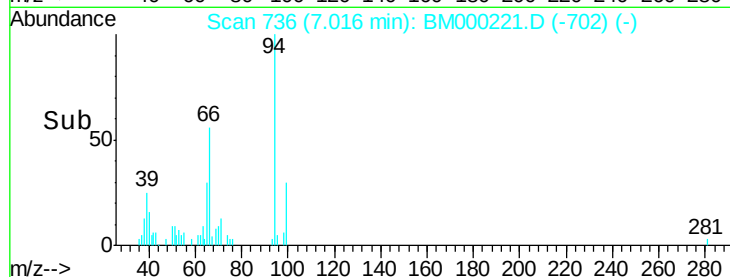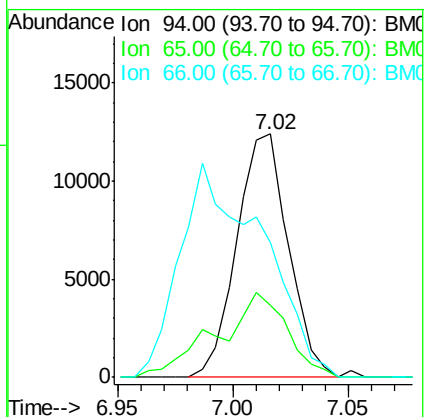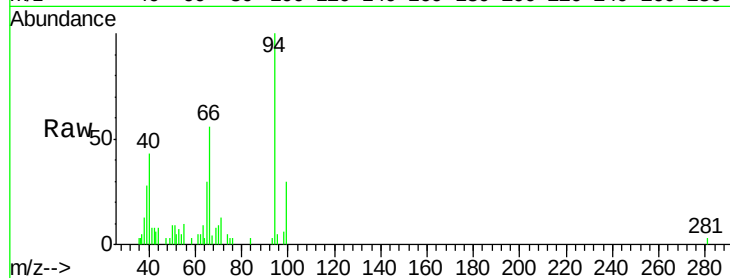

#44

Dimethylphthalate

Concen: 2.70 ng/ul

RT: 13.92 min Scan# 1909

Delta R.T. -0.01 min

Lab File: BM000221.D

Acq: 16 Jan 2015 04:12

Tgt Ion: 163 Resp: 92376

Ion Ratio Lower Upper

163 100

194 4.1 3.0 4.4

164 7.9 8.5 12.7#

