

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011516\
 Data File : BM004027.D
 Acq On : 15 Jan 2016 00:26
 Operator : SJ/UM
 Sample : H1099-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC9A3

Quant Time: Jan 15 01:07:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 15 00:28:21 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	41439	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	201042	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.32	164	117854	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.07	188	258204	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	225723	20.00	ng/ul	0.00
86) Perylene-d12	23.51	264	196537	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	3985	4.30	ng/uL	0.00
5) Phenol-d5	6.84	99	102321	29.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	60206	30.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	87197	30.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	86696	31.10	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	44443	29.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	48697	29.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	84650	28.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	123843	31.81	ng/ul	0.00
44) Dimethylphthalate-d6	13.73	166	277635	30.01	ng/ul	0.00
47) Acenaphthylene-d8	14.01	160	348186	30.89	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	40584	24.42	ng/ul	0.00
58) Fluorene-d10	15.32	176	245560	31.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	29040	19.94	ng/ul	0.00
71) Anthracene-d10	17.17	188	378345	31.68	ng/ul	0.00
79) Pyrene-d10	19.47	212	394286	33.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	318507	32.45	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.78	163	86581	9.18	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011516\
Data File : BM004027.D
Acq On : 15 Jan 2016 00:26
Operator : SJ/UM
Sample : H1099-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC9A3

Quant Time: Jan 15 01:07:23 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 15 00:28:21 2016
Response via : Initial Calibration

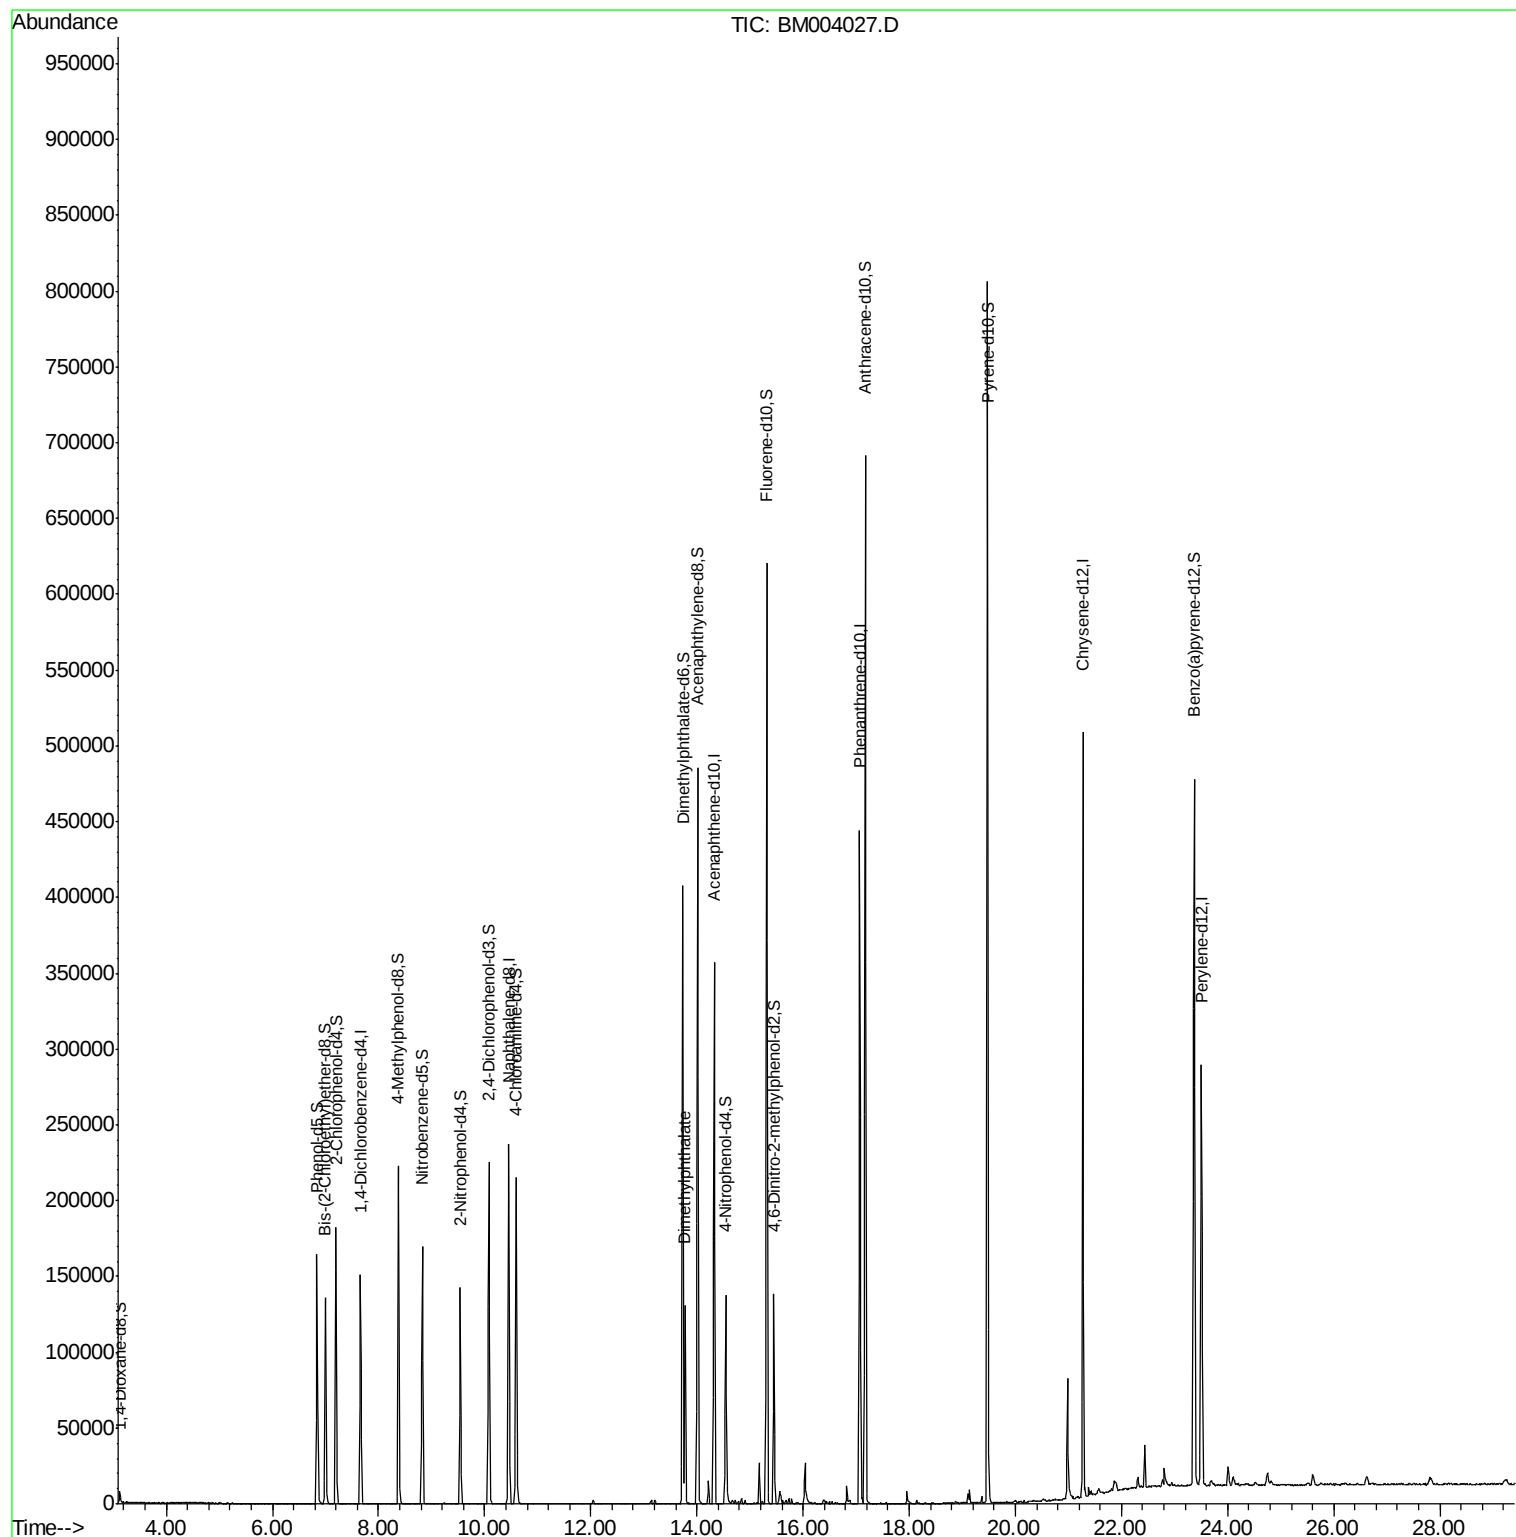

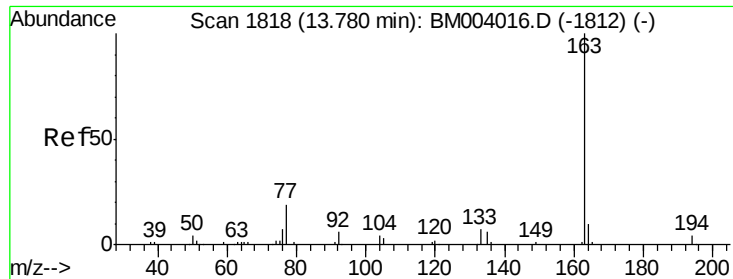

#45

Dimethylphthalate

Concen: 9.18 ng/ul

RT: 13.78 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BM004027.D


Acq: 15 Jan 2016 00:26

Instrument :

BNA_M

ClientSampleId :

BC9A3

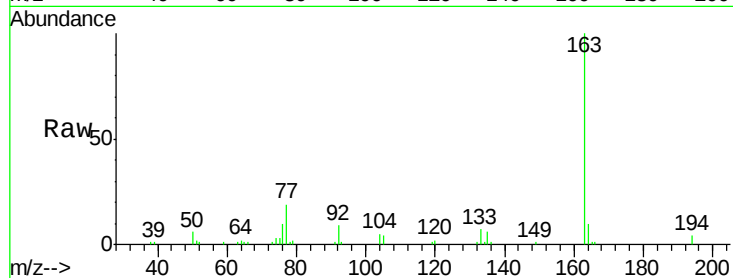


Tgt Ion:163 Resp: 86581

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 9.7 7.8 11.8

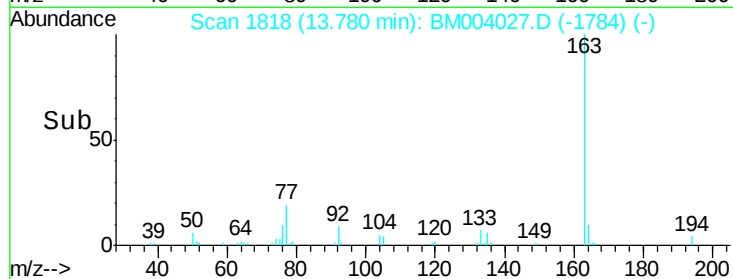

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

