


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011516\
Data File : BM004025.D
Acq On : 14 Jan 2016 23:14
Operator : SJ/UM
Sample : H1099-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jan 15 01:00:23 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 15 00:28:21 2016
Response via : Initial Calibration

Instrument :
BNA M
ClientSampleId :
BC9A1

Manual Integrations
APPROVED

mohammad
1/15/2016 3:03:06 PM

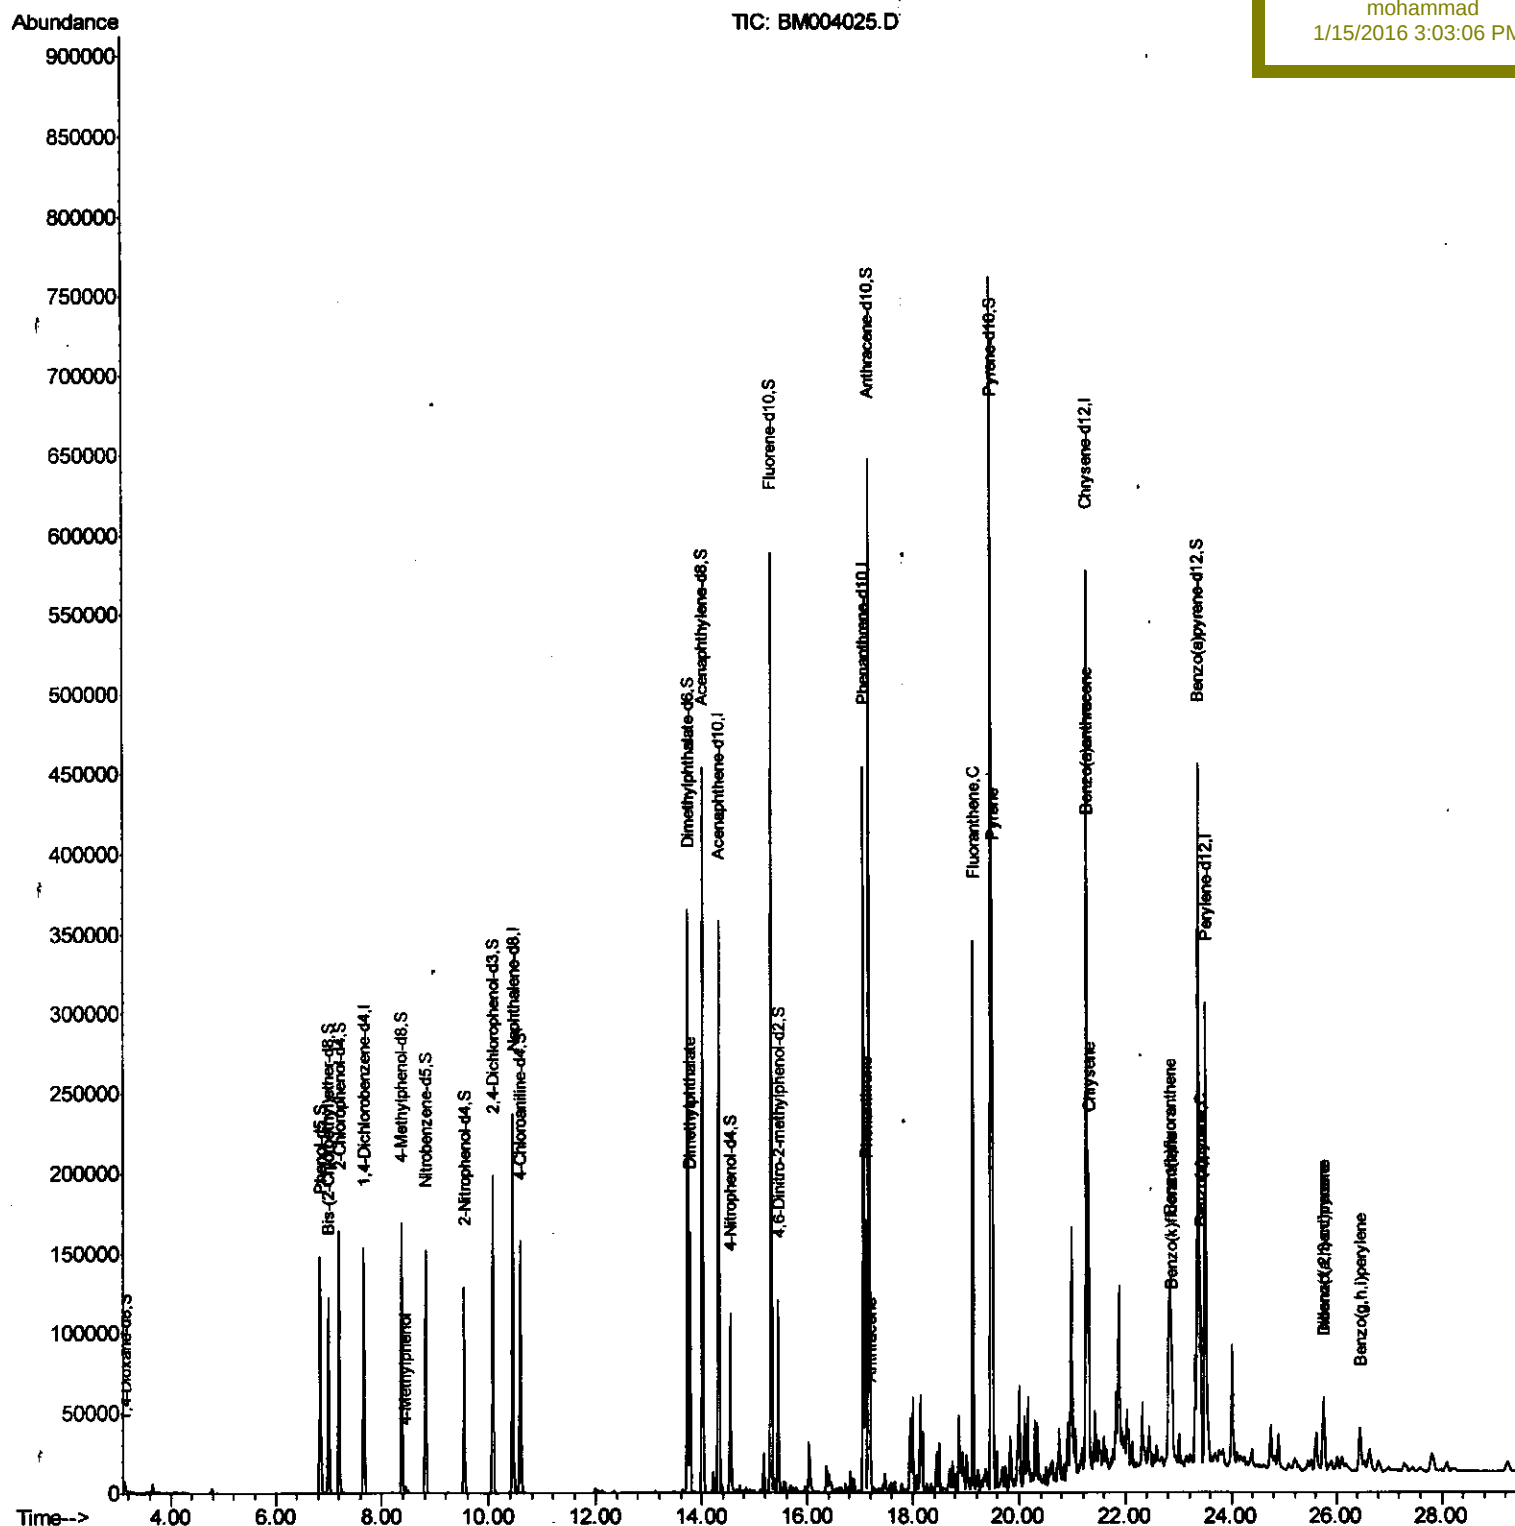

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011516\
Data File : BM004025.D
Acq On : 14 Jan 2016 23:14
Operator : SJ/UM
Sample : H1099-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jan 15 01:00:23 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 15 00:28:21 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BC9A1

Manual Integrations
APPROVED
mohammad
1/15/2016 3:03:06 PM


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	41713	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	201083	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.32	164	118857	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.07	188	262125	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	231272	20.00	ng/ul	0.00
86) Perylene-d12	23.51	264	199297	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.13	96	3895	4.18	ng/ul	0.00
5) Phenol-d5	6.84	99	92954	26.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	54253	27.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	78981	27.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	66616	23.74	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	40105	26.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	43920	26.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	77194	26.17	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	93086	23.90	ng/ul	0.00
44) Dimethylphthalate-d6	13.73	166	253391	27.16	ng/ul	0.00
47) Acenaphthylene-d8	14.01	160	316295	27.82	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	32908	19.64	ng/ul	0.00
58) Fluorene-d10	15.32	176	225551	28.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	25751	17.42	ng/ul	0.00
71) Anthracene-d10	17.17	188	340623	28.10	ng/ul	0.00
79) Pyrene-d10	19.47	212	353510	29.51	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	281378	28.27	ng/ul	0.00
Target Compounds						
16) 4-Methylphenol	8.45	108	3156	1.04	ng/ul	98
45) Dimethylphthalate	13.77	163	105498	11.09	ng/ul	99
70) Phenanthrene	17.11	178	101690	6.90	ng/ul	99
72) Anthracene	17.20	178	20515	1.36	ng/ul	100
77) Fluoranthene	19.14	202	199963	13.05	ng/ul	99
80) Pyrene	19.50	202	215357	13.72	ng/ul	98
83) Benzo(a)anthracene	21.26	228	86785	6.30	ng/ul	98
85) Chrysene	21.31	228	97040	7.42	ng/ul	98
88) Benzo(b)fluoranthene	22.84	252	95848	7.91	ng/ul	97
89) Benzo(k)fluoranthene	22.87	252	31778m	2.76	ng/ul	
91) Benzo(a)pyrene	23.41	252	72356	6.30	ng/ul	95
92) Indeno(1,2,3-cd)pyrene	25.76	276	42994	3.38	ng/ul	98
93) Dibenzo(a,h)anthracene	25.76	278	13106	1.23	ng/ul#	80
94) Benzo(g,h,i)perylene	26.45	276	34534	3.24	ng/ul	98

S. J
01/15/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jan 15 00:33:52 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 15 00:28:21 2016
Response via : Initial Calibration

mohammad
1/15/2016 3:03:06 PM

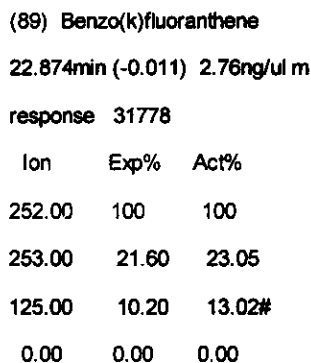
$$\begin{array}{r} \text{S.I} \\ \hline 10 \overline{) 115116} \end{array}$$


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011516\
 Data File : BM004025.D
 Acq On : 14 Jan 2016 23:14
 Operator : SJ/UM
 Sample : H1099-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jan 15 00:33:52 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 15 00:28:21 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampled :
 BC9A1

Manual Integrations
 APPROVED

mohammad
 1/15/2016 3:03:06 PM

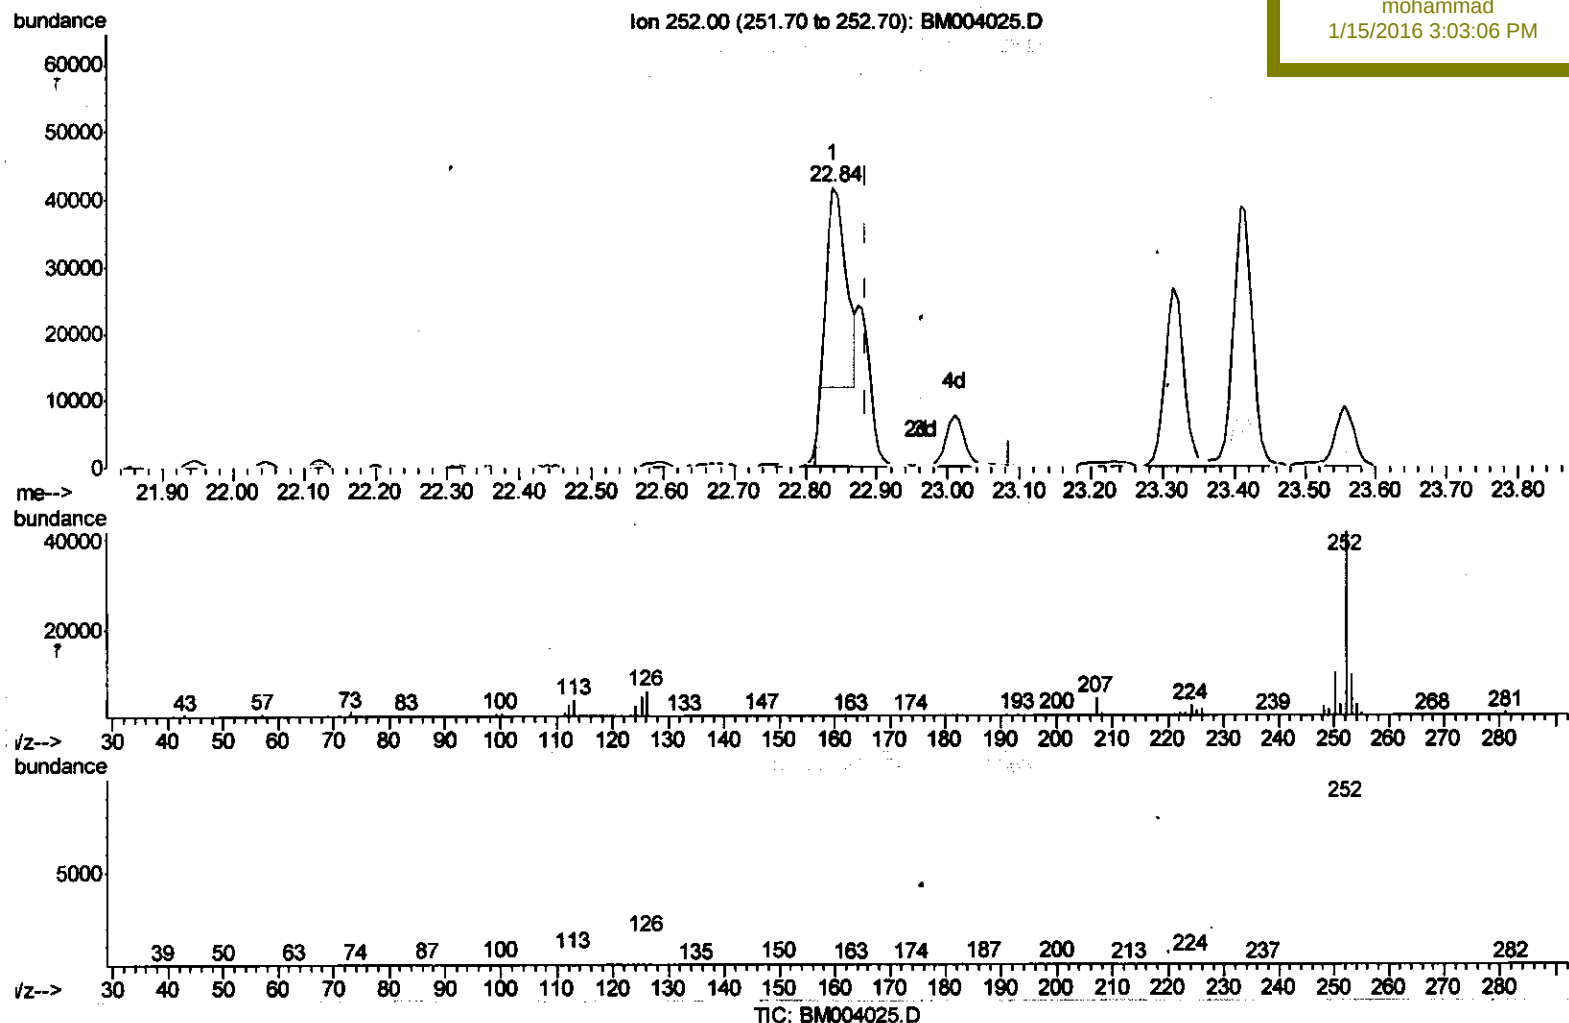

(89) Benzo(k)fluoranthene

22.839min (-0.047) 4.87ng/ul

response 56144

Ion	Exp%	Act%
252.00	100	100
253.00	21.60	22.98
125.00	10.20	11.92
0.00	0.00	0.00