

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011516\
 Data File : BM004023.D
 Acq On : 14 Jan 2016 21:32
 Operator : SJ/UM
 Sample : H1099-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC999

Quant Time: Jan 15 00:33:22 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 15 00:28:21 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	44382	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	214115	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.32	164	123914	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.07	188	271682	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	230734	20.00	ng/ul	0.00
86) Perylene-d12	23.51	264	201605	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	4668	4.70	ng/uL	0.00
5) Phenol-d5	6.85	99	113110	30.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	67180	32.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	96186	31.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	96979	32.48	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	49694	30.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	54743	30.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	93420	29.74	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	141249	34.06	ng/ul	0.00
44) Dimethylphthalate-d6	13.73	166	316645	32.55	ng/ul	0.00
47) Acenaphthylene-d8	14.01	160	388870	32.81	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	48903	27.99	ng/ul	0.00
58) Fluorene-d10	15.32	176	277624	33.65	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	35268	23.02	ng/ul	0.00
71) Anthracene-d10	17.17	188	429732	34.20	ng/ul	0.00
79) Pyrene-d10	19.47	212	442089	37.00	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	352730	35.03	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.78	163	174700	17.62	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011516\
Data File : BM004023.D
Acq On : 14 Jan 2016 21:32
Operator : SJ/UM
Sample : H1099-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC999

Quant Time: Jan 15 00:33:22 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 15 00:28:21 2016
Response via : Initial Calibration

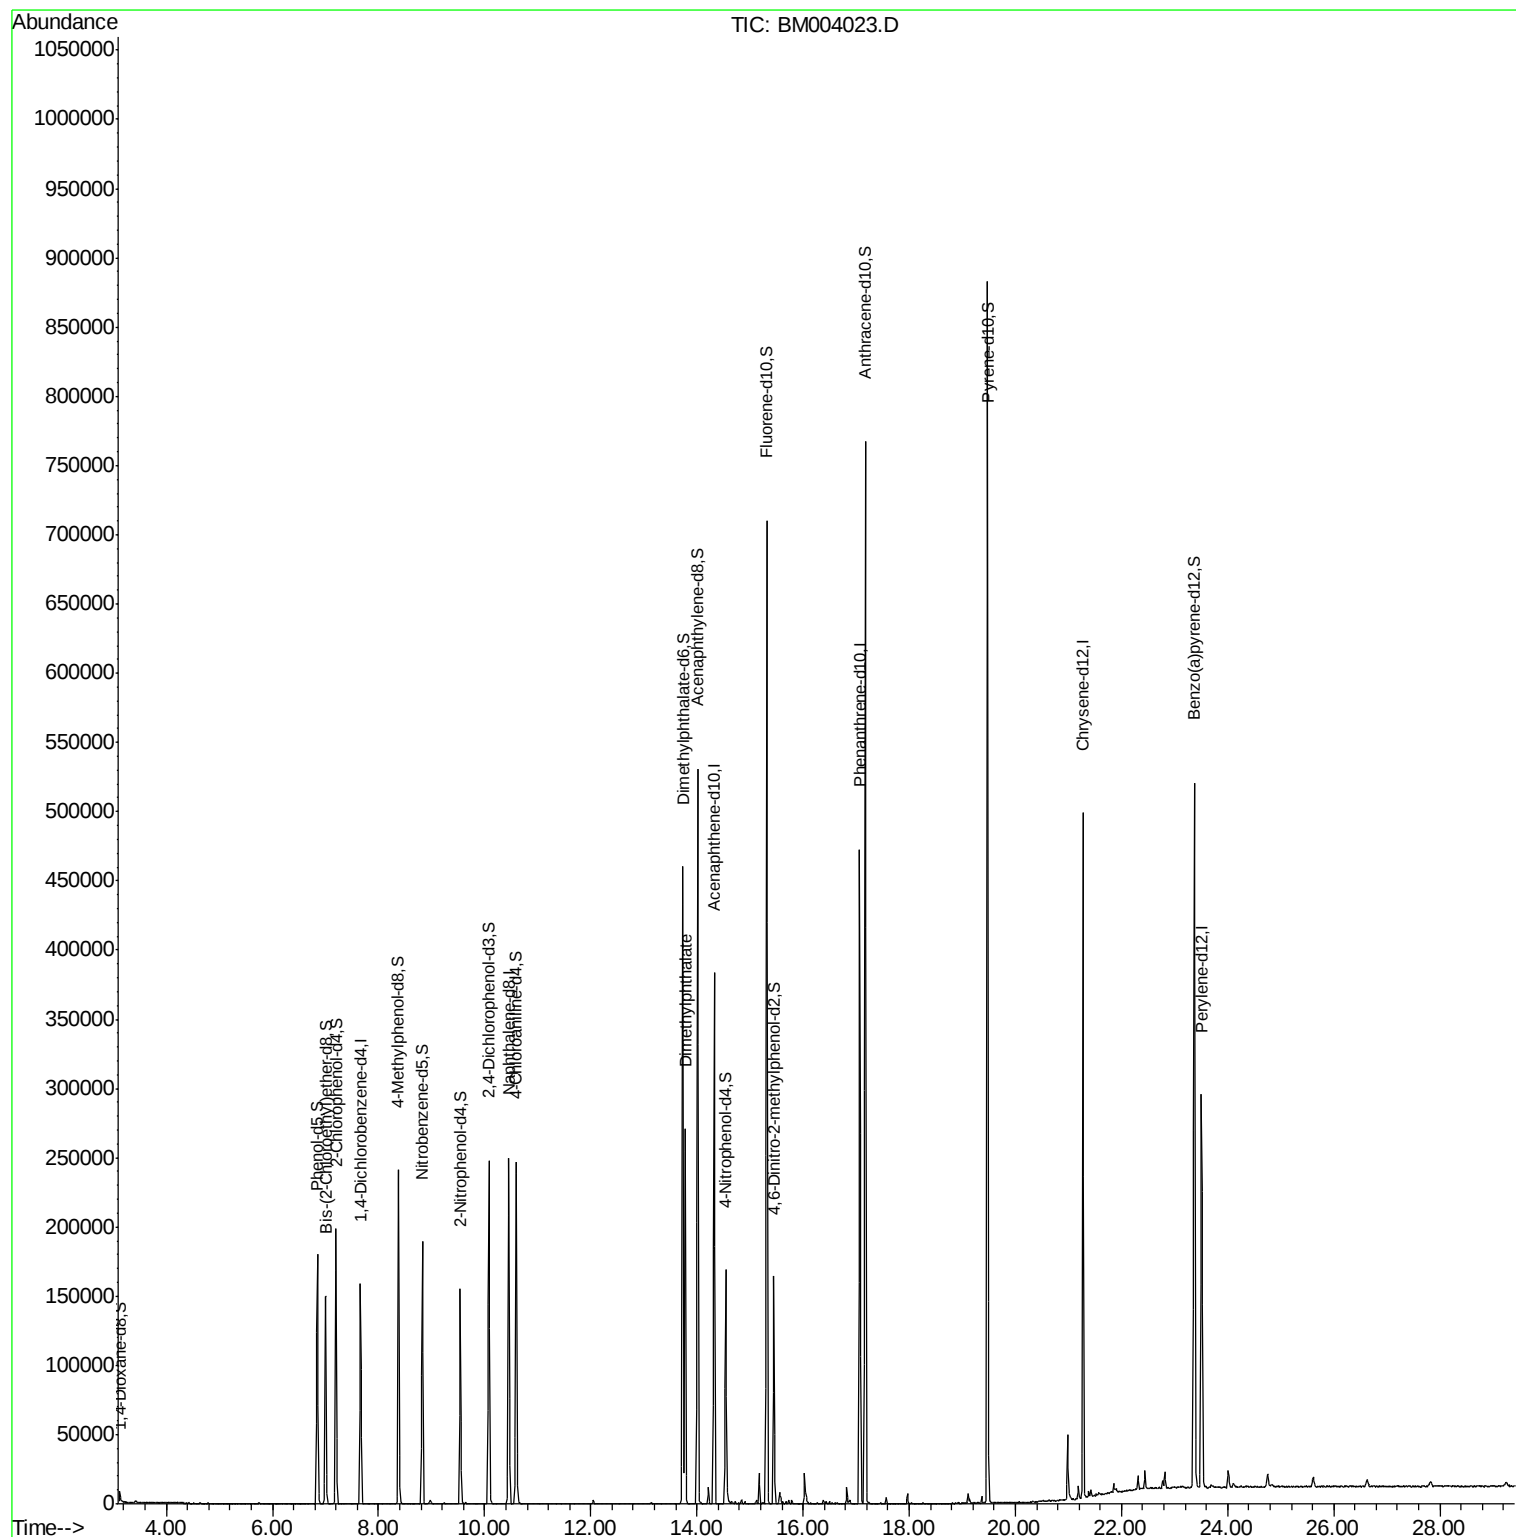

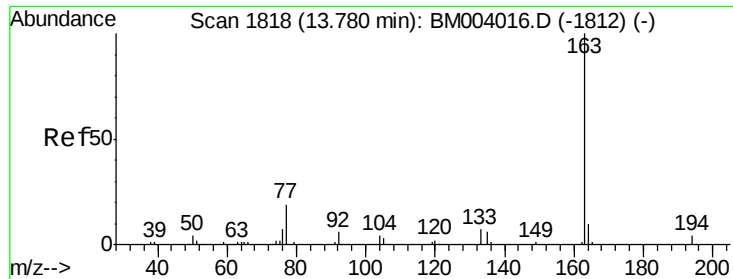

#45

Dimethylphthalate

Concen: 17.62 ng/ul

RT: 13.78 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BM004023.D


Acq: 14 Jan 2016 21:32

Instrument :

BNA_M

ClientSampleId :

BC999

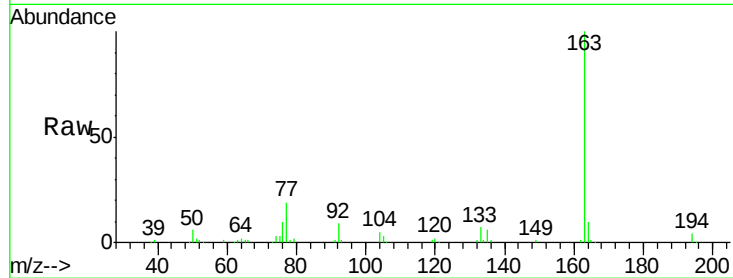


Tgt Ion:163 Resp: 174700

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 9.8 7.8 11.8

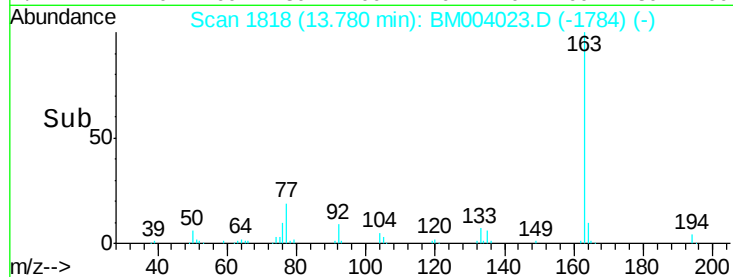

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

