

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011516\
 Data File : BM004026.D
 Acq On : 14 Jan 2016 23:50
 Operator : SJ/UM
 Sample : H1099-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC9E2

Quant Time: Jan 15 00:34:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 15 00:28:21 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	43139	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	206977	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.32	164	122071	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.07	188	266084	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	225149	20.00	ng/ul	0.00
86) Perylene-d12	23.51	264	196915	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	4311	4.47	ng/uL	0.00
5) Phenol-d5	6.85	99	105260	29.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	62375	30.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	88539	30.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	87782	30.25	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	46331	29.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	51446	30.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	87673	28.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	132484	33.05	ng/ul	0.00
44) Dimethylphthalate-d6	13.73	166	292769	30.55	ng/ul	0.00
47) Acenaphthylene-d8	14.01	160	371101	31.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	41928	24.36	ng/ul	0.00
58) Fluorene-d10	15.32	176	260105	32.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	30901	20.59	ng/ul	0.00
71) Anthracene-d10	17.17	188	391094	31.78	ng/ul	0.00
79) Pyrene-d10	19.47	212	397704	34.11	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	321068	32.65	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.78	163	105255	10.77	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011516\
Data File : BM004026.D
Acq On : 14 Jan 2016 23:50
Operator : SJ/UM
Sample : H1099-16
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC9E2

Quant Time: Jan 15 00:34:13 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 15 00:28:21 2016
Response via : Initial Calibration

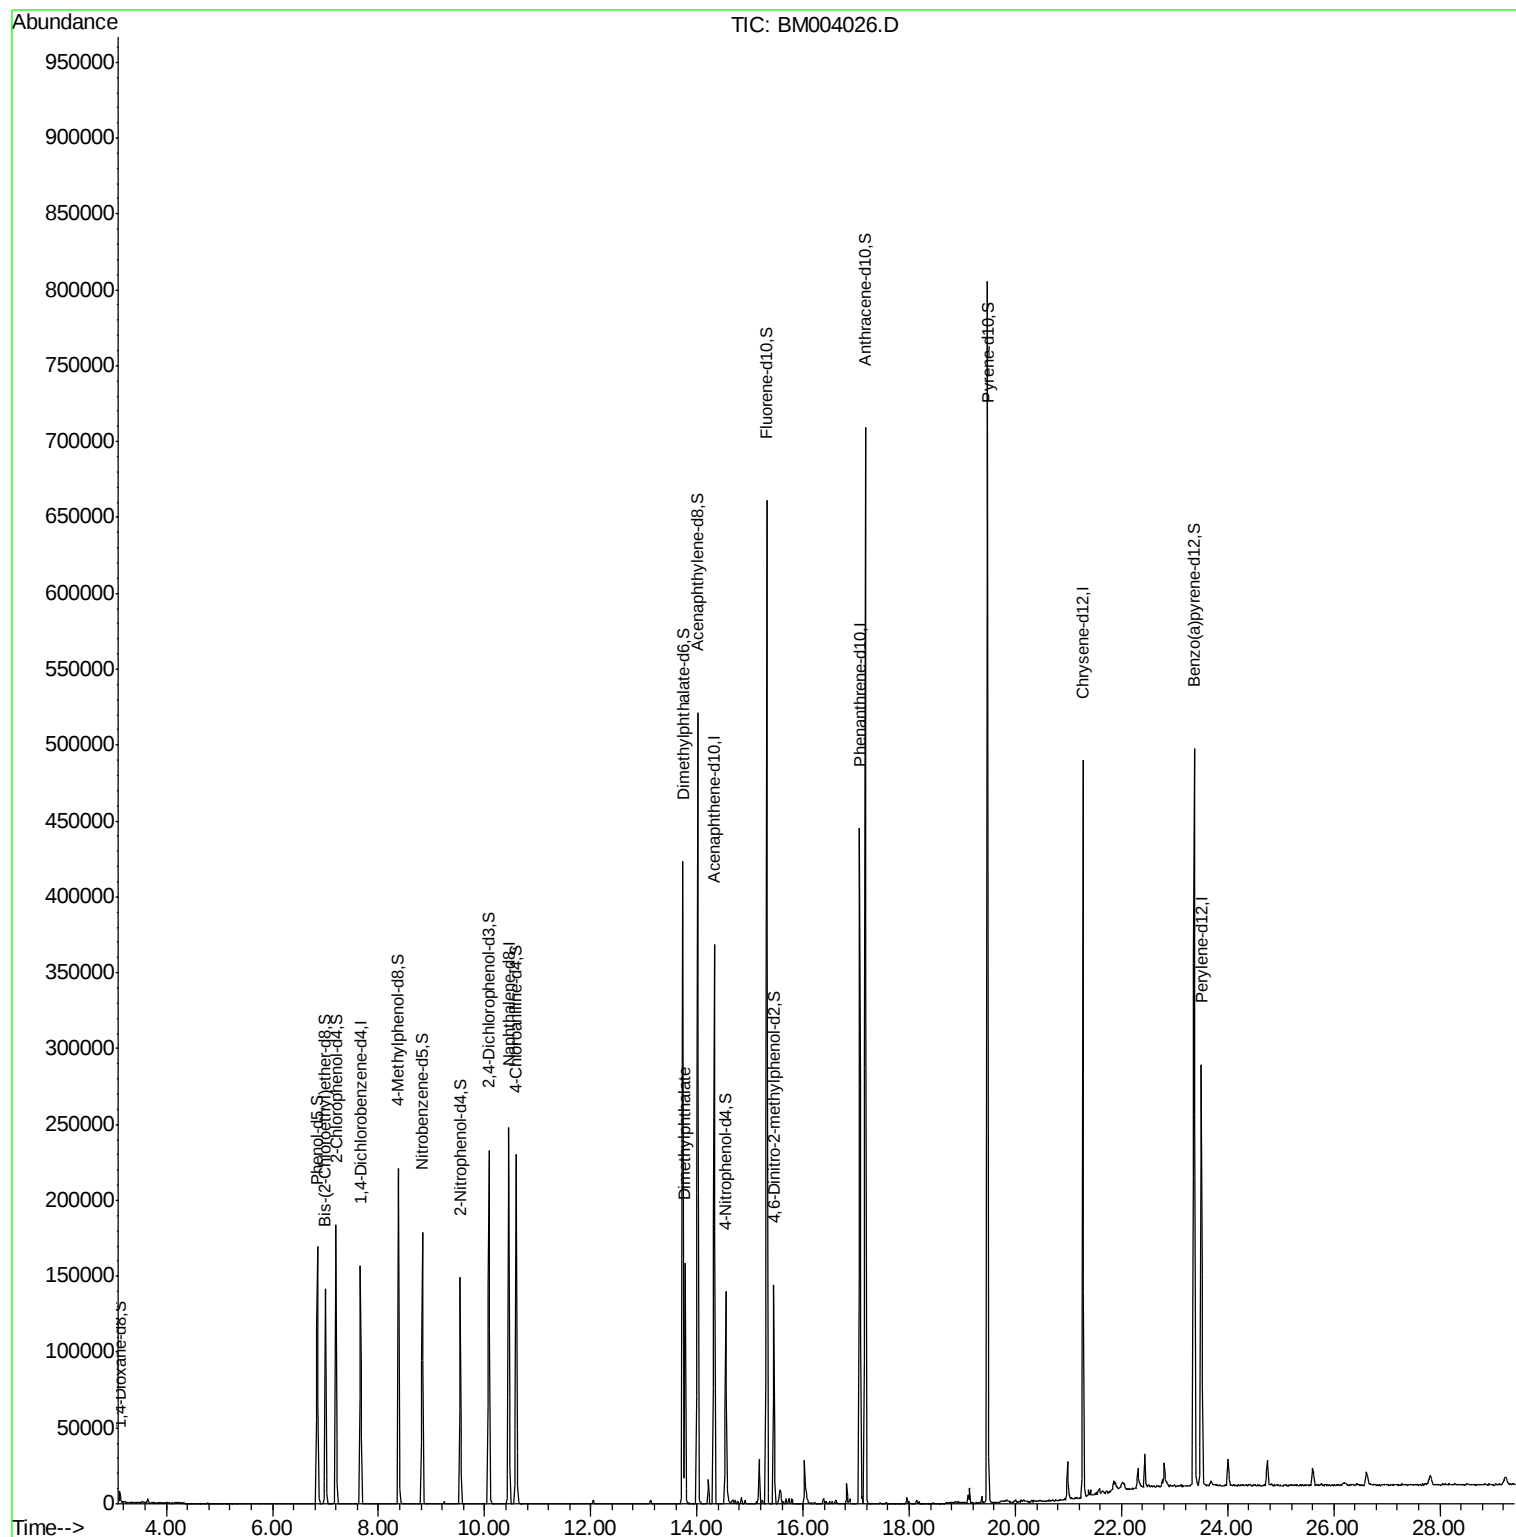

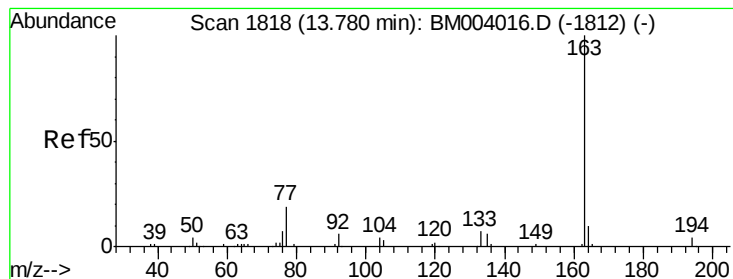

#45

Dimethylphthalate

Concen: 10.77 ng/ul

RT: 13.78 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BM004026.D


Acq: 14 Jan 2016 23:50

Instrument :

BNA_M

ClientSampleId :

BC9E2

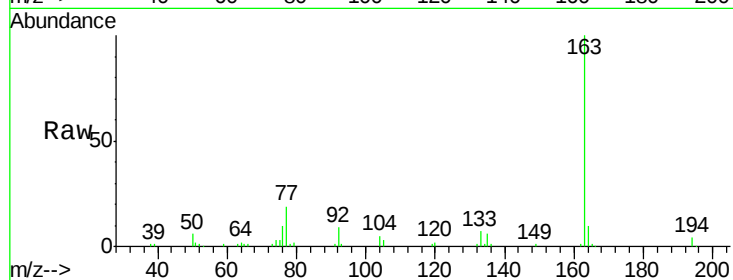


Tgt Ion:163 Resp: 105255

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 10.0 7.8 11.8

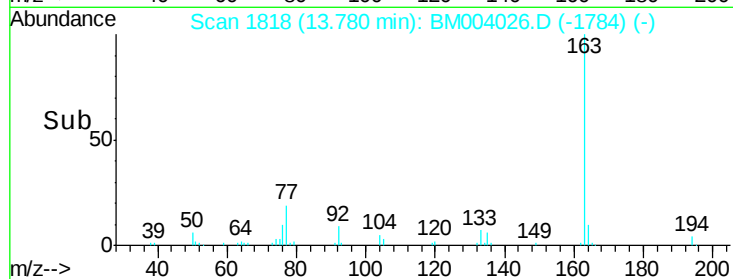

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

