


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011516\
Data File : BM004015.D
Acq On : 14 Jan 2016 16:21
Operator : SJ/UM
Sample : DFTPP38
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP38

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Title : SVOA CALIBRATION
Last Update : Fri Jan 15 00:28:21 2016

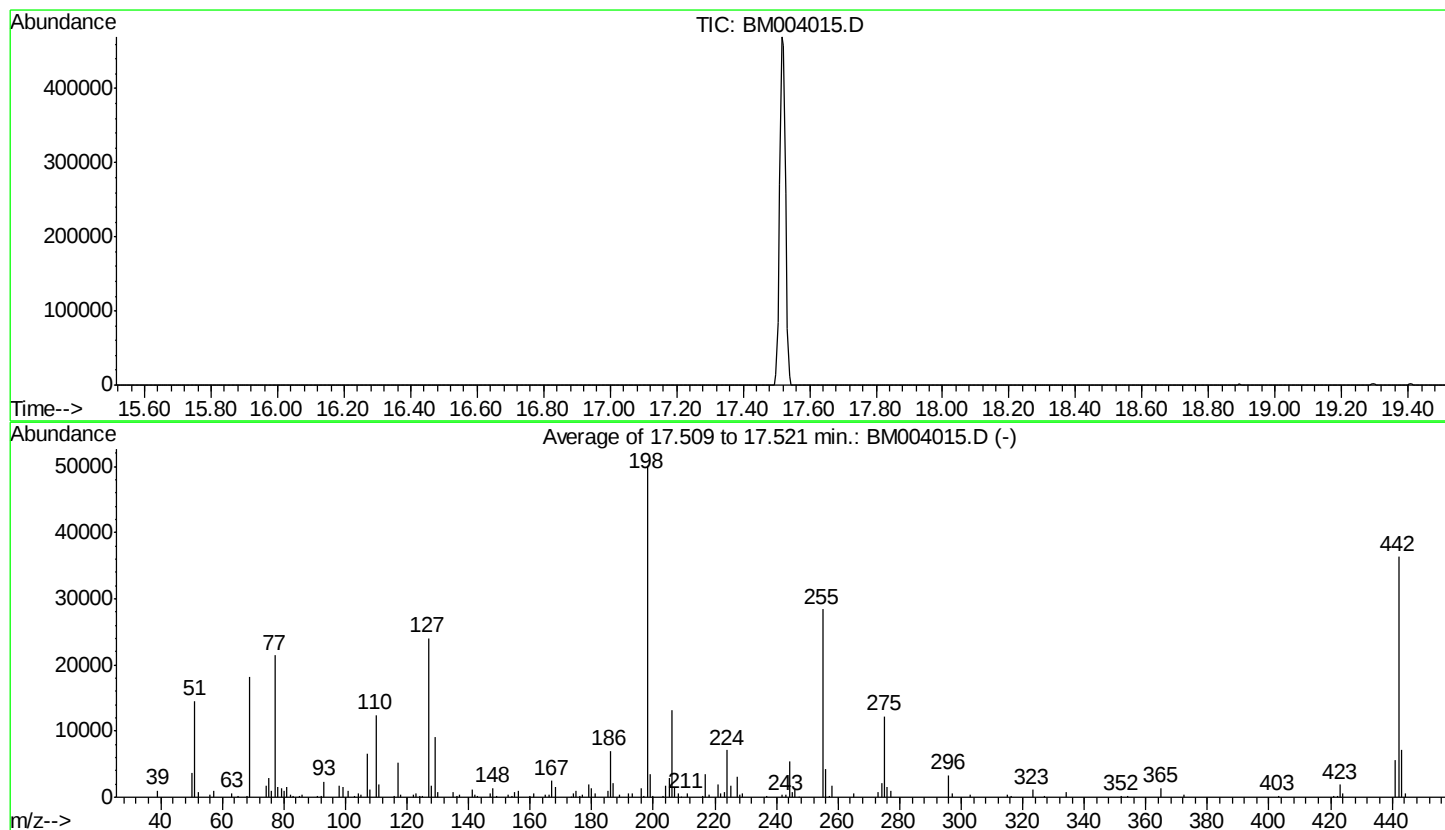

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2447


Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	14616	PASS
68	69	0.00	2	0.6	115	PASS
69	198	0.00	100	36.3	18187	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	24080	PASS
197	198	0.00	2	0.4	216	PASS
198	198	100	100	100.0	50154	PASS
199	198	5	9	6.9	3450	PASS
275	198	10	60	24.4	12233	PASS
365	198	1	100	2.7	1356	PASS
441	443	0.01	100	78.1	5562	PASS
442	198	50	100	72.4	36333	PASS
443	442	15	24	19.6	7123	PASS

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011516\
 Data File : BM004015.D
 Acq On : 14 Jan 2016 16:21
 Operator : SJ/UM
 Sample : DFTPP38
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP38

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
 Title : SVOA CALIBRATION
 Last Update : Fri Jan 15 00:28:21 2016

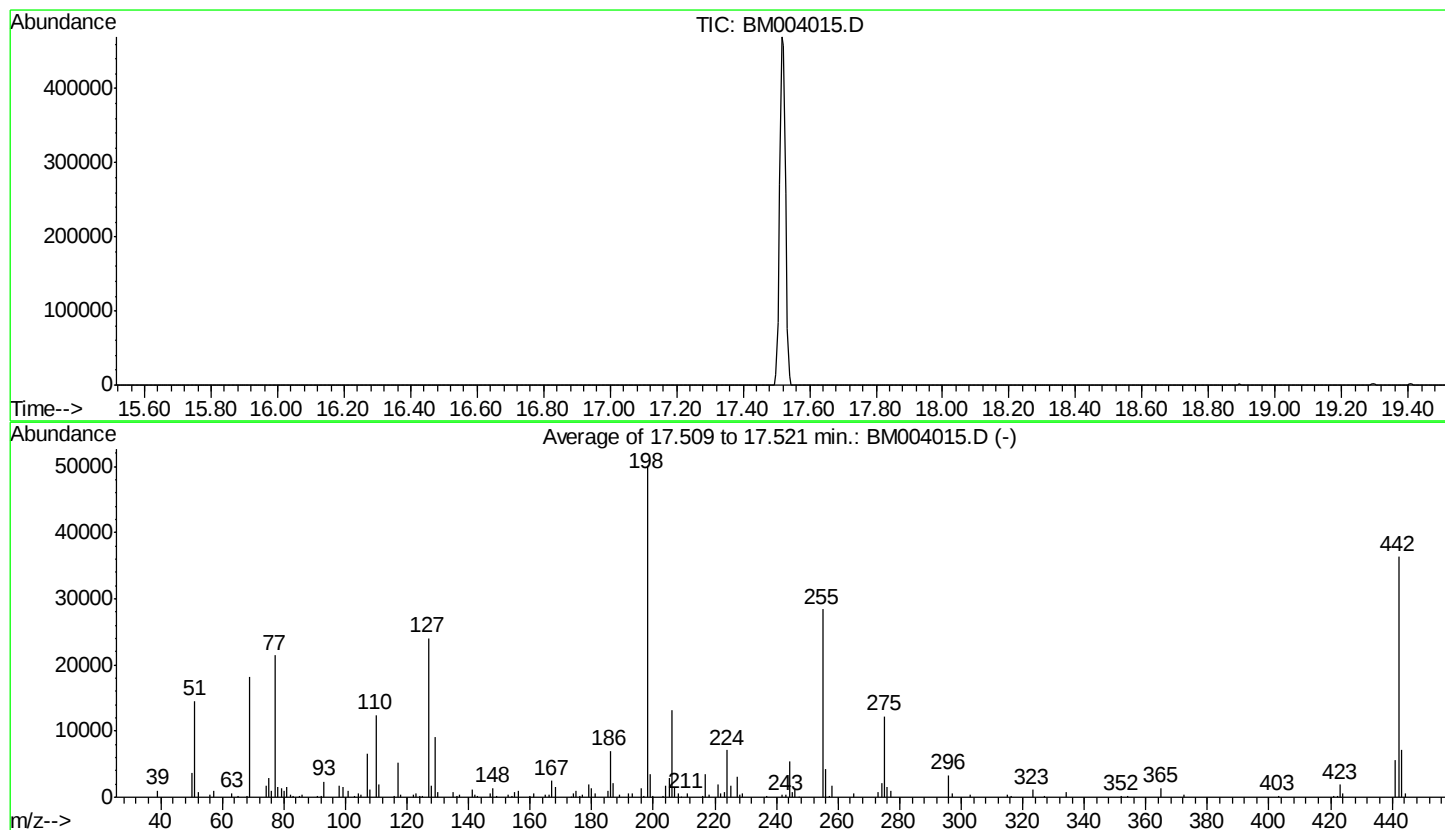

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	14616	PASS
68	69	0.00	2	0.6	115	PASS
69	198	0.00	100	36.3	18187	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	24080	PASS
197	198	0.00	2	0.4	216	PASS
198	198	100	100	100.0	50154	PASS
199	198	5	9	6.9	3450	PASS
275	198	10	60	24.4	12233	PASS
365	198	1	100	2.7	1356	PASS
441	443	0.01	100	78.1	5562	PASS
442	198	50	100	72.4	36333	PASS
443	442	15	24	19.6	7123	PASS

m/z	Abundance
39.10	850.0
50.10	3145.0
51.10	11883.0
52.10	620.0
56.00	398.0
57.00	862.0
63.10	602.0
69.00	14513.0
74.00	1390.0
75.00	2252.0
76.10	762.0
77.10	17000.0
78.10	1207.0
79.00	1160.0
80.00	831.0
81.00	1214.0
82.00	325.0
86.00	348.0
93.00	1854.0
98.00	1362.0
99.00	1396.0
101.00	676.0
104.00	384.0
105.00	361.0
107.00	5014.0
108.10	829.0
110.00	9442.0
111.00	1485.0
117.00	3971.0
118.00	352.0
123.00	475.0
127.00	17840.0
128.00	1335.0
129.00	7000.0
130.00	529.0
135.00	539.0
137.00	323.0
141.00	878.0
142.10	305.0
147.00	499.0
148.00	1093.0
153.00	301.0
155.00	478.0
156.00	766.0
161.00	358.0
165.00	364.0
166.00	339.0
167.00	1771.0
168.00	1213.0
174.00	390.0
175.00	703.0
179.00	1252.0
180.00	930.0
181.00	461.0
185.00	637.0
186.10	4984.0
187.00	1454.0
189.00	332.0
192.00	395.0
193.00	417.0
196.00	981.0
198.00	34400.0
199.00	2536.0
204.10	1288.0
205.00	2052.0
206.10	9308.0
207.10	1501.0
208.00	391.0
211.00	339.0
217.00	2299.0
218.00	350.0
221.10	1321.0
221.80	314.0
223.00	552.0
224.10	4714.0
225.00	1258.0
227.00	2109.0
228.00	311.0
229.00	421.0
244.10	3552.0
245.10	459.0
246.00	719.0
255.10	18408.0
256.10	2676.0
258.00	1047.0
265.10	449.0
273.00	577.0
274.00	1404.0
275.10	7613.0
276.00	1004.0
277.10	715.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38

296.00	1996.0
297.00	340.0
323.10	625.0
334.10	469.0
365.00	687.0
423.10	962.0
424.10	331.0
441.10	2851.0
442.10	18088.0
443.10	3841.0
444.10	315.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38

m/z	Abundance
39.10	1240.0
50.10	4255.0
51.10	17272.0
52.00	898.0
56.00	518.0
57.00	1233.0
63.00	762.0
65.00	360.0
68.00	346.0
69.00	21600.0
74.10	2148.0
75.00	3470.0
76.10	1214.0
77.10	25160.0
78.10	1901.0
79.00	1560.0
80.00	1198.0
81.00	1835.0
82.00	431.0
83.00	429.0
85.00	377.0
86.00	501.0
91.00	455.0
92.00	470.0
93.00	2804.0
98.00	2044.0
99.00	1878.0
101.00	1060.0
102.90	326.0
104.00	685.0
105.00	490.0
107.00	7772.0
108.00	1285.0
110.00	14638.0
111.00	2292.0
116.00	406.0
117.00	6099.0
118.00	508.0
122.00	511.0
123.00	729.0
124.00	365.0
125.00	381.0
127.10	28824.0
128.00	2239.0
129.00	10632.0
130.00	923.0
135.00	913.0
136.00	404.0
137.10	492.0
141.00	1288.0
142.00	455.0
143.00	356.0
147.00	731.0
148.00	1506.0
148.90	372.0
153.00	398.0
154.00	345.0
155.00	834.0
156.10	1229.0
160.00	424.0
161.00	647.0
165.00	598.0
166.00	461.0
167.10	2909.0
168.00	1742.0
173.00	310.0
174.00	592.0
175.10	1083.0
176.00	327.0
177.00	522.0
179.00	2248.0
180.00	1681.0
181.00	717.0
185.00	1094.0
186.00	8237.0
187.10	2413.0
189.10	553.0
192.00	694.0
193.10	762.0
196.00	1685.0
197.10	350.0
198.00	59200.0
199.00	3997.0
200.00	309.0
203.00	399.0
204.10	2094.0
205.10	3598.0
206.10	15214.0
207.00	2323.0
208.00	593.0
208.90	307.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38

211.00	672.0
216.00	315.0
217.00	4027.0
218.00	539.0
221.00	2267.0
221.80	642.0
223.00	910.0
224.10	8383.0
225.10	2161.0
227.00	3546.0
228.00	495.0
229.00	626.0
237.00	346.0
242.00	471.0
243.10	483.0
244.10	6291.0
245.10	848.0
246.00	1247.0
247.00	304.0
255.10	33360.0
256.10	4997.0
257.10	361.0
258.10	1986.0
265.00	737.0
273.00	983.0
274.10	2528.0
275.10	14311.0
276.00	1820.0
277.00	1233.0
296.00	3955.0
297.00	572.0
303.10	456.0
315.00	406.0
323.10	1299.0
334.00	728.0
352.10	310.0
354.10	414.0
365.10	1515.0
372.20	563.0
403.00	328.0
421.10	304.0
422.10	313.0
423.10	2018.0
424.10	667.0
441.10	6235.0
442.10	40392.0
443.10	7802.0
444.10	734.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38

m/z	Abundance
39.10	1122.0
50.10	3641.0
51.10	14695.0
52.00	715.0
56.00	491.0
57.00	1061.0
63.00	599.0
65.00	331.0
69.00	18448.0
74.00	1912.0
75.00	3092.0
76.10	1055.0
77.10	22248.0
78.10	1526.0
79.10	1352.0
80.00	1023.0
81.00	1511.0
82.00	335.0
83.00	338.0
85.00	417.0
86.00	397.0
91.00	374.0
92.00	423.0
93.00	2412.0
98.00	1907.0
99.00	1548.0
101.00	904.0
104.00	598.0
105.00	525.0
107.00	6975.0
108.00	1126.0
110.00	13380.0
111.00	1976.0
116.00	351.0
117.00	5633.0
118.00	432.0
122.00	470.0
123.00	716.0
125.00	365.0
127.10	25576.0
128.00	1914.0
129.00	9748.0
130.00	807.0
135.00	838.0
137.00	430.0
141.00	1238.0
142.00	431.0
147.00	692.0
148.00	1590.0
149.00	339.0
153.00	440.0
154.00	323.0
155.00	844.0
156.00	1160.0
160.00	369.0
161.00	664.0
165.00	506.0
166.00	358.0
167.00	2774.0
168.00	1581.0
174.00	606.0
175.10	1139.0
176.00	368.0
177.00	551.0
179.00	2054.0
180.00	1436.0
181.00	793.0
185.10	1007.0
186.10	7959.0
187.00	2262.0
189.00	508.0
192.00	705.0
193.00	798.0
196.00	1588.0
196.90	300.0
198.00	56864.0
199.00	3819.0
200.00	333.0
203.00	408.0
204.00	2118.0
205.10	3372.0
206.10	15186.0
207.10	2123.0
208.10	498.0
211.00	539.0
216.00	342.0
217.00	4064.0
218.00	523.0
221.00	2243.0
221.90	554.0
223.00	1068.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38

224.10	8368.0
225.00	2048.0
227.10	3437.0
228.00	522.0
229.00	708.0
237.00	327.0
242.00	439.0
243.10	455.0
244.10	6322.0
245.00	815.0
246.00	1352.0
255.10	33392.0
256.10	4898.0
257.00	364.0
258.00	2090.0
265.00	703.0
273.00	954.0
274.10	2714.0
275.10	14775.0
276.10	1927.0
277.00	1221.0
296.10	4007.0
297.10	639.0
303.10	480.0
315.00	516.0
316.10	325.0
323.10	1402.0
327.00	330.0
334.10	868.0
352.10	357.0
354.10	458.0
365.10	1868.0
372.10	658.0
403.10	454.0
421.10	314.0
422.10	385.0
423.10	2593.0
424.10	606.0
441.10	7602.0
442.10	50520.0
443.10	9727.0
444.10	850.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38

m/z	Abundance
207.00	337.0

Instrument :
BNA_M
ClientSampleId :
DFTPP38