


Data Path : Z:\HPCHEM1\BNA M\DATA\BM011518\
Data File : BM013594.D
Acq On : 15 Jan 2018 20:30
Operator : SJ/JU
Sample : J1079-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
DAJK4

Manual Integrations
APPROVED

Sohil
1/16/2018 5:06:07 PM

Quant Time: Jan 16 04:21:40 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 16 03:03:13 2018
Response via : Initial Calibration

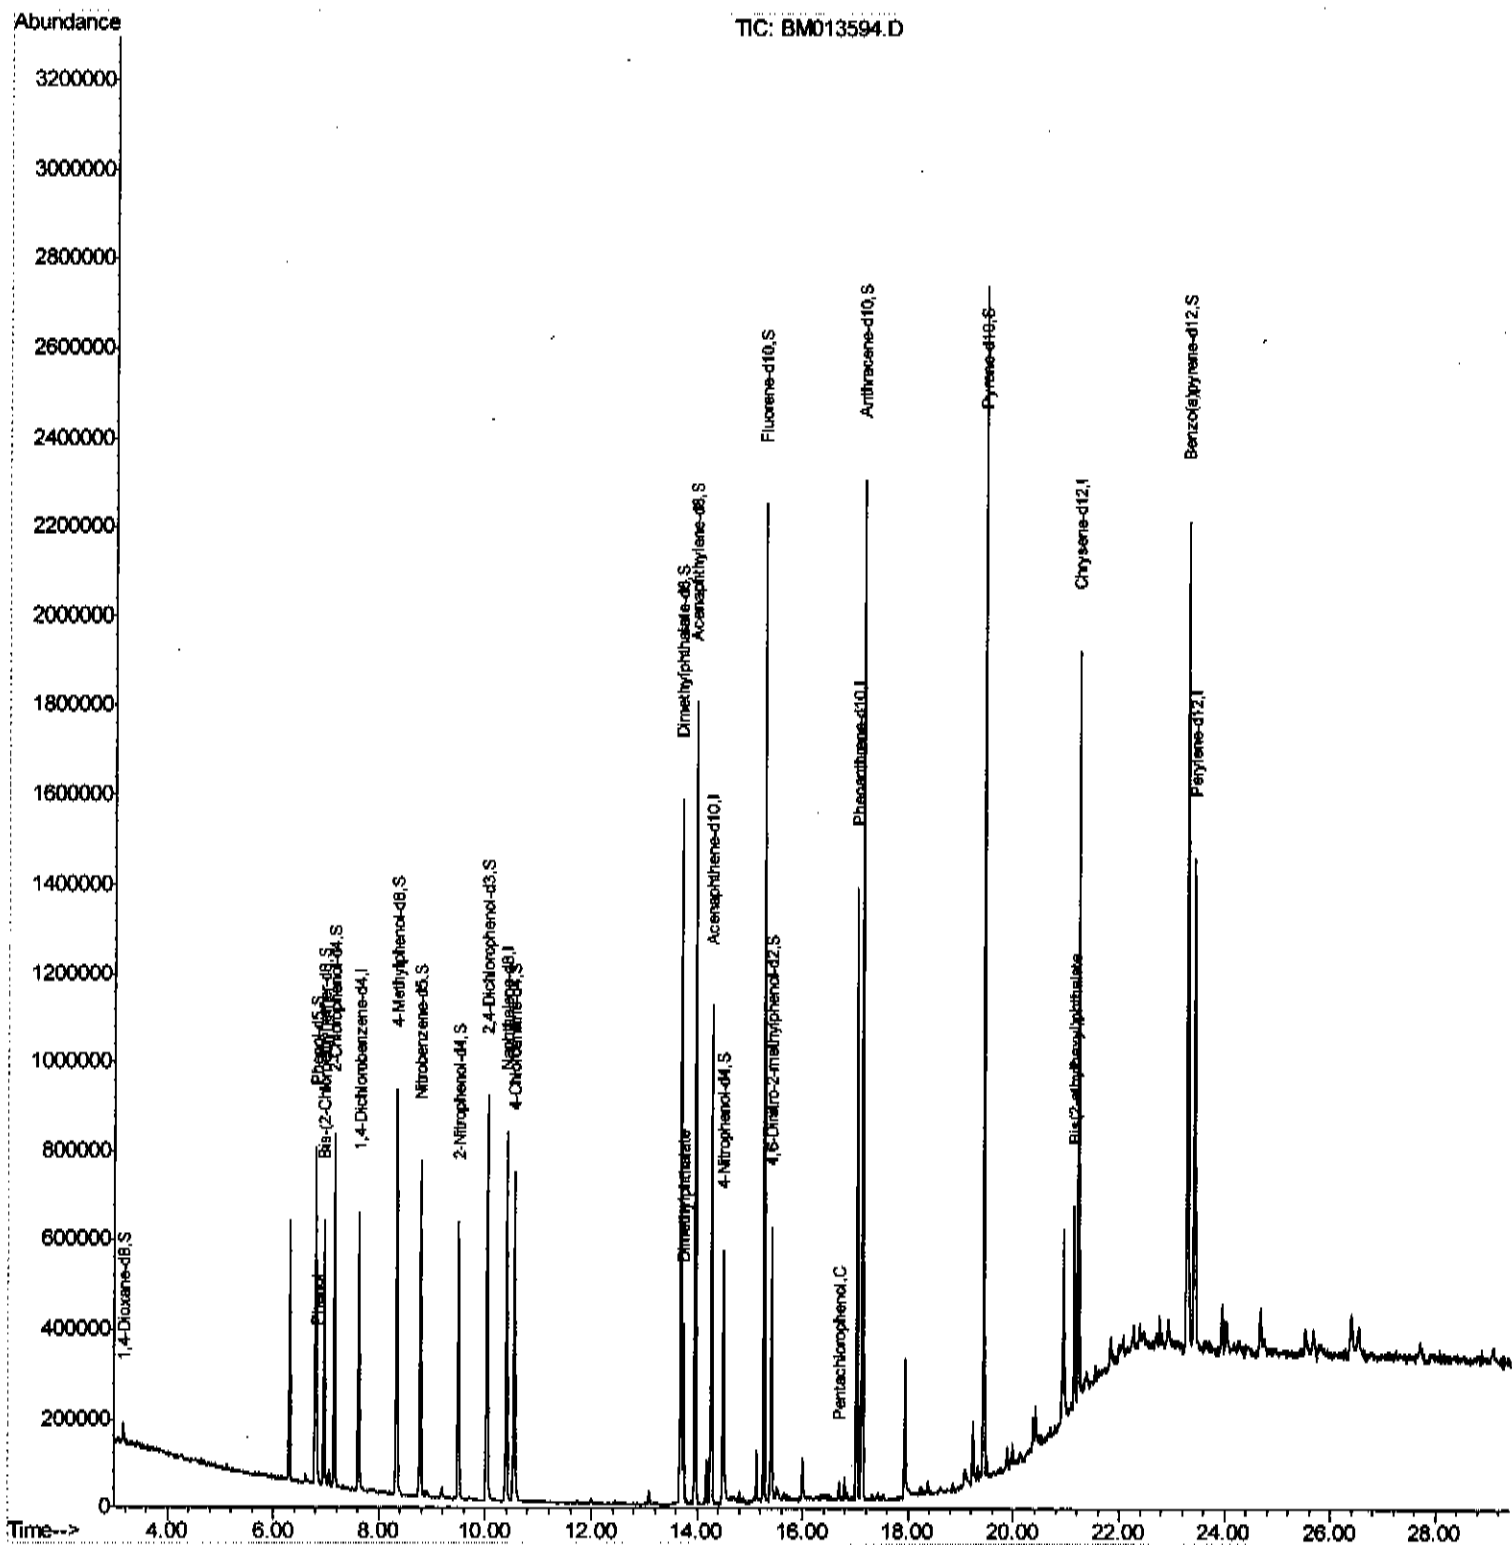


Data Path : Z:\HPCHEM1\BNA M\DATA\BM011518\
 Data File : BM013594.D
 Acq On : 15 Jan 2018 20:30
 Operator : SJ/JU
 Sample : J1079-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DAJK4

Manual Integrations
 APPROVED

Sohil
 1/16/2018 5:06:07 PM

Quant Time: Jan 16 03:10:47 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 16 03:03:13 2018
 Response via : Initial Calibration

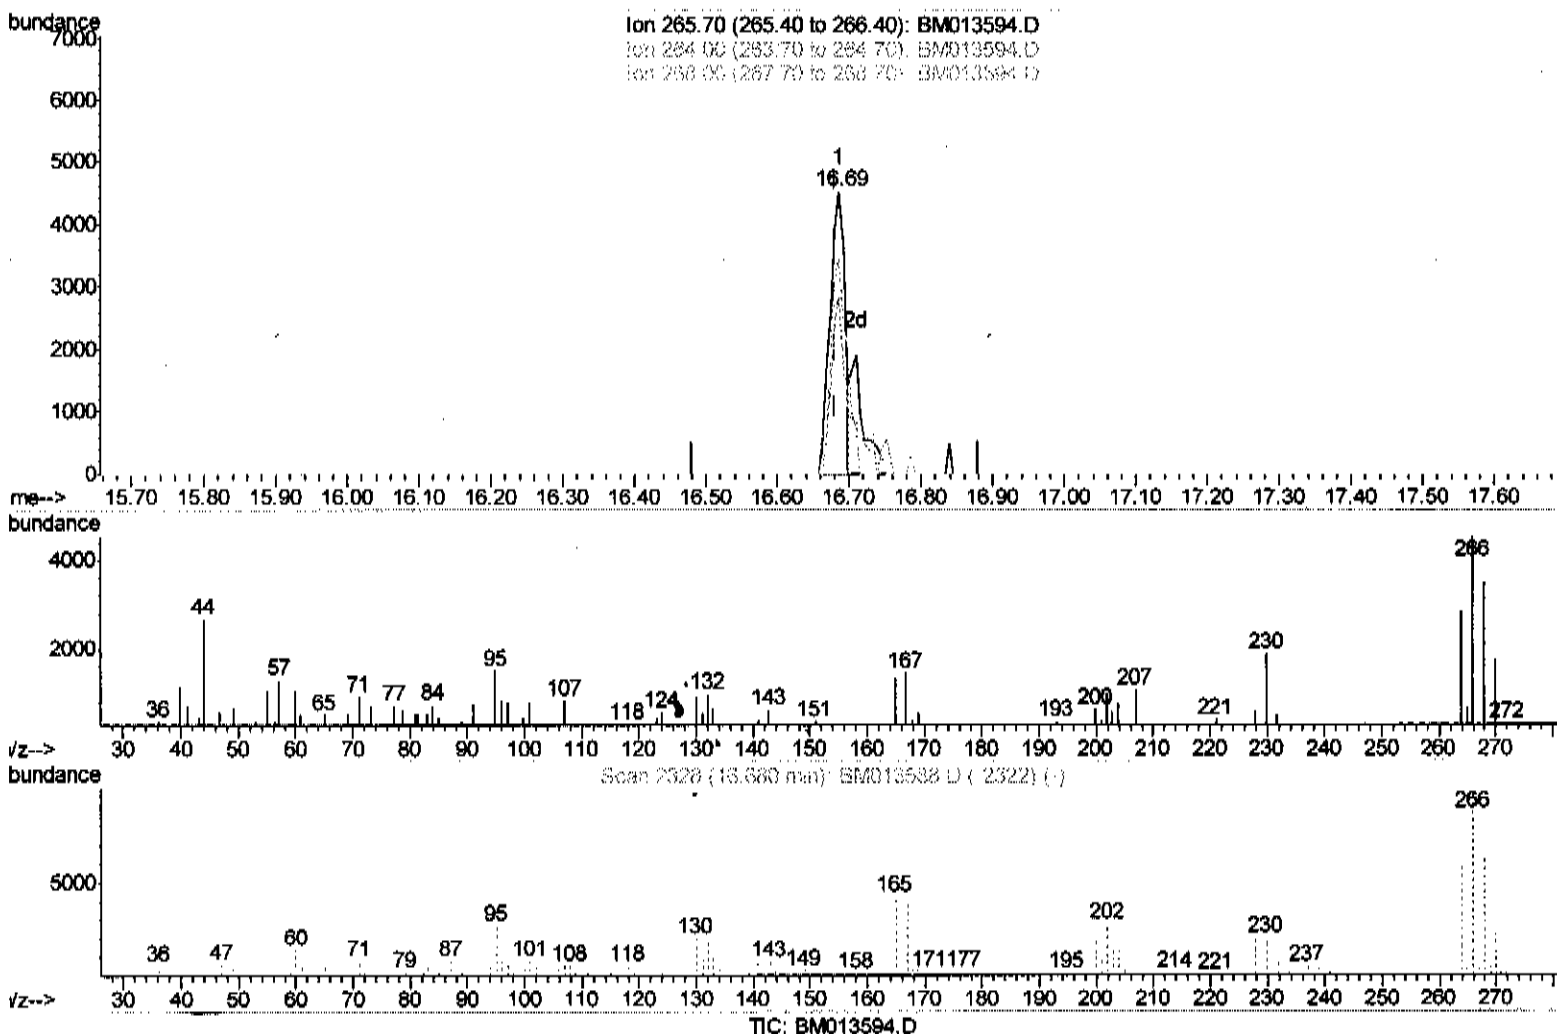

(68) Pentachlorophenol (C)

16.666min (+0.006) 1.27ng/ul

response 6486

Ion	Exp%	Act%
265.70	100	100
264.00	61.60	63.27
268.00	65.70	77.01
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA M\DATA\BM011518\
 Data File : BM013594.D
 Acq On : 15 Jan 2018 20:30
 Operator : SJ/JU
 Sample : J1079-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DAJK4

Manual Integrations
 APPROVED

Sohil
 1/16/2018 5:06:07 PM

Quant Time: Jan 16 03:10:47 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 16 03:03:13 2018
 Response via : Initial Calibration

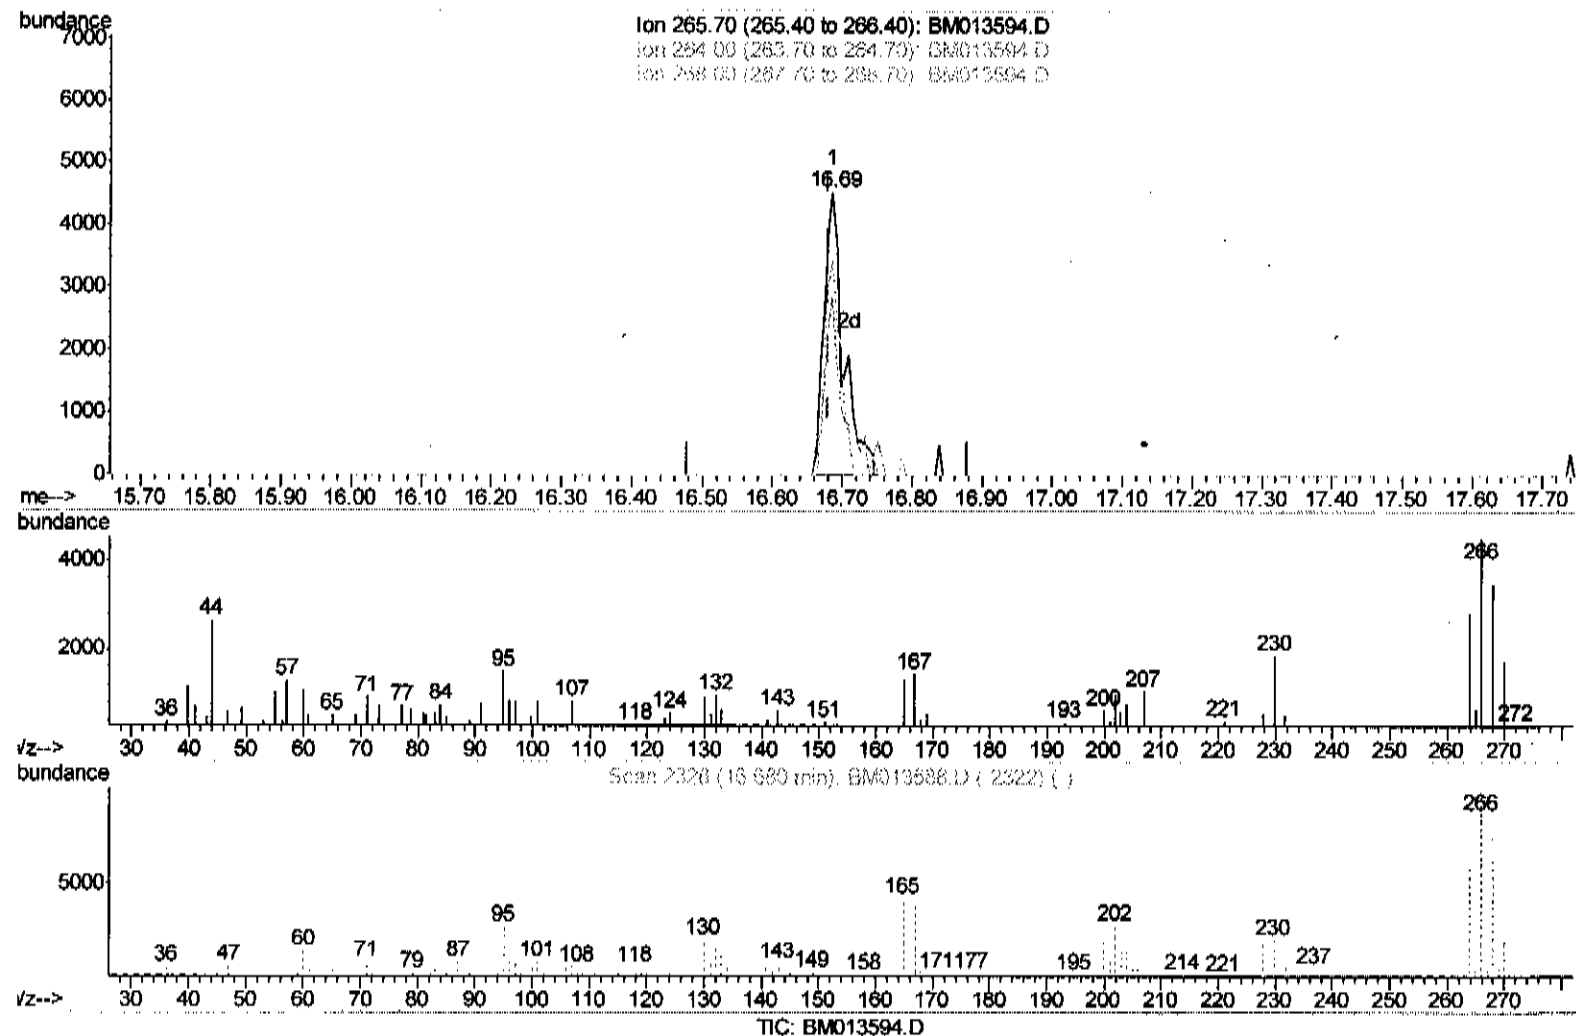

(68) Pentachlorophenol (C)

16.686min (+0.006) 1.75ng/ul *mg/L 01/17/18*

response 8919

Ion	Exp%	Act%
265.70	100	100
264.00	61.60	63.27
268.00	65.70	77.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011518\
 Data File : BM013594.D
 Acq On : 15 Jan 2018 20:30
 Operator : SJ/JU
 Sample : J1079-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DAJK4

Manual Integrations
 APPROVED

Sohil
 1/16/2018 5:06:07 PM

Quant Time: Jan 16 04:21:40 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 16 03:03:13 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	159056	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	644662	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	351471	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	753535	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	778238	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	760504	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	21464	5.33	ng/uL	0.00
5) Phenol-d5	6.80	99	400783	32.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	244085	32.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	329744	33.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	326502	34.78	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	167408	33.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	175135	33.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	330282	32.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	388207	43.82	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	970276	33.50	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	1262064	34.16	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	138743	29.47	ng/ul	0.00
57) Fluorene-d10	15.27	176	816322	32.04	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	124221	27.39	ng/ul	0.00
70) Anthracene-d10	17.12	188	1204917	32.83	ng/ul	0.00
76) Pyrene-d10	19.42	212	1310644	36.17	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1223059	34.99	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)	Ovalue
6) Phenol	6.83	94	56758	4.634	ng/ul#	88	
44) Dimethylphthalate	13.73	163	229272	8.050	ng/ul	99	
68) Pentachlorophenol	16.69	266	8919m	1.752	ng/ul		
81) Bis(2-ethylhexyl)phthalate	21.14	149	148406	5.935	ng/ul#	96	

Handwritten note: 24 01/17/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed