

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_M\DATA\BM011518\
 Data File : BM013607.D
 Acq On : 16 Jan 2018 04:17
 Operator : SJ/JU
 Sample : J1080-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DAJL5

Quant Time: Jan 16 07:19:31 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 16 07:13:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	131256	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	514035	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	296542	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	681927	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	797031	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	799579	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	16523	4.98	ng/uL	0.00
5) Phenol-d5	6.80	99	314860	31.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	193524	31.70	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	258147	31.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	259676	33.52	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	130447	32.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	137302	32.58	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	250345	30.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	299882	42.45	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	811244	33.19	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	1036605	33.26	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	112027	28.20	ng/ul	0.00
57) Fluorene-d10	15.27	176	720245	33.51	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	102773	25.04	ng/ul	0.00
70) Anthracene-d10	17.12	188	1114075	33.54	ng/ul	0.00
76) Pyrene-d10	19.42	212	1283042	34.57	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1336669	36.37	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Phenol	6.82	94	31370	3.104	ng/ul#	88
44) Dimethylphthalate	13.73	163	170121	7.079	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_M\DATA\BM011518\
Data File : BM013607.D
Acq On : 16 Jan 2018 04:17
Operator : SJ/JU
Sample : J1080-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DAJL5

Quant Time: Jan 16 07:19:31 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 16 07:13:29 2018
Response via : Initial Calibration

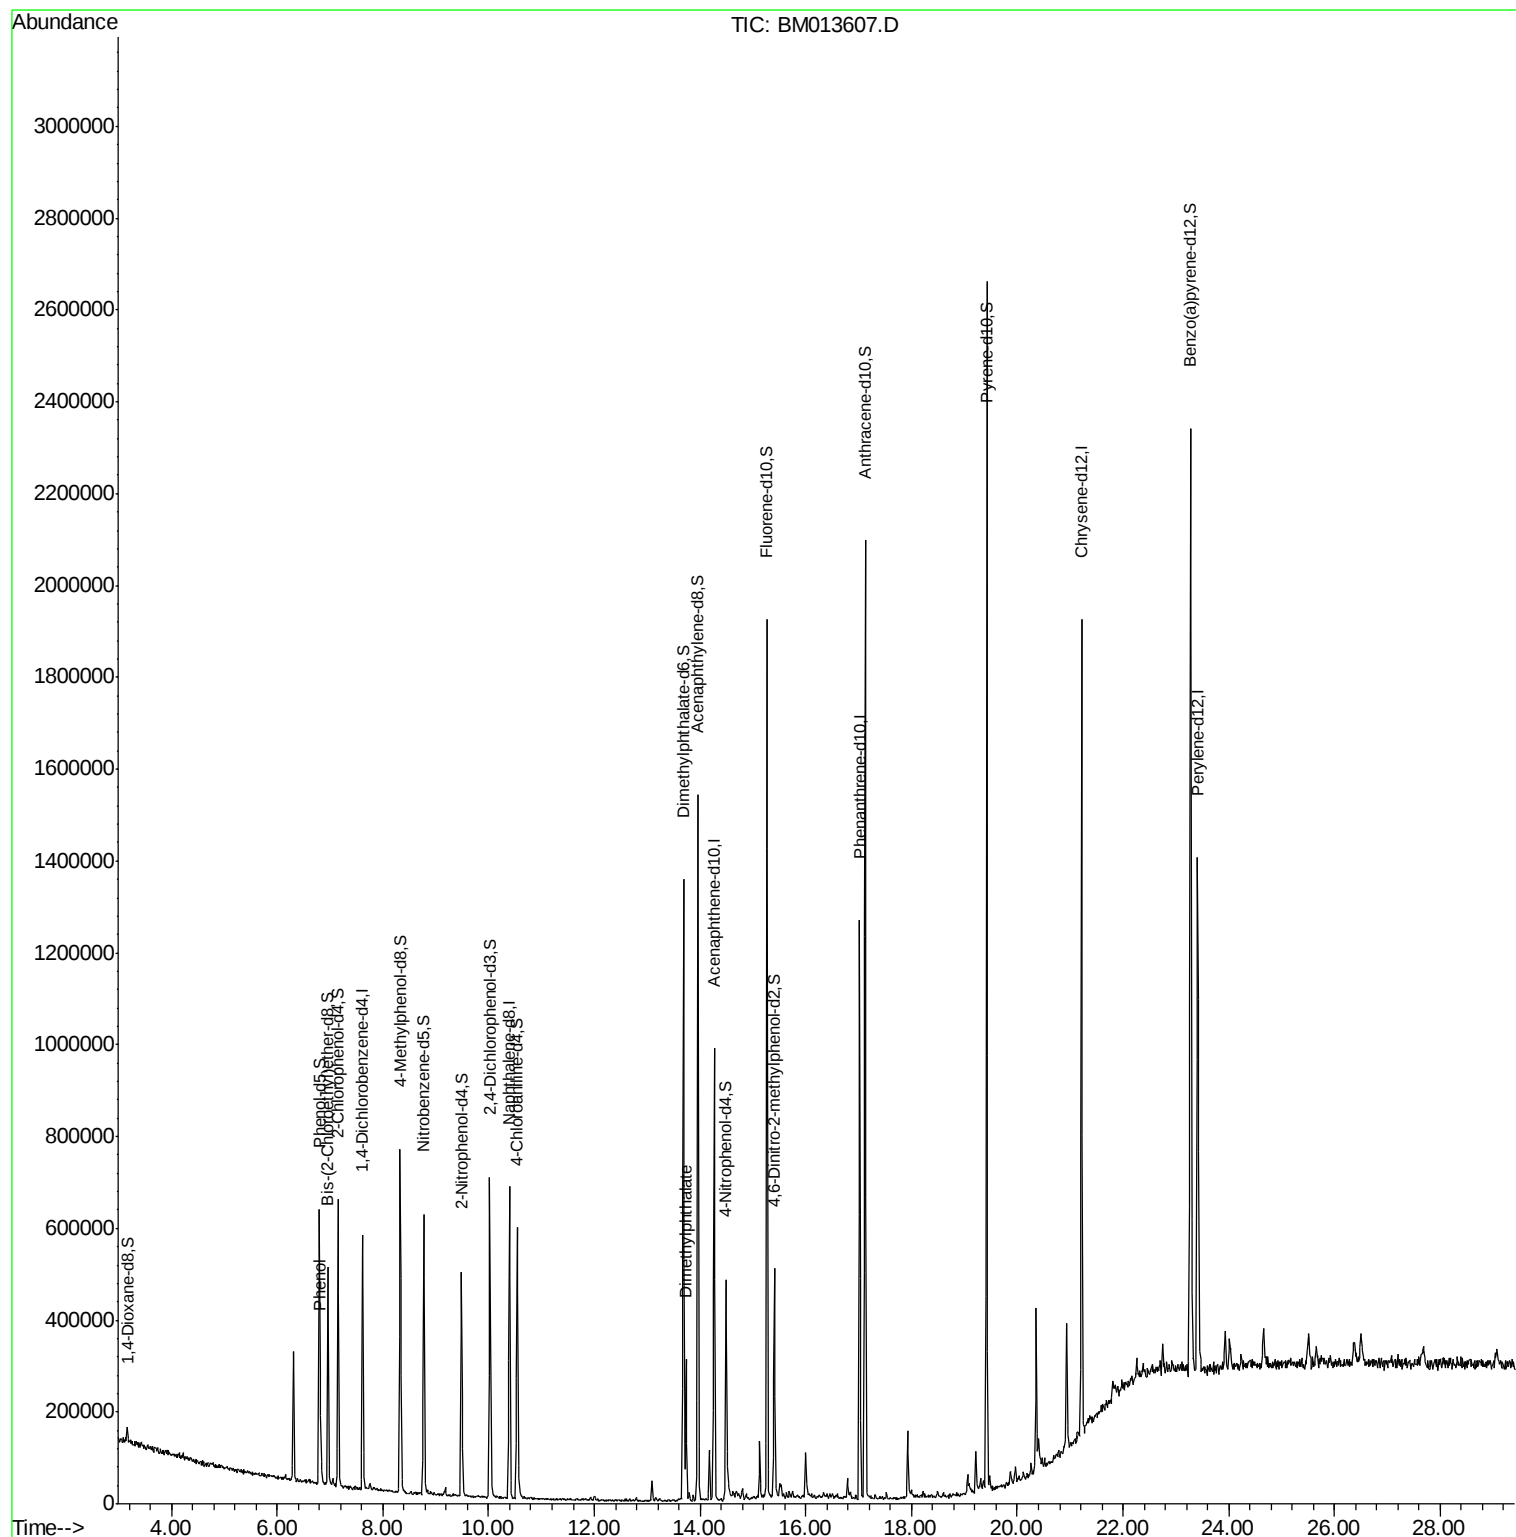

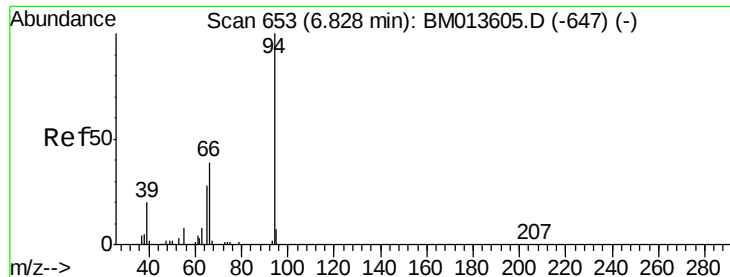

#6

Phenol

Concen: 3.104 ng/ul

RT: 6.82 min Scan# 652

Delta R.T. -0.01 min

Lab File: BM013607.D

Acq: 16 Jan 2018 04:17

Instrument :

BNA_M

ClientSampleId :

DAJL5


Tgt Ion: 94 Resp: 31370

Ion Ratio Lower Upper

94 100

65 33.6 28.2 42.4




66 45.7 47.2 70.8#

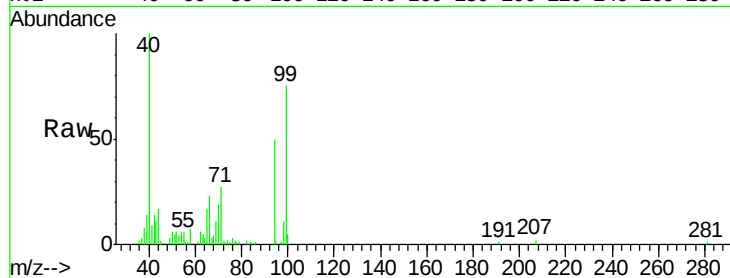

Abundance Ion 94.00 (93.70 to 94.70): BM013607.D (-619) (-)

Ion 65.00 (64.70 to 65.70): BM013607.D (-619) (-)

Ion 66.00 (65.70 to 66.70): BM013607.D (-619) (-)

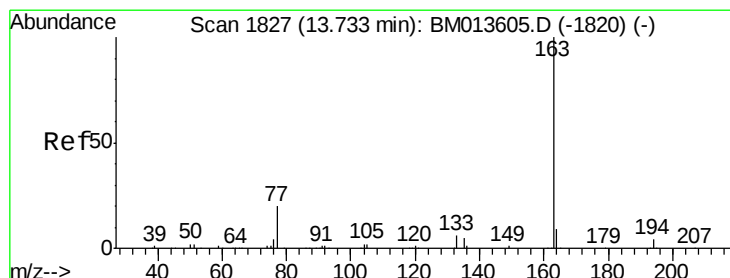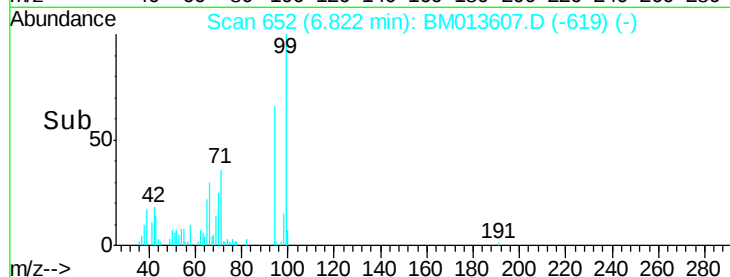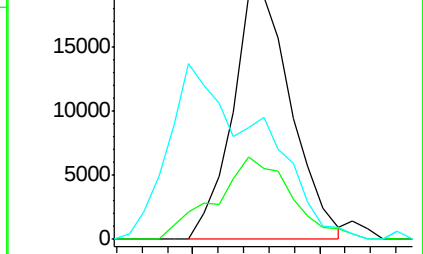

#44

Dimethylphthalate

Concen: 7.079 ng/ul

RT: 13.73 min Scan# 1827

Delta R.T. 0.00 min

Lab File: BM013607.D

Acq: 16 Jan 2018 04:17


Tgt Ion: 163 Resp: 170121

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 8.5 8.2 12.4

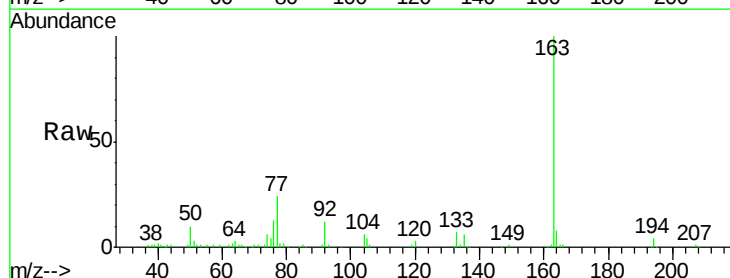

Abundance Ion 163.00 (162.70 to 163.70): BM013607.D (-1793) (-)

Ion 194.00 (193.70 to 194.70): BM013607.D (-1793) (-)

Ion 164.00 (163.70 to 164.70): BM013607.D (-1793) (-)

