

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011615\
 Data File : BM000250.D
 Acq On : 17 Jan 2015 01:42
 Operator : TP/IZ
 Sample : G1065-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 C0AG5

Quant Time: Jan 17 03:06:06 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 17 02:31:22 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	131028	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	543935	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	372142	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	756212	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	821417	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	778502	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	14245	6.30	ng/uL	0.00
5) Phenol-d5	6.99	99	330479	29.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	219182	31.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	252513	31.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	252294	28.77	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	118029	31.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	132709	34.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	252585	29.77	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	328580	34.14	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	856993	31.22	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	987897	30.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	112449	25.17	ng/ul	0.00
57) Fluorene-d10	15.45	176	707375	30.01	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	101573	28.34	ng/ul	0.00
70) Anthracene-d10	17.30	188	1089778	31.17	ng/ul	0.00
76) Pyrene-d10	19.60	212	1187446	31.34	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.53	264	1136284	32.16	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Phenol	7.01	94	30947	2.66	ng/ul	96
44) Dimethylphthalate	13.91	163	99883	3.65	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011615\
Data File : BM000250.D
Acq On : 17 Jan 2015 01:42
Operator : TP/IZ
Sample : G1065-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ClientSampleId :
C0AG5

Quant Time: Jan 17 03:06:06 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jan 17 02:31:22 2015
Response via : Initial Calibration

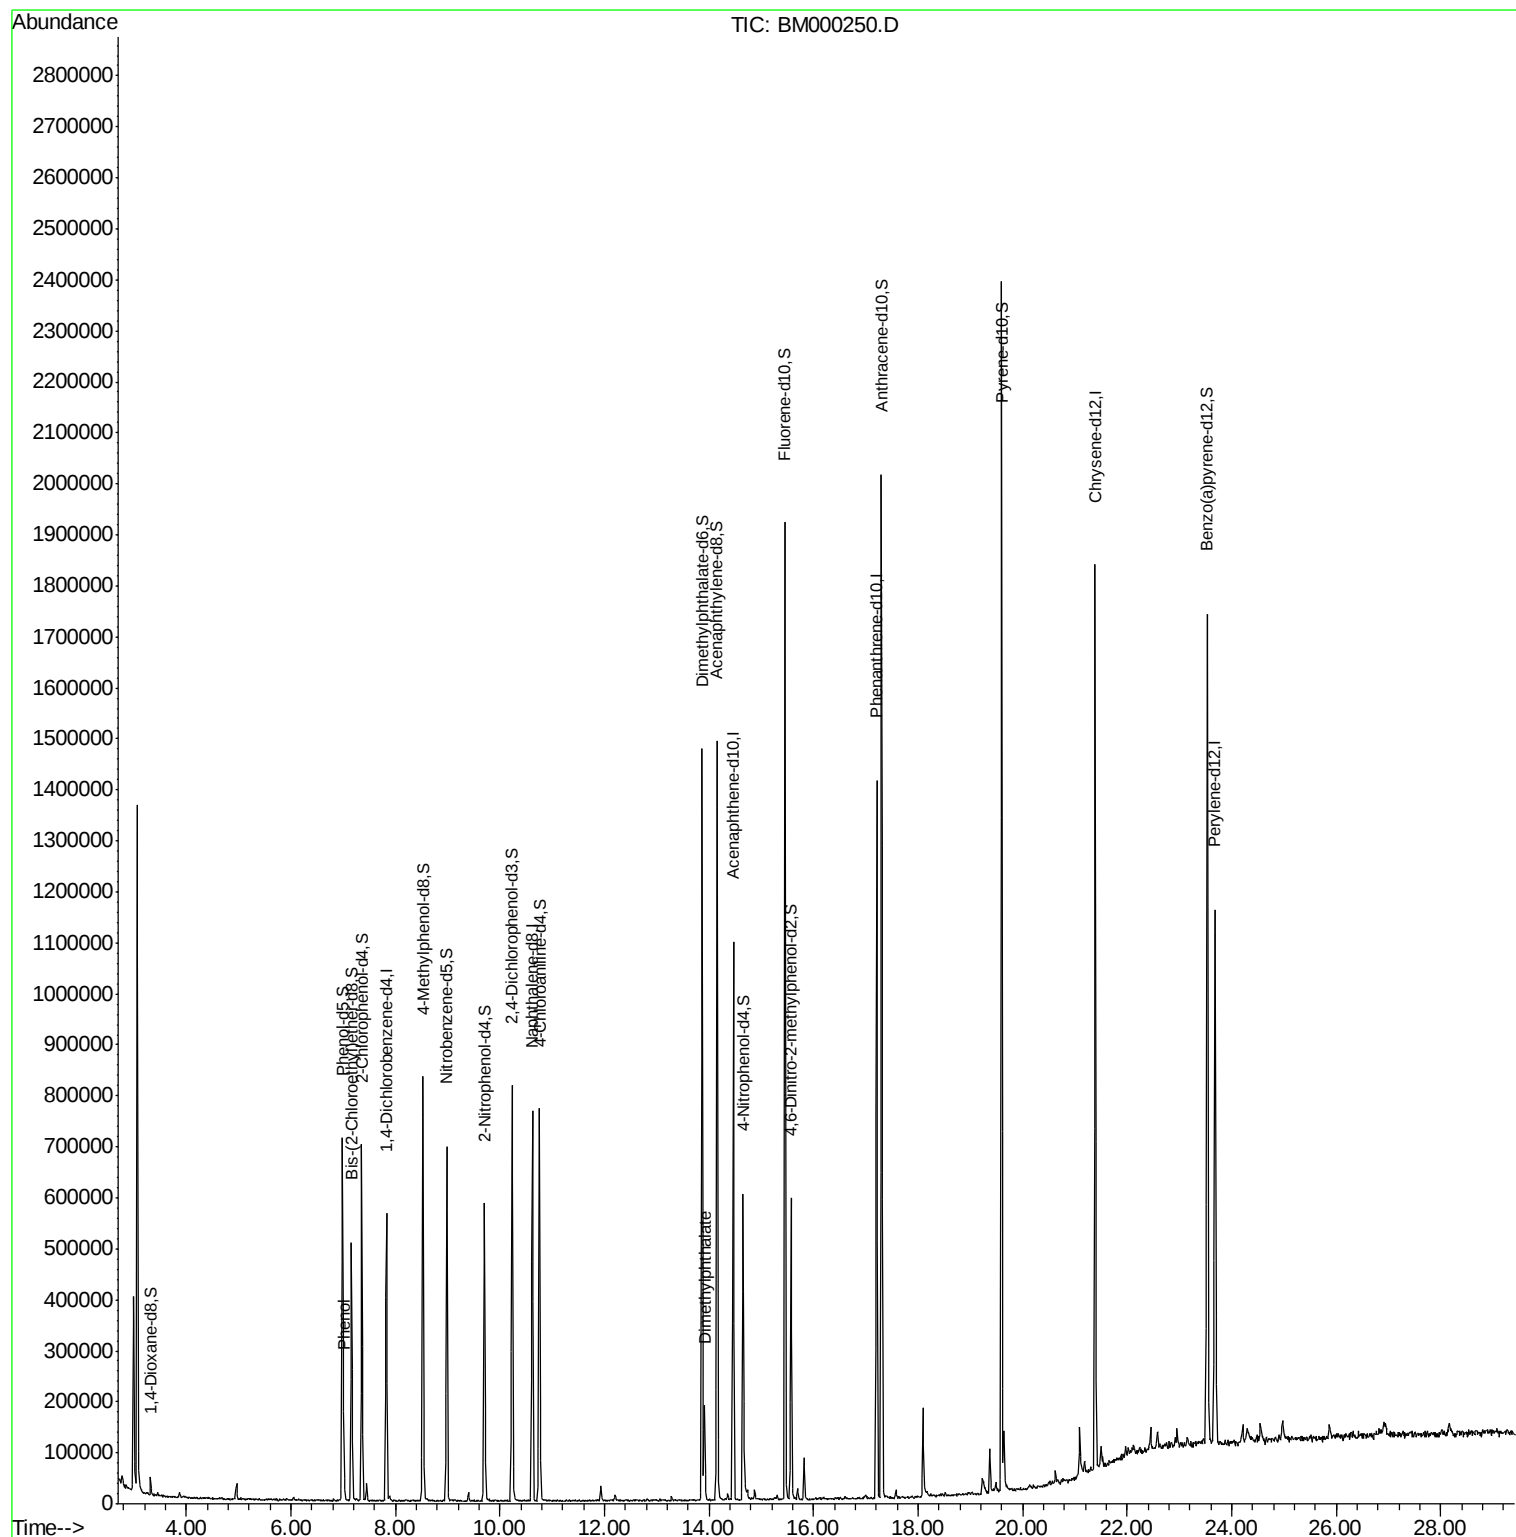

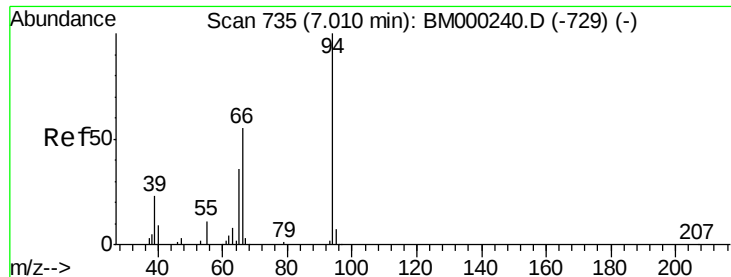

#6

Phenol

Concen: 2.66 ng/ul

RT: 7.01 min Scan# 735

Delta R.T. 0.00 min


Lab File: BM000250.D

Acq: 17 Jan 2015 01:42

Instrument :
ClientSampled :
C0AG5

Tgt Ion: 94 Resp: 30947




Ion	Ratio	Lower	Upper
94	100		
65	37.0	27.4	41.0
66	56.1	42.5	63.7

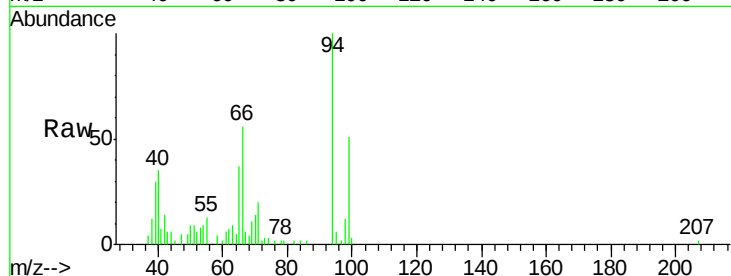

Abundance Ion 94.00 (93.70 to 94.70): BM000240.D (-729) (-)

Ion 65.00 (64.70 to 65.70): BM000240.D (-729) (-)

Ion 66.00 (65.70 to 66.70): BM000240.D (-729) (-)

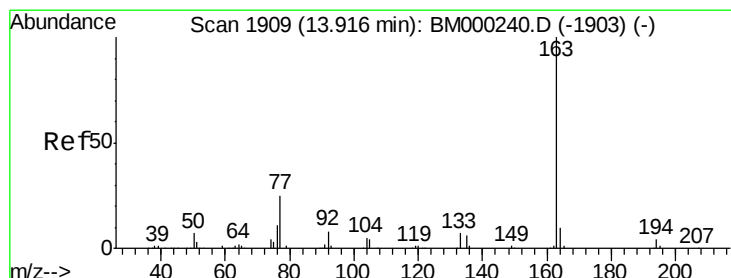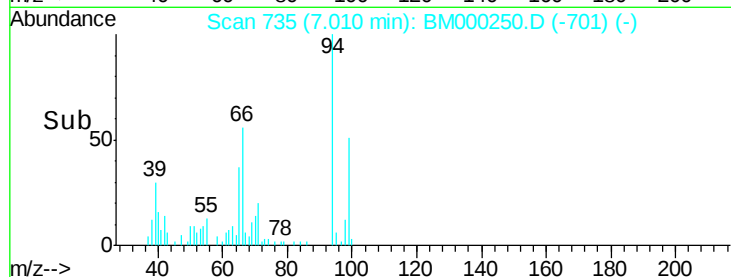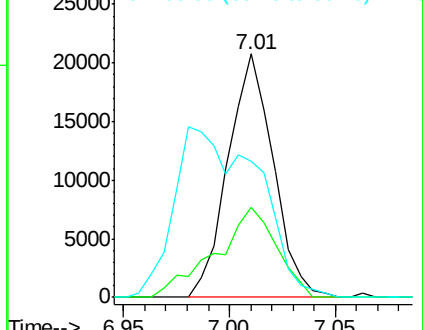

#44

Dimethylphthalate

Concen: 3.65 ng/ul

RT: 13.91 min Scan# 1908


Delta R.T. -0.01 min

Lab File: BM000250.D

Acq: 17 Jan 2015 01:42

Tgt Ion: 163 Resp: 99883

Ion	Ratio	Lower	Upper
163	100		
194	4.5	3.0	4.4#
164	10.7	8.5	12.7

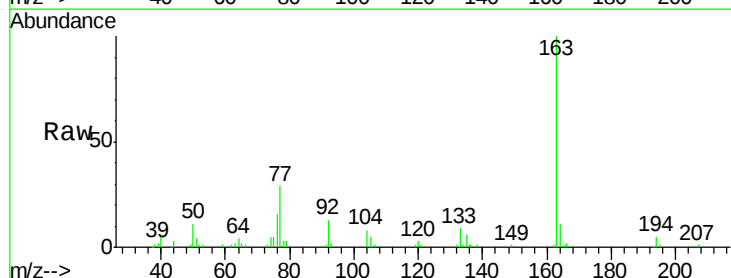

Abundance Ion 163.00 (162.70 to 163.70): BM000240.D (-1903) (-)

Ion 194.00 (193.70 to 194.70): BM000240.D (-1903) (-)

Ion 164.00 (163.70 to 164.70): BM000240.D (-1903) (-)

