


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE011615\
Data File : BE089407.D
Acq On : 16 Jan 2015 23:53
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
LabSampleId :
SSTDCCC001

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BE011615.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 16 22:56:59 2015

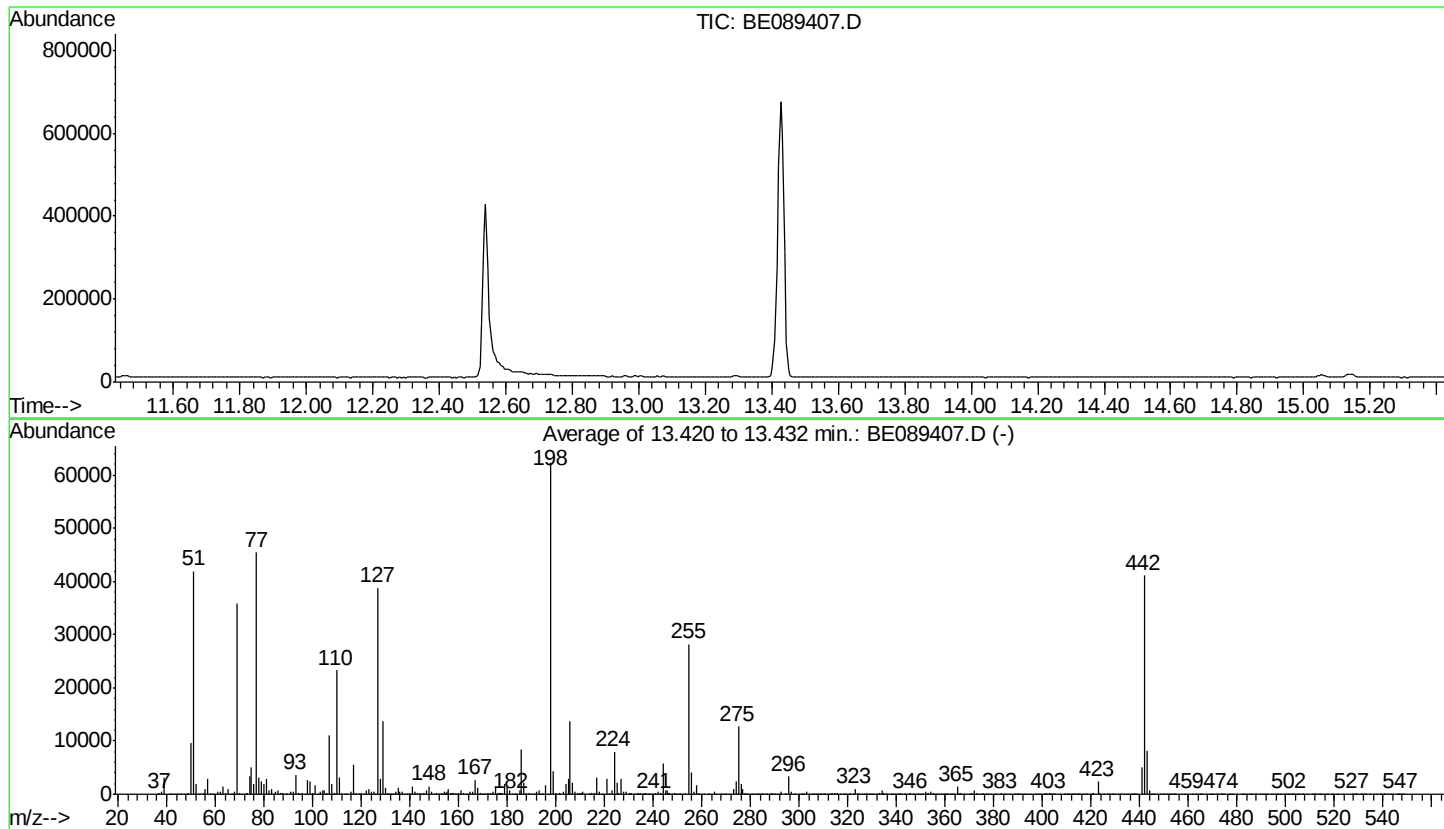

AutoFind: Scans 2048, 2049, 2050; Background Corrected with Scan 2037

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.2	41920	PASS
68	69	0.00	2	1.2	421	PASS
69	198	0.00	100	57.7	35945	PASS
70	69	0.00	2	0.5	178	PASS
127	198	10	80	62.2	38783	PASS
197	198	0.00	2	0.1	85	PASS
198	198	100	100	100.0	62349	PASS
199	198	5	9	7.0	4392	PASS
275	198	10	60	20.3	12684	PASS
365	198	1	100	2.3	1423	PASS
441	442	0.01	24	12.0	4948	PASS
442	198	50	100	65.9	41095	PASS
443	442	15	24	19.7	8087	PASS