


Data Path : Z:\HPCHEM1\BNA_M\Data\BM011615\
 Data File : BM000229.D
 Acq On : 16 Jan 2015 12:15
 Operator : TP/IZ
 Sample : DFTPP09
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 DFTPP09

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Title : SVOA CALIBRATION
 Last Update : Wed Jan 14 12:47:10 2015

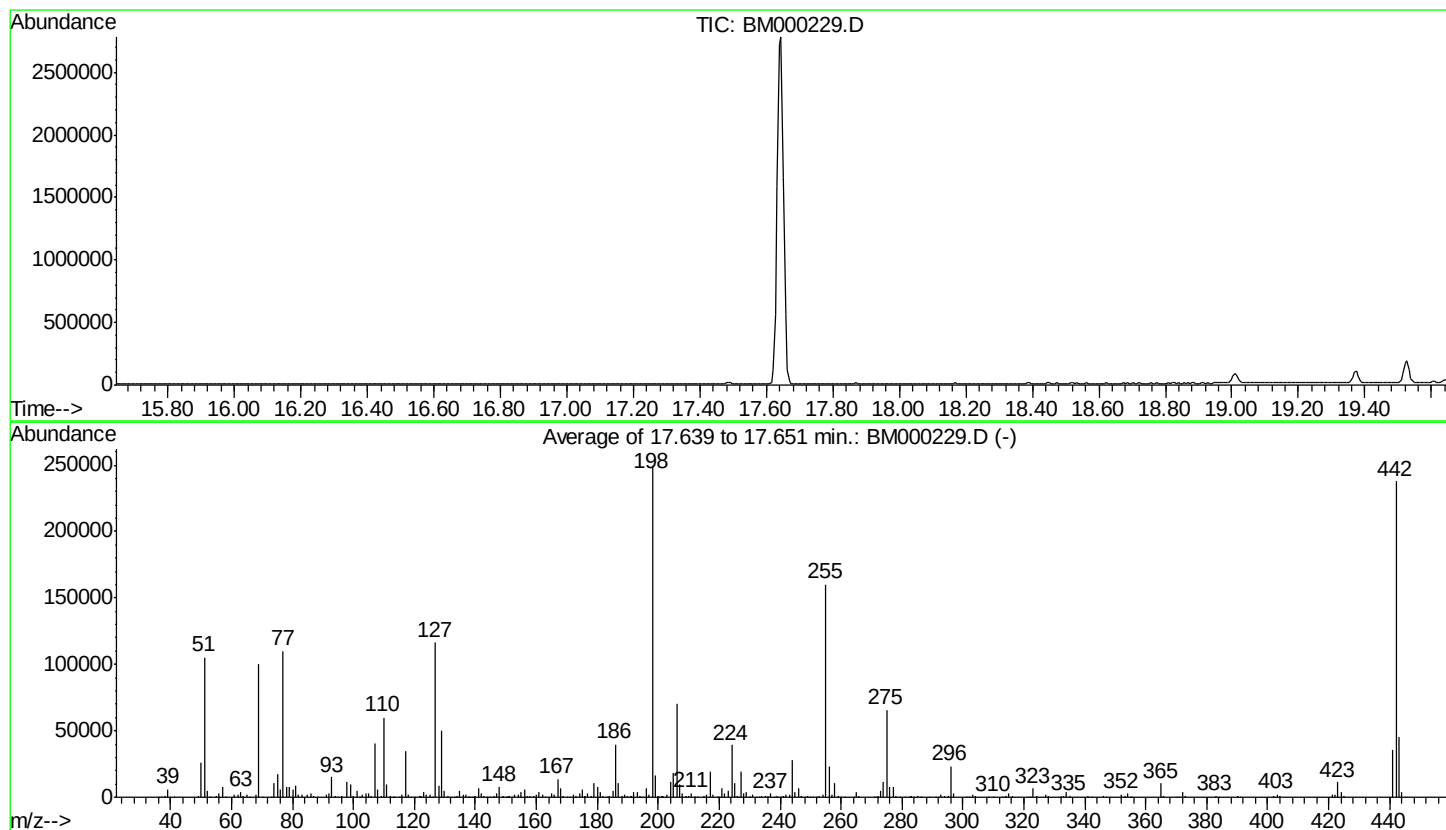

AutoFind: Scans 2542, 2543, 2544; Background Corrected with Scan 2536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	105090	PASS
68	69	0.00	2	1.8	1757	PASS
69	198	0.00	100	40.1	100005	PASS
70	69	0.00	2	0.4	421	PASS
127	198	10	80	46.7	116482	PASS
197	198	0.00	2	0.6	1529	PASS
198	198	100	100	100.0	249557	PASS
199	198	5	9	6.6	16368	PASS
275	198	10	60	26.4	65914	PASS
365	198	1	100	4.2	10575	PASS
441	443	0.01	100	78.9	35530	PASS
442	198	50	100	95.3	237824	PASS
443	442	15	24	18.9	45005	PASS