


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011615\
Data File : BM000249.D
Acq On : 17 Jan 2015 01:06
Operator : TP/IZ
Sample : G1065-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ClientSampleId :
C0AG2

Quant Time: Jan 17 03:13:17 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jan 17 02:31:22 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

TEJASKUMAR
1/19/2015 6:02:27 PM

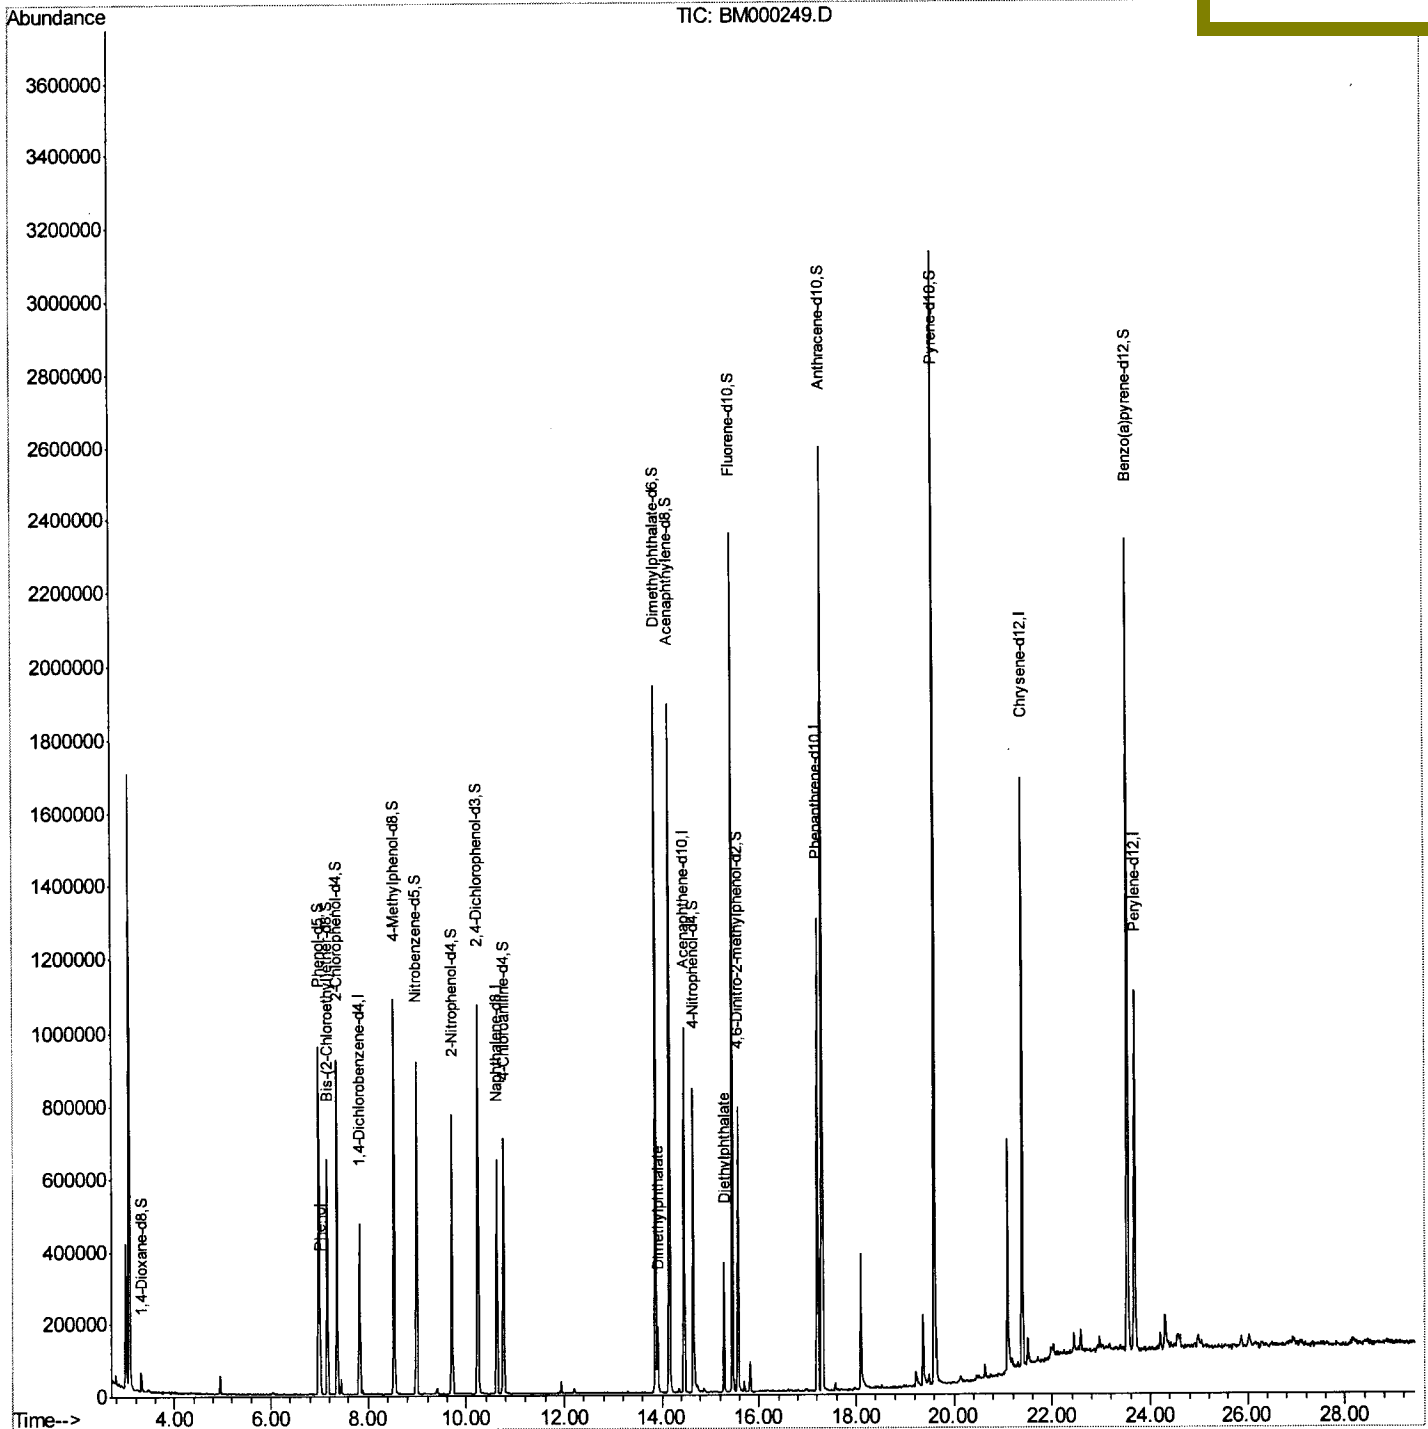

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011615\
 Data File : BM000249.D
 Acq On : 17 Jan 2015 01:06
 Operator : TP/IZ
 Sample : G1065-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 C0AG2

Quant Time: Jan 17 03:13:17 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 17 02:31:22 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

TEJASKUMAR
 1/19/2015 6:02:27 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	108021	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	453288	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	343672	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	695978	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	741355	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	728709	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	19404	10.42	ng/uL	0.00
5) Phenol-d5	6.99	99	441569	48.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	285021	49.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	325548	48.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	331794	45.90	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	160033	51.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	176495	55.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	322007	45.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	293288	36.56	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	1060930	41.86	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	1252235	41.24	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	151664m	36.77	ng/ul	0.00
57) Fluorene-d10	15.45	176	891247	40.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	135213	40.99	ng/ul	0.00
70) Anthracene-d10	17.30	188	1393338	43.29	ng/ul	0.00
76) Pyrene-d10	19.60	212	1491892	43.62	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.53	264	1461055	44.17	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Phenol	7.01	94	38412	4.01	ng/ul#	87
44) Dimethylphthalate	13.92	163	102659	4.07	ng/ul	96
56) Diethylphthalate	15.28	149	177918	6.71	ng/ul	97

} T.P
 01/23/15

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011615\
 Data File : BM000249.D
 Acq On : 17 Jan 2015 01:06
 Operator : TP/IZ
 Sample : G1065-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 C0AG2

Quant Time: Jan 17 03:05:59 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 17 02:31:22 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

TEJASKUMAR
 1/19/2015 6:02:27 PM

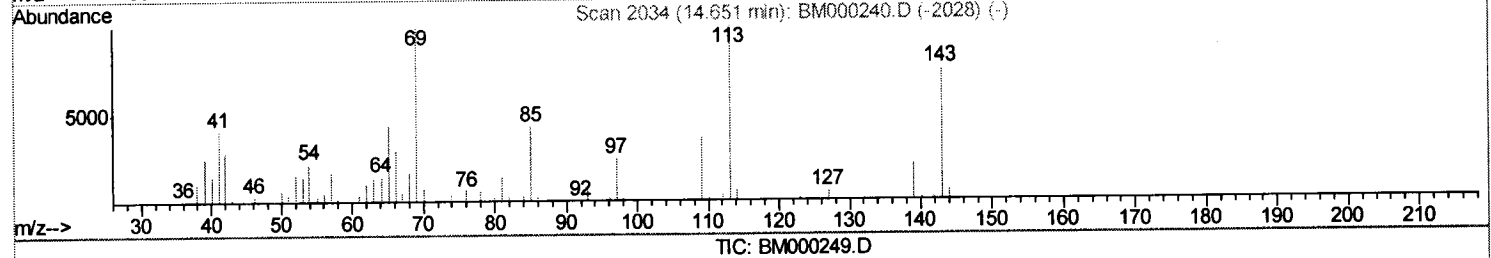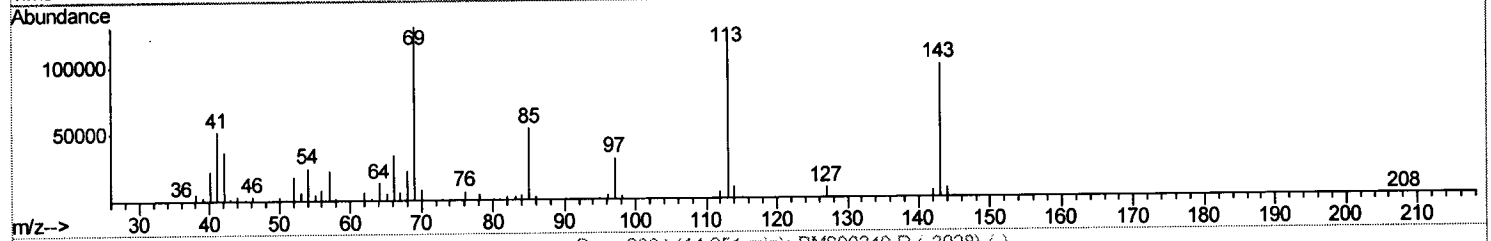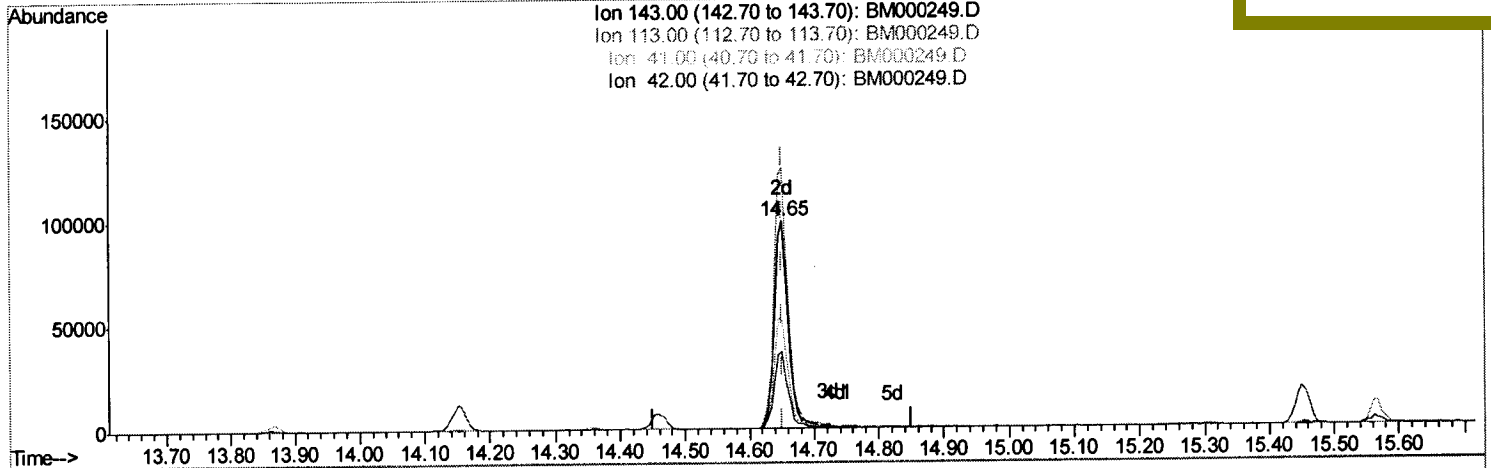

(51) 4-Nitrophenol-d4 (S)

14.651min (+0.000) 36.77ng/ul m

response 151664

Ion	Exp%	Act%
143.00	100	100
113.00	112.90	125.95
41.00	44.00	51.96
42.00	28.90	36.78#

T.P
 01/23/15

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011615\
Data File : BM000249.D
Acq On : 17 Jan 2015 01:06
Operator : TP/IZ
Sample : G1065-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ClientSampleId :
C0AG2

Quant Time: Jan 17 03:05:59 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jan 17 02:31:22 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

TEJASKUMAR
1/19/2015 6:02:27 PM

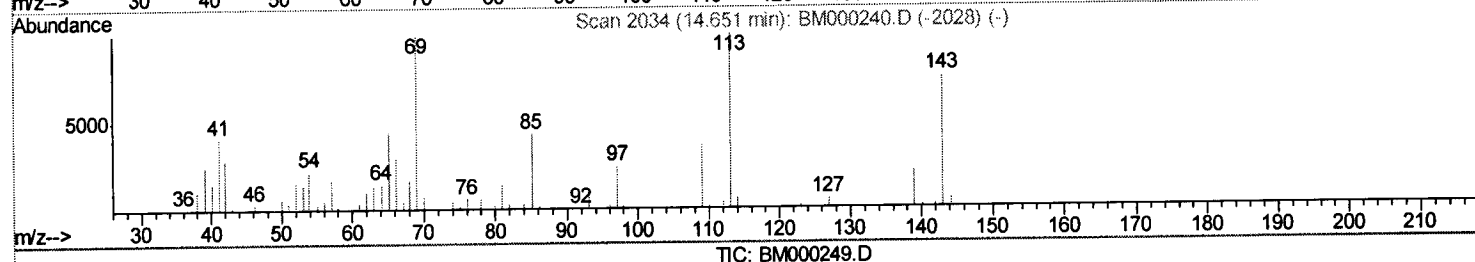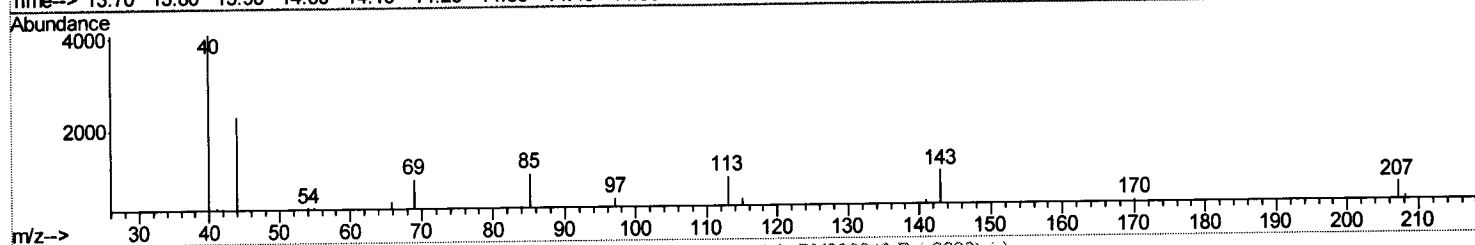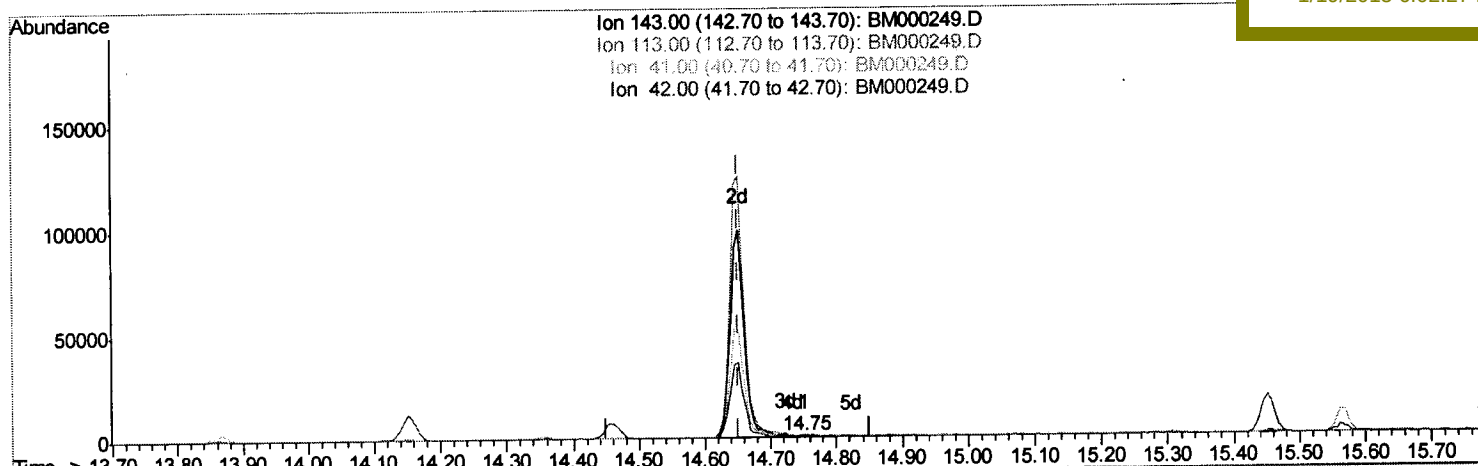

(51) 4-Nitrophenol-d4 (S)

14.751min (+0.100) 0.13ng/ul

response 556

Ion	Exp%	Act%
143.00	100	100
113.00	112.90	91.17
41.00	44.00	35.53
42.00	28.90	32.09