

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011615\
 Data File : BM000243.D
 Acq On : 16 Jan 2015 21:33
 Operator : TP/IZ
 Sample : G1065-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 C0AJ1

Manual Integrations
 APPROVED

TEJASKUMAR
 1/19/2015 6:02:28 PM

Quant Time: Jan 17 02:50:10 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jan 17 02:31:22 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	113261	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	472088	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	334066	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	667675	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	710407	20.00	ng/ul	0.00
83) Perylene-d12	23.69	264	694305	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	17797	9.11	ng/uL	0.00
5) Phenol-d5	6.99	99	381607	40.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	246637	40.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	282302	40.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	290140	38.28	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	136783	41.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	150110	45.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	283352	38.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	358843m	42.95	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	933262	37.88	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	1073639	36.37	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	130654	32.58	ng/ul	0.00
57) Fluorene-d10	15.45	176	770438	36.41	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	118760	37.53	ng/ul	0.00
70) Anthracene-d10	17.30	188	1199922	38.87	ng/ul	0.00
76) Pyrene-d10	19.60	212	1268653	38.71	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.54	264	1263424	40.09	ng/ul	0.00

Target Compounds

						Ovalue
6) Phenol	7.01	94	34916	3.47	ng/ul#	82
44) Dimethylphthalate	13.92	163	91528	3.73	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM011615\
Data File : BM000243.D
Acq On : 16 Jan 2015 21:33
Operator : TP/IZ
Sample : G1065-09
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
ClientSampled :
C0AJ1

Manual Integrations
APPROVED

TEJASKUMAR
1/19/2015 6:02:28 PM

Quant Time: Jan 17 02:50:10 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jan 17 02:31:22 2015
Response via : Initial Calibration

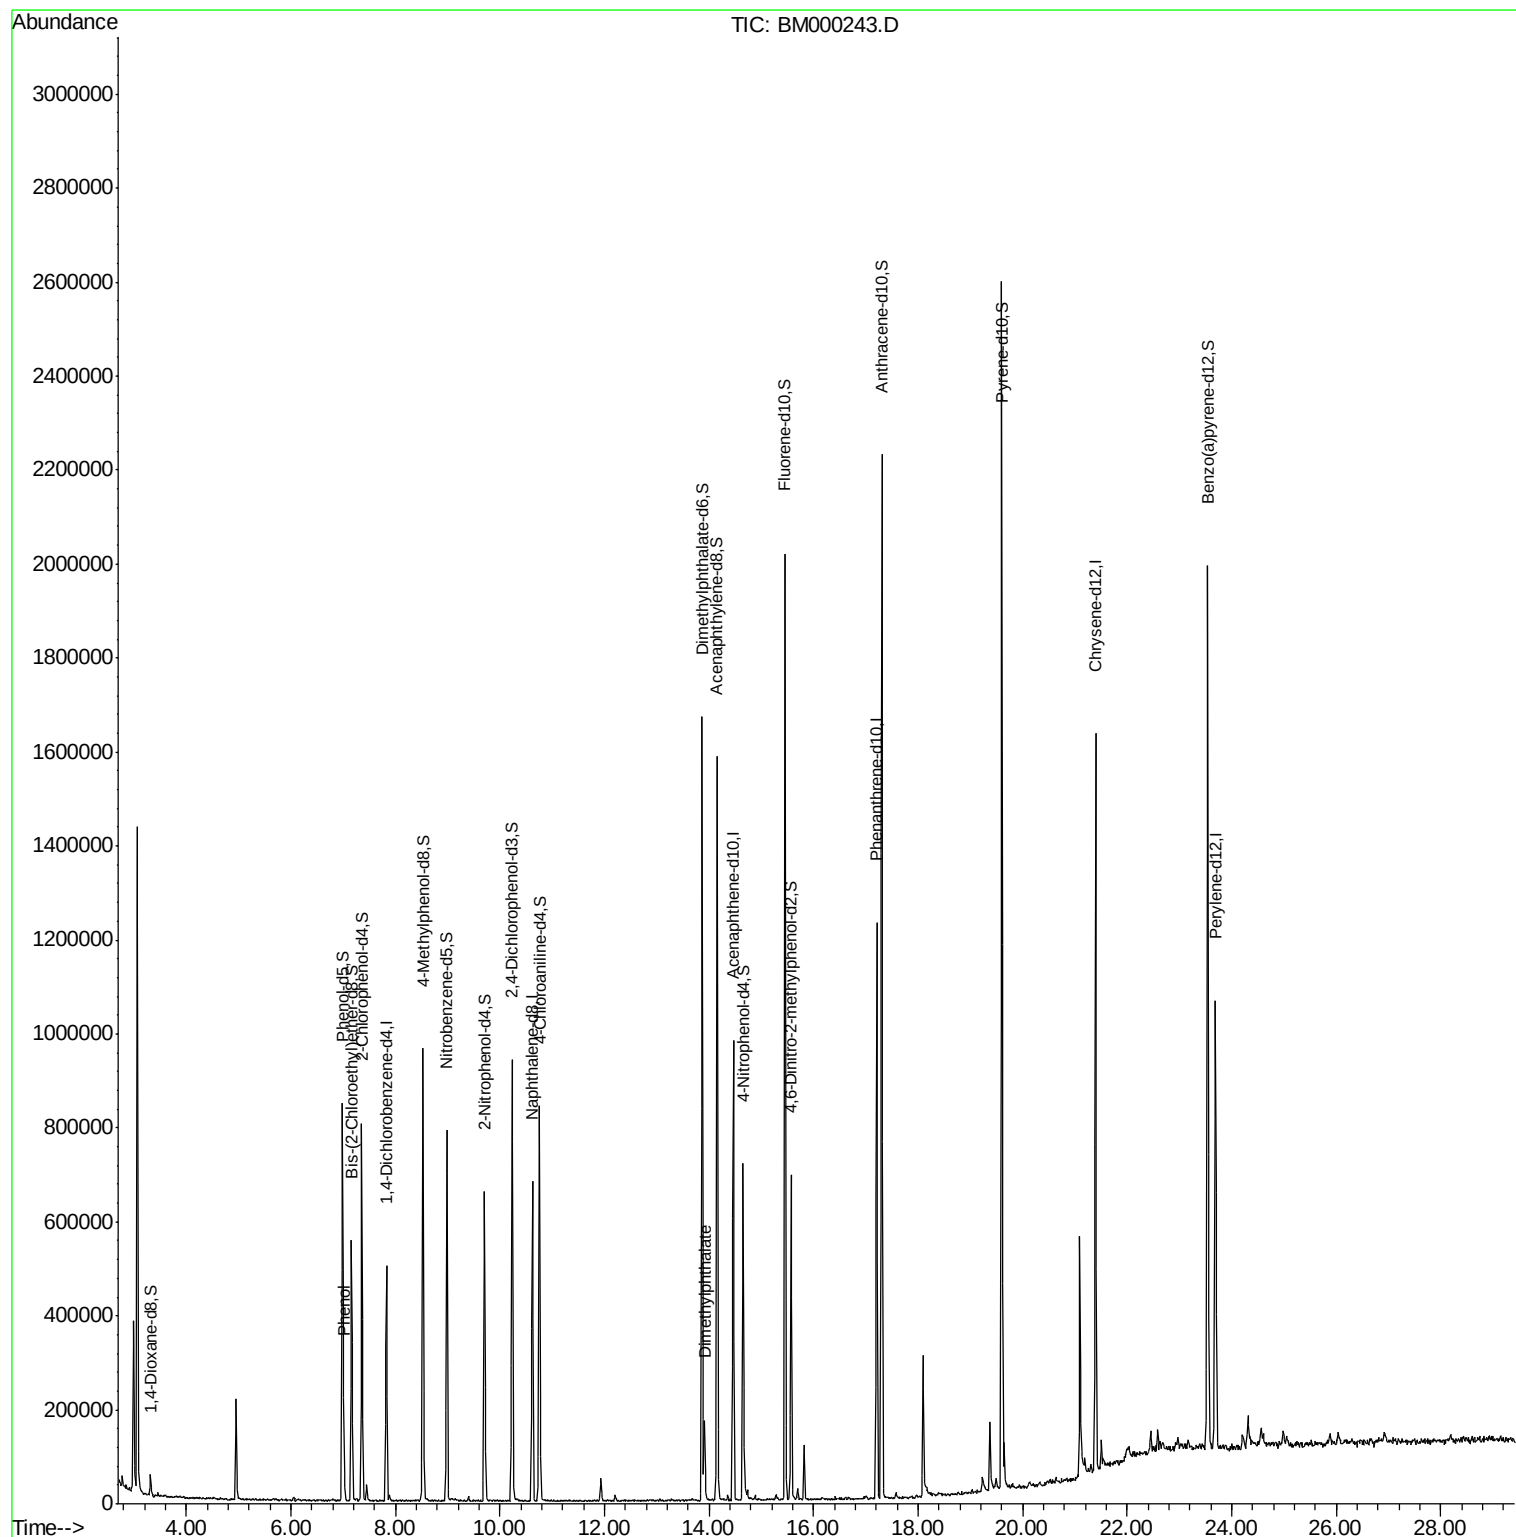

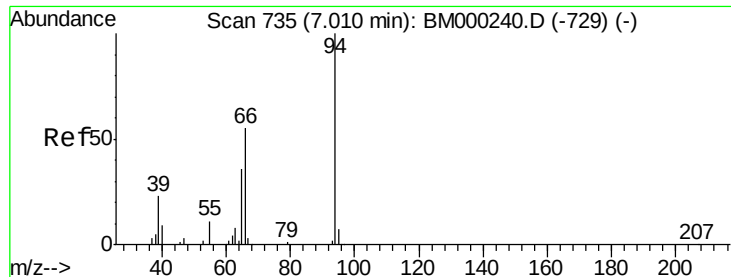

#6

Phenol

Concen: 3.47 ng/ul

RT: 7.01 min Scan# 735

Delta R.T. -0.00 min

Lab File: BM000243.D

Acq: 16 Jan 2015 21:33

Instrument :





ClientSampled :

C0AJ1

Manual Integrations
APPROVED

TEJASKUMAR
1/19/2015 6:02:28 PM

Tot Ion:	94	Resp:	34916
Ion	Ratio	Lower	Upper
94	100		
65	38.8	27.4	41.0
66	70.3	42.5	63.7#

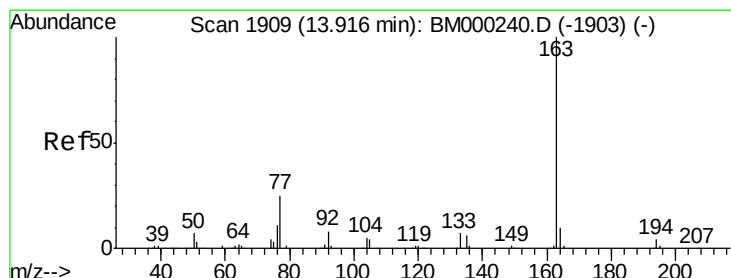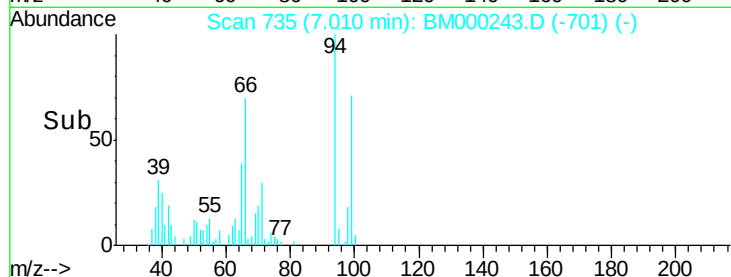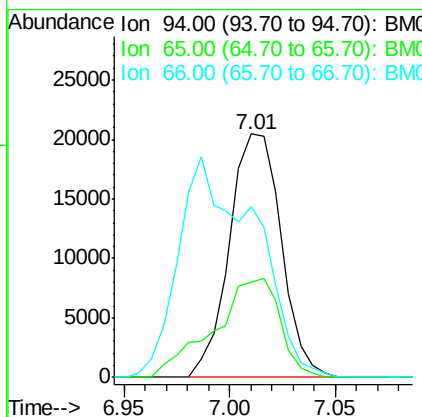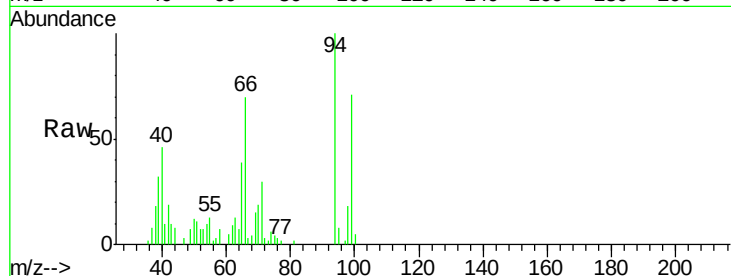

#44

Dimethylphthalate

Concen: 3.73 ng/ul

RT: 13.92 min Scan# 1909

Delta R.T. -0.00 min

Lab File: BM000243.D

Acq: 16 Jan 2015 21:33

Tgt Ion:	163	Resp:	91528
Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.0	4.4
164	11.8	8.5	12.7

