

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011615\
 Data File : BM000257.D
 Acq On : 17 Jan 2015 05:50
 Operator : TP/IZ
 Sample : G1063-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 C0AR1

Manual Integrations
 APPROVED

TEJASKUMAR
 1/21/2015 3:54:26 PM

Quant Time: Jan 19 00:28:55 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 14 12:47:10 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	125187	20.00	ng/ul	-0.03
18) Naphthalene-d8	10.62	136	510416	20.00	ng/ul	-0.03
35) Acenaphthene-d10	14.46	164	346699	20.00	ng/ul	-0.03
61) Phenanthrene-d10	17.20	188	688100	20.00	ng/ul	-0.02
75) Chrysene-d12	21.39	240	759195	20.00	ng/ul	-0.02
83) Perylene-d12	23.68	264	737897	20.00	ng/ul	-0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	17317m	8.02	ng/uL	-0.01
5) Phenol-d5	6.99	99	62743	5.96	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	7.16	67	189789	28.51	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.36	132	179541	23.25	ng/ul	-0.02
13) 4-Methylphenol-d8	8.52	113	117048	13.97	ng/ul	-0.02
19) Nitrobenzene-d5	8.98	128	113988	32.29	ng/ul	-0.03
22) 2-Nitrophenol-d4	9.70	143	124020	34.42	ng/ul	-0.03
26) 2,4-Dichlorophenol-d3	10.23	165	224664	28.22	ng/ul	-0.02
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	13.87	166	937397	36.66	ng/ul	-0.02
46) Acenaphthylene-d8	14.15	160	1014002	33.10	ng/ul	-0.02
51) 4-Nitrophenol-d4	14.65	143	23453	5.64	ng/ul	-0.01
57) Fluorene-d10	15.45	176	776877	35.38	ng/ul	-0.03
62) 4,6-Dinitro-2-methylphenol	15.56	200	116664	35.78	ng/ul	-0.03
70) Anthracene-d10	17.30	188	1264772	39.75	ng/ul	-0.01
76) Pyrene-d10	19.60	212	1430714	40.85	ng/ul	-0.02
87) Benzo(a)pyrene-d12	23.53	264	1316730	39.31	ng/ul	-0.04

Target Compounds					Qvalue
2) 1,4-Dioxane	3.35	88	106312	35.52 ng/uL	92
81) Bis(2-ethylhexyl)phthalate	21.30	149	462650	17.10 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011615\
Data File : BM000257.D
Acq On : 17 Jan 2015 05:50
Operator : TP/IZ
Sample : G1063-19
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
ClientSampleId :
C0AR1

Manual Integrations
APPROVED

TEJASKUMAR
1/21/2015 3:54:26 PM

Quant Time: Jan 19 00:28:55 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM122914.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 14 12:47:10 2015
Response via : Initial Calibration

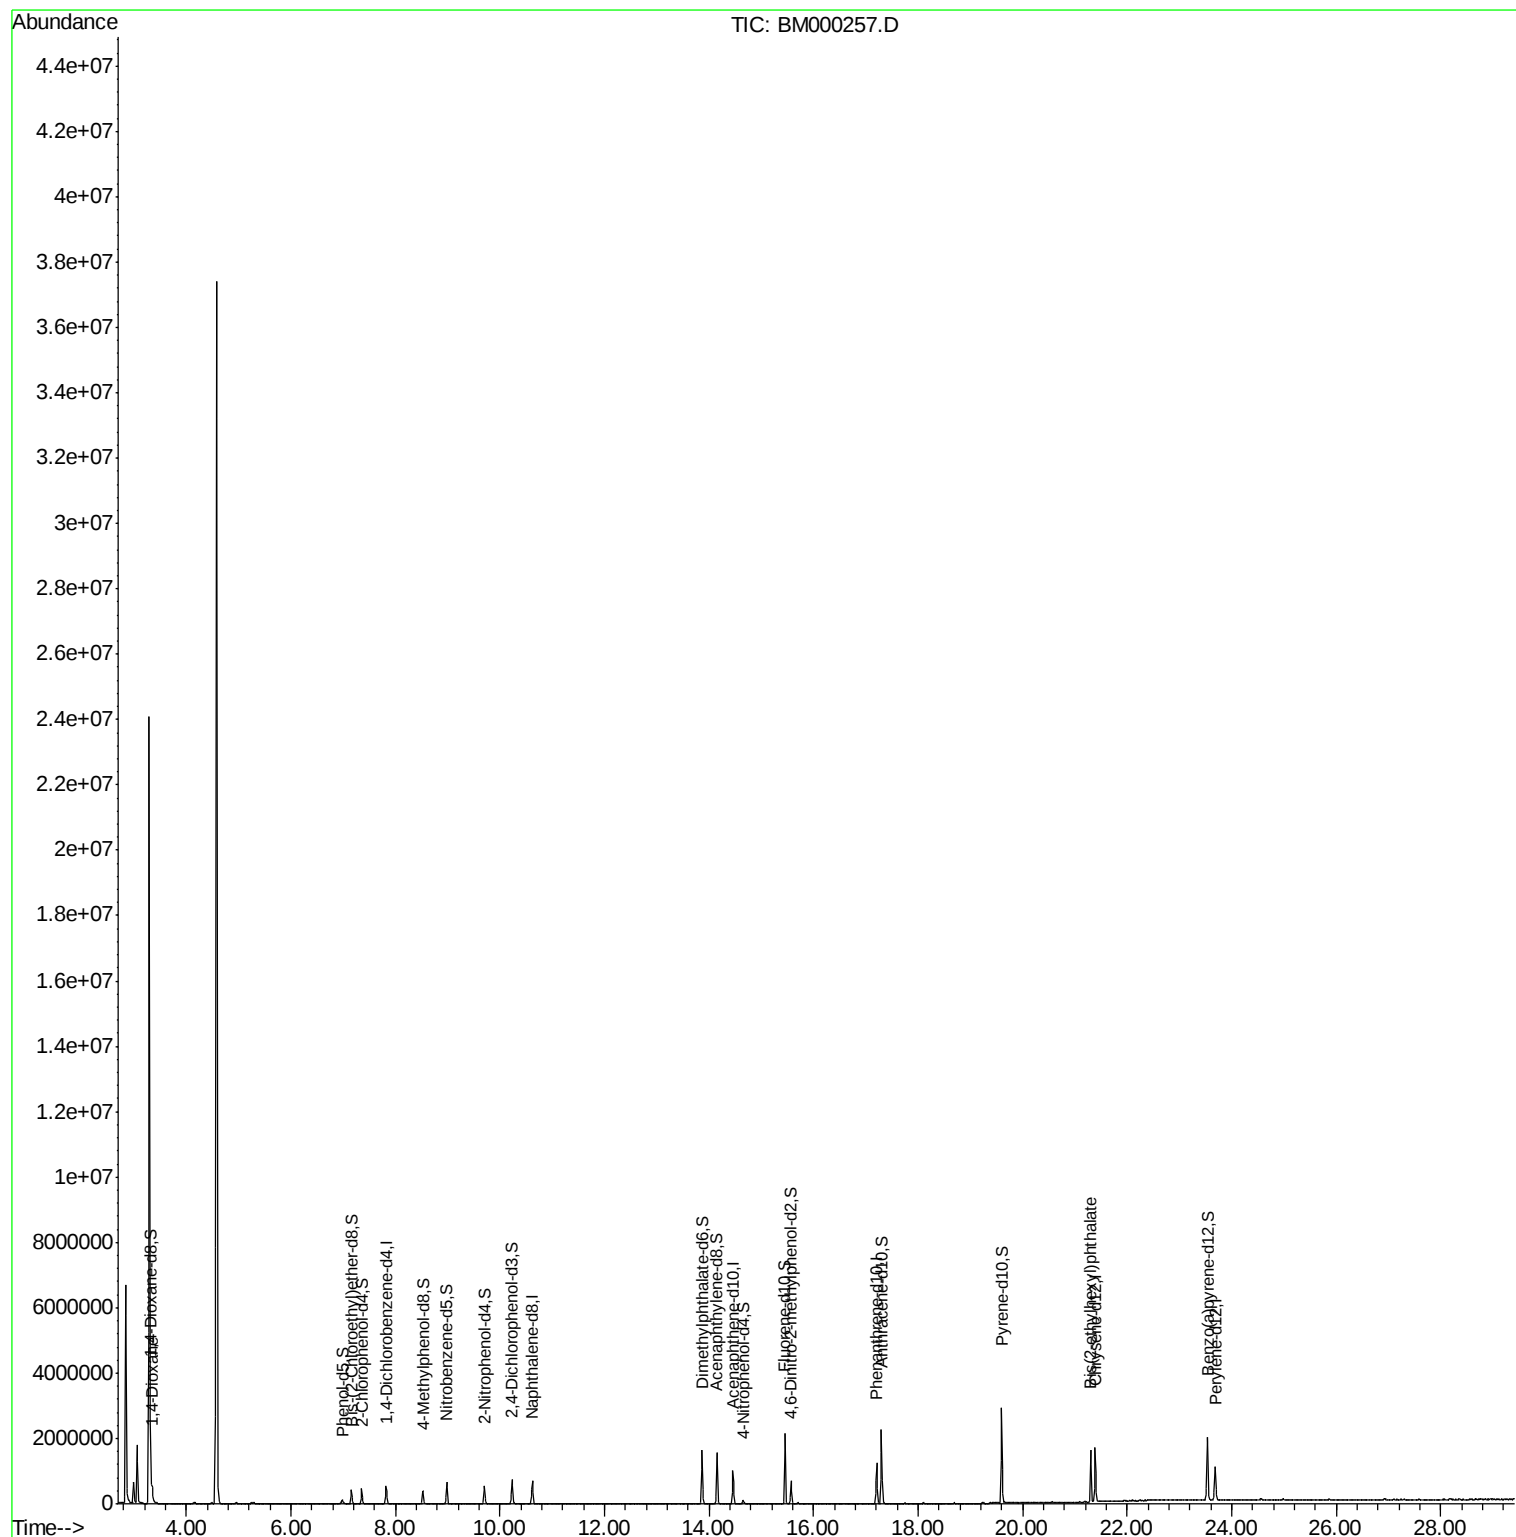

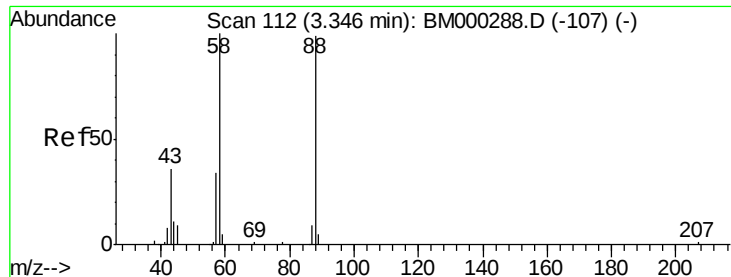

#2

1,4-Dioxane

Concen: 35.52 ng/uL

RT: 3.35 min Scan# 112

Delta R.T. -0.02 min

Lab File: BM000257.D

Acq: 17 Jan 2015 05:50

Instrument :





ClientSampled :

C0AR1

Manual Integrations
APPROVED

TEJASKUMAR
1/21/2015 3:54:26 PM

Tgt Ion	Ratio	Lower	Upper
88	100		
43	41.4	34.9	52.3
58	93.6	67.3	100.9

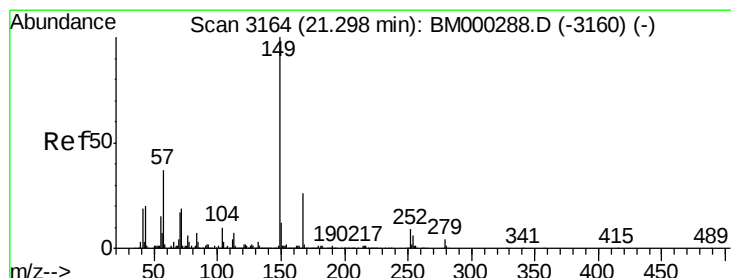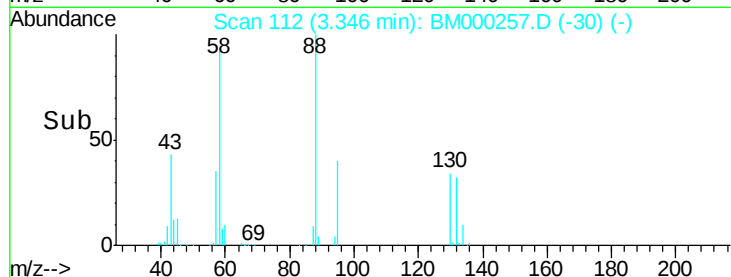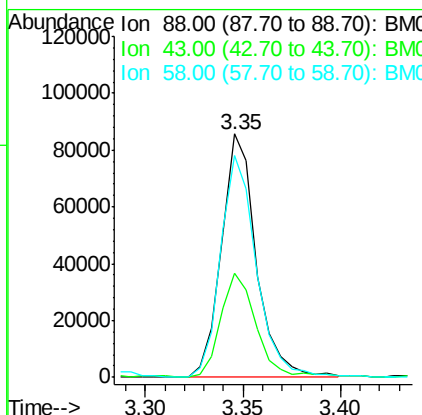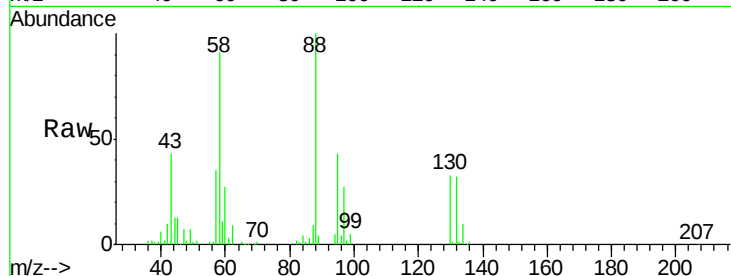

#81

Bis(2-ethylhexyl)phthalate

Concen: 17.10 ng/uL

RT: 21.30 min Scan# 3164

Delta R.T. -0.03 min

Lab File: BM000257.D

Acq: 17 Jan 2015 05:50

Tgt Ion	Ratio	Lower	Upper
149	100		
167	26.1	22.1	33.1
279	3.8	3.0	4.6

