


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011616\
Data File : BM004040.D
Acq On : 15 Jan 2016 10:35
Operator : SJ/UM
Sample : DFTPP39
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP39

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM010116.M
Title : SVOA CALIBRATION
Last Update : Sat Jan 16 03:00:58 2016

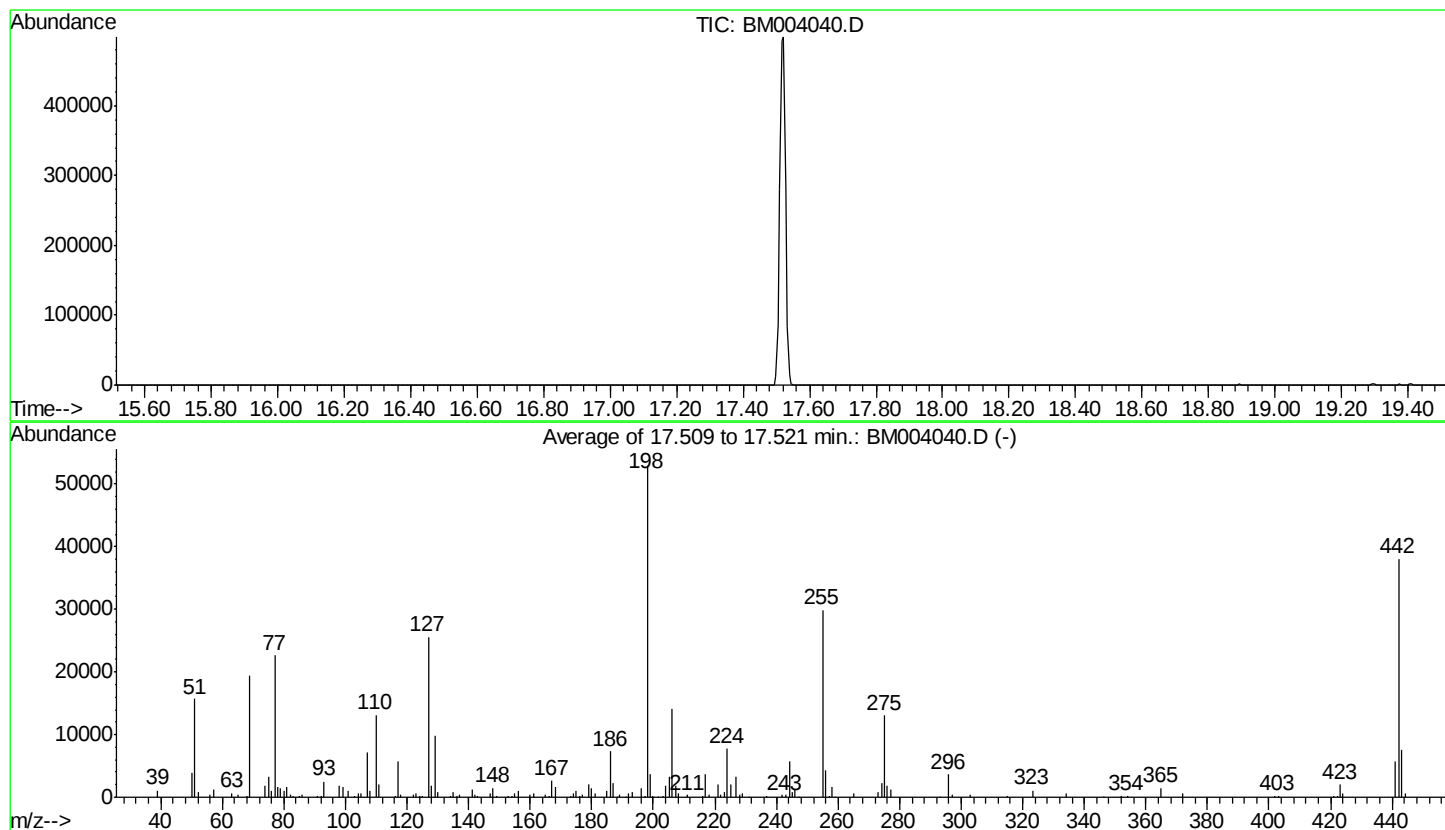

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	15723	PASS
68	69	0.00	2	0.7	126	PASS
69	198	0.00	100	36.5	19333	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.3	25557	PASS
197	198	0.00	2	0.4	237	PASS
198	198	100	100	100.0	52949	PASS
199	198	5	9	6.8	3622	PASS
275	198	10	60	24.7	13057	PASS
365	198	1	100	2.8	1459	PASS
441	443	0.01	100	77.0	5804	PASS
442	198	50	100	71.8	38042	PASS
443	442	15	24	19.8	7536	PASS

m/z	Abundance
207.10	385.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

m/z	Abundance
39.10	940.0
50.10	3143.0
51.10	12732.0
52.00	617.0
56.00	427.0
57.00	938.0
63.10	582.0
65.00	333.0
69.00	15377.0
74.00	1543.0
75.00	2470.0
76.10	818.0
77.10	17576.0
78.10	1254.0
79.00	1077.0
80.00	865.0
81.00	1335.0
82.00	307.0
86.00	320.0
93.00	1896.0
98.00	1464.0
99.00	1442.0
101.00	644.0
104.00	423.0
105.00	421.0
107.00	5439.0
108.00	836.0
110.00	9781.0
111.00	1592.0
117.00	4269.0
118.00	318.0
123.00	490.0
127.00	18600.0
128.00	1414.0
129.00	7139.0
130.00	636.0
135.00	585.0
137.00	386.0
141.00	974.0
142.00	306.0
147.00	501.0
148.00	1089.0
155.00	535.0
156.00	780.0
160.00	322.0
161.10	432.0
164.90	318.0
167.00	1812.0
168.00	1208.0
174.10	404.0
175.00	712.0
177.00	352.0
179.00	1376.0
180.00	984.0
181.00	443.0
185.00	691.0
186.10	4971.0
187.00	1533.0
191.90	457.0
193.10	522.0
196.00	1021.0
198.00	35720.0
199.00	2521.0
204.00	1313.0
205.10	2298.0
206.10	9490.0
207.10	1670.0
208.00	391.0
210.90	370.0
217.00	2380.0
218.00	307.0
221.10	1349.0
223.00	540.0
224.10	4913.0
225.10	1346.0
227.00	2105.0
228.00	348.0
229.00	464.0
244.10	3598.0
245.10	465.0
246.00	708.0
255.10	18520.0
256.10	2848.0
258.10	1043.0
265.00	381.0
273.00	517.0
274.10	1482.0
275.10	7846.0
276.00	1130.0
277.00	732.0
296.10	2217.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

323.10	578.0
334.00	442.0
365.00	745.0
372.10	336.0
423.10	995.0
424.10	304.0
441.10	2813.0
442.10	19016.0
443.10	3798.0
444.10	365.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

m/z	Abundance
39.10	1324.0
50.10	4461.0
51.10	18560.0
52.00	930.0
56.00	651.0
57.00	1344.0
63.00	797.0
65.00	373.0
68.00	378.0
69.00	22704.0
74.00	2298.0
75.00	3776.0
76.10	1309.0
77.10	26464.0
78.10	1851.0
79.00	1697.0
80.10	1259.0
81.00	1825.0
82.00	432.0
83.00	411.0
85.00	433.0
86.00	544.0
91.00	406.0
92.00	468.0
93.00	3010.0
98.00	2272.0
99.00	1931.0
101.00	1084.0
103.00	308.0
104.00	707.0
105.00	649.0
107.00	8295.0
108.00	1218.0
110.00	15210.0
111.00	2397.0
116.10	441.0
117.00	6874.0
118.00	484.0
122.00	579.0
123.00	773.0
124.00	388.0
125.00	341.0
127.00	29848.0
128.10	2223.0
129.00	11415.0
130.00	1095.0
134.00	342.0
135.00	962.0
136.00	418.0
137.00	504.0
141.00	1574.0
142.10	543.0
143.00	343.0
147.00	692.0
148.00	1684.0
149.00	440.0
153.00	446.0
154.00	337.0
155.00	801.0
156.10	1214.0
160.00	455.0
161.00	700.0
165.00	638.0
166.00	461.0
167.00	3097.0
168.00	1789.0
173.00	332.0
174.10	641.0
175.00	1159.0
176.00	375.0
177.00	497.0
179.00	2310.0
180.00	1619.0
181.00	739.0
185.00	1144.0
186.10	8541.0
187.10	2681.0
188.00	319.0
189.00	489.0
192.00	801.0
193.10	875.0
196.00	1619.0
197.10	347.0
198.00	62072.0
199.00	4139.0
200.00	341.0
202.90	404.0
204.00	2233.0
205.10	3874.0
206.10	16355.0
207.10	2406.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

208.00	650.0
211.10	565.0
216.00	354.0
217.00	4319.0
218.00	506.0
221.00	2164.0
221.80	640.0
223.00	950.0
224.10	9118.0
225.10	2298.0
227.00	3704.0
228.00	497.0
229.00	791.0
237.00	374.0
242.00	506.0
243.10	491.0
244.10	6691.0
245.00	914.0
246.10	1361.0
247.00	320.0
255.10	34488.0
256.10	4980.0
257.10	442.0
258.00	2037.0
265.00	820.0
273.00	1000.0
274.10	2606.0
275.10	14926.0
276.10	2010.0
277.00	1342.0
296.10	4179.0
297.00	564.0
303.10	439.0
315.00	460.0
323.10	1211.0
334.10	752.0
352.10	340.0
354.00	367.0
365.10	1633.0
372.10	656.0
403.10	386.0
421.00	321.0
422.10	387.0
423.10	2222.0
424.10	668.0
441.10	6491.0
442.10	41408.0
443.10	8435.0
444.10	817.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

m/z	Abundance
39.10	1126.0
50.10	3862.0
51.10	15877.0
52.10	821.0
56.00	474.0
57.00	1142.0
63.00	708.0
65.00	340.0
69.00	19920.0
74.00	1962.0
75.00	3306.0
76.00	1084.0
77.10	23896.0
78.10	1602.0
79.00	1453.0
80.00	1076.0
81.00	1738.0
82.00	444.0
83.00	388.0
85.00	423.0
86.00	441.0
91.00	355.0
92.00	426.0
93.00	2498.0
98.00	2097.0
99.00	1674.0
101.00	1063.0
103.00	350.0
104.00	670.0
105.00	628.0
107.00	7556.0
108.00	1211.0
110.00	14255.0
111.00	2071.0
116.00	491.0
117.00	5995.0
118.00	432.0
122.00	494.0
123.00	878.0
123.90	308.0
125.00	359.0
127.00	28224.0
128.00	2157.0
129.00	10958.0
130.00	954.0
134.00	306.0
135.00	877.0
136.00	345.0
137.00	463.0
141.00	1314.0
142.00	469.0
143.00	315.0
147.00	793.0
148.00	1649.0
149.00	394.0
153.00	465.0
154.00	308.0
155.00	795.0
156.00	1297.0
160.00	469.0
161.00	691.0
165.00	529.0
166.00	370.0
167.00	2910.0
168.00	1695.0
173.00	310.0
174.00	686.0
175.10	1111.0
176.00	353.0
177.00	524.0
179.00	2238.0
180.00	1478.0
181.00	680.0
185.00	1017.0
186.10	8487.0
187.00	2534.0
189.00	517.0
191.00	314.0
192.00	757.0
193.00	781.0
196.10	1911.0
197.10	366.0
198.00	61056.0
199.00	4208.0
200.00	318.0
201.60	313.0
203.00	424.0
204.00	2175.0
205.10	3768.0
206.10	16704.0
207.10	2402.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39

208.00	663.0
211.00	630.0
216.00	304.0
217.00	4230.0
218.00	565.0
221.10	2430.0
221.80	608.0
223.00	924.0
224.10	9233.0
225.00	2271.0
227.00	3786.0
228.00	501.0
229.00	803.0
231.00	320.0
237.00	330.0
242.00	490.0
243.00	518.0
244.10	6951.0
245.10	895.0
246.00	1406.0
255.10	36760.0
256.10	5308.0
257.00	433.0
258.00	2096.0
259.00	315.0
265.00	890.0
273.00	1070.0
274.10	2849.0
275.10	16400.0
276.10	2190.0
277.00	1333.0
293.10	306.0
296.00	4478.0
297.00	720.0
303.00	569.0
315.00	478.0
323.10	1445.0
334.00	903.0
346.00	305.0
352.10	405.0
354.10	486.0
365.10	2000.0
372.10	751.0
402.00	355.0
403.10	390.0
421.10	415.0
422.00	343.0
423.10	2709.0
424.10	732.0
441.20	8108.0
442.10	53704.0
443.10	10376.0
444.10	944.0

Instrument :
BNA_M
ClientSampleId :
DFTPP39