

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011618\
 Data File : BM013622.D
 Acq On : 16 Jan 2018 14:39
 Operator : SJ/JU
 Sample : J1180-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jan 17 00:59:58 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 17 00:57:07 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	146615	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	591744	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	337709	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	740388	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	812827	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	801822	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.16	96	18171	4.90	ng/uL	0.00
5) Phenol-d5	6.80	99	334373	29.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	214889	31.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	277705	30.28	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	288971	33.40	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	149864	32.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	129026	26.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	244443	26.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	256571	31.55	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	886499	31.85	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	1200875	33.83	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	18180	4.02	ng/ul	0.01
57) Fluorene-d10	15.27	176	803550	32.83	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.41	200	25109	5.63	ng/ul	0.00
70) Anthracene-d10	17.12	188	1222640	33.90	ng/ul	0.00
76) Pyrene-d10	19.42	212	1384637	36.59	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1321809	35.87	ng/ul	0.00
Target Compounds						
6) Phenol	6.83	94	52189	4.623	ng/ul#	86
15) N-Nitroso-di-n-propylamine	8.33	70	8010	1.147	ng/ul#	1
44) Dimethylphthalate	13.73	163	148058	5.410	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM011618\
Data File : BM013622.D
Acq On : 16 Jan 2018 14:39
Operator : SJ/JU
Sample : J1180-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jan 17 00:59:58 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM011018.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 17 00:57:07 2018
Response via : Initial Calibration

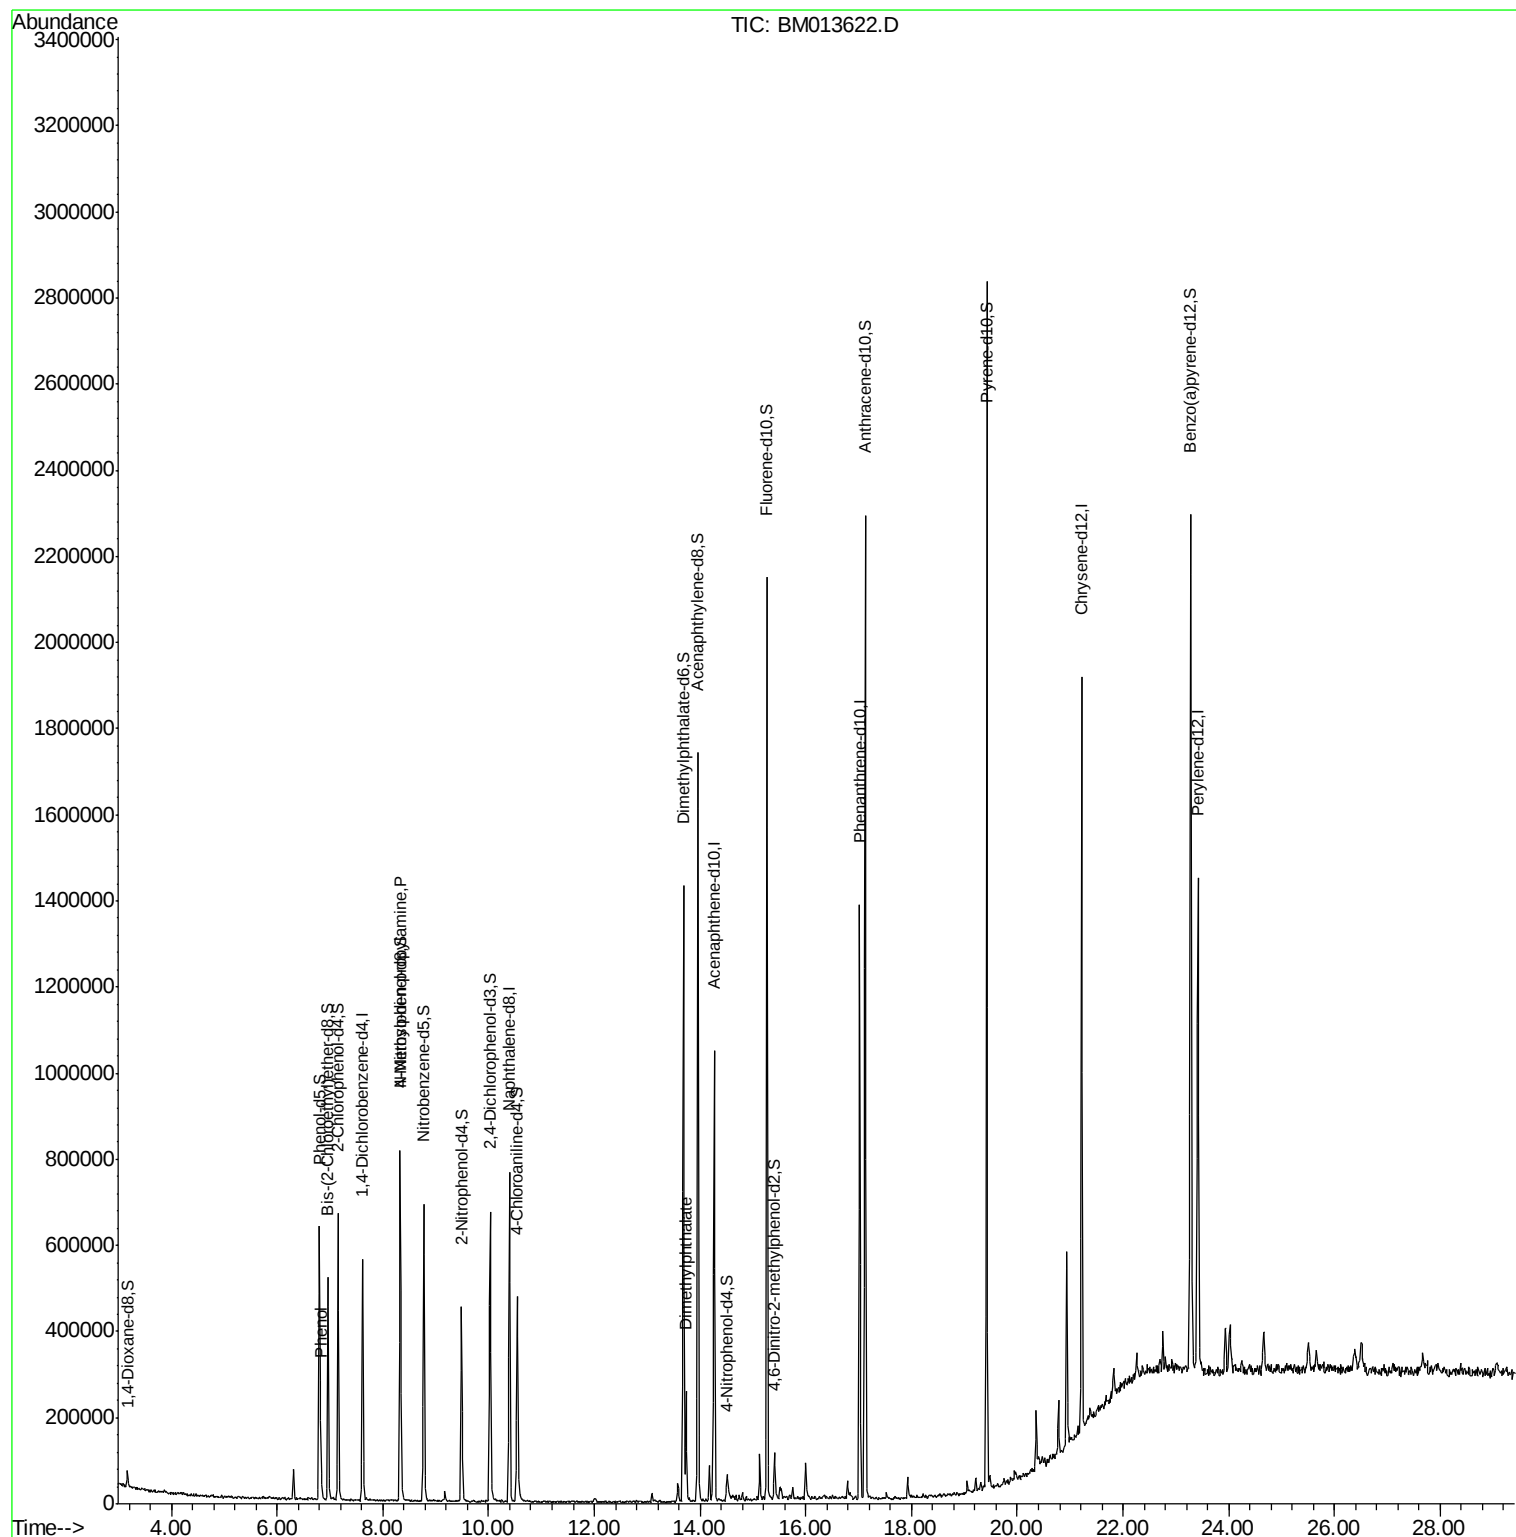

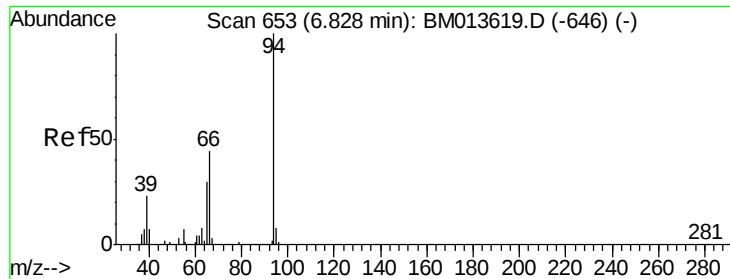

#6

Phenol

Concen: 4.623 ng/ul

RT: 6.83 min Scan# 653

Delta R.T. 0.00 min

Lab File: BM013622.D

Acq: 16 Jan 2018 14:39

Instrument :

BNA_M

ClientSampleId :





Tot Ion: 94 Resp: 52189

Ion Ratio Lower Upper

94 100

65 33.2 28.2 42.4

66 43.5 47.2 70.8#

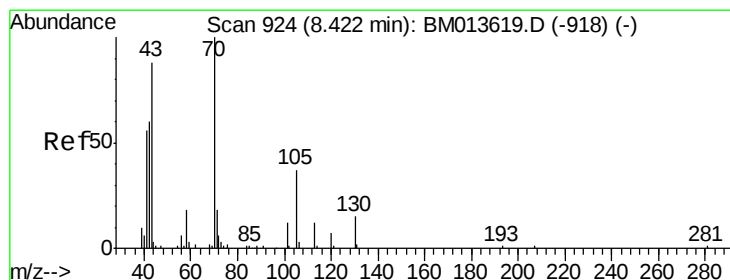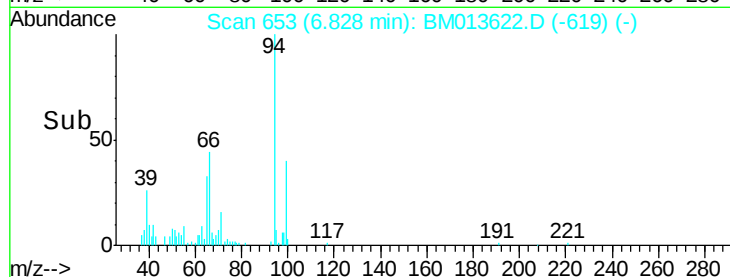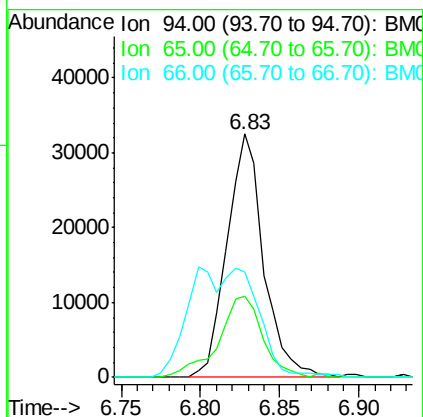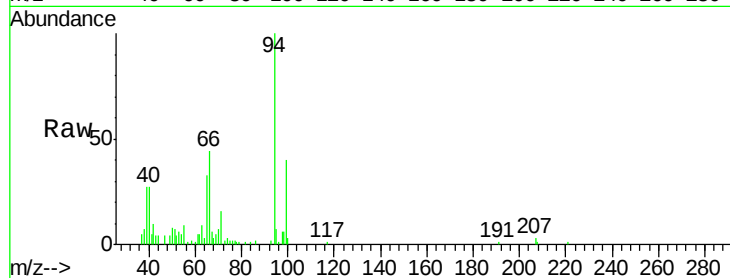

#15

N-Nitroso-di-n-propylamine

Concen: 1.147 ng/ul

RT: 8.33 min Scan# 908

Delta R.T. -0.09 min

Lab File: BM013622.D

Acq: 16 Jan 2018 14:39

Tgt Ion: 70 Resp: 8010




Ion Ratio Lower Upper


70 100

42 381.5 76.0 114.0#

101 0.0 6.7 10.1#

130 0.0 14.6 22.0#

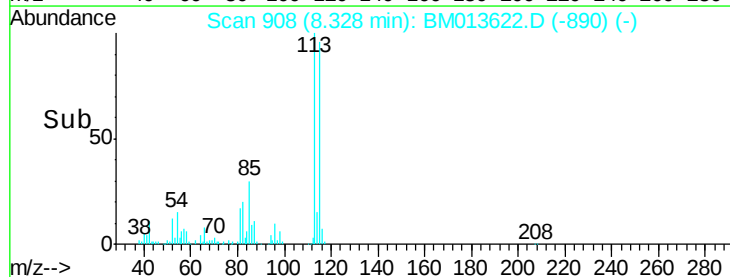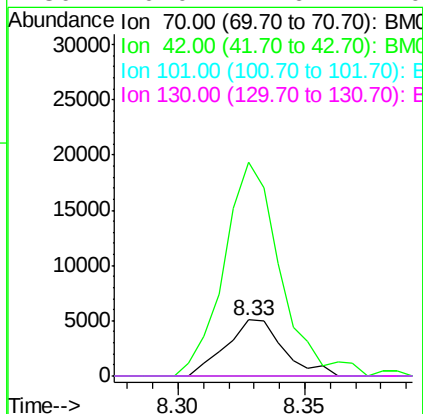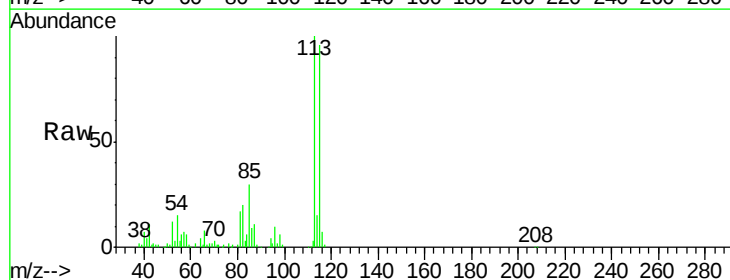


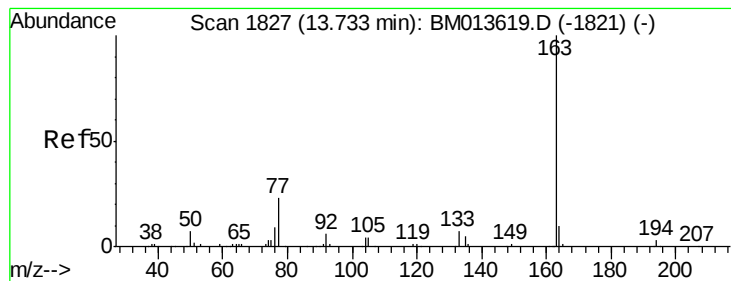

#44
 Dimethylphthalate
 Concen: 5.410 ng/ul
 RT: 13.73 min Scan# 1827
 Delta R.T. 0.00 min
 Lab File: BM013622.D
 Acq: 16 Jan 2018 14:39

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:	163	Resp:	148058
Ion Ratio	Lower	Upper	
163	100		
194	4.8	3.5	5.3
164	9.3	8.2	12.4

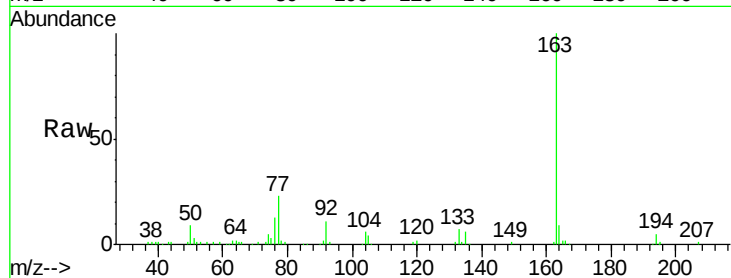

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

