


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM011618\
 Data File : BM013618.D
 Acq On : 16 Jan 2018 12:16
 Operator : SJ/JU
 Sample : DFTPP75
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP75

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011018.M
 Title : SVOA CALIBRATION
 Last Update : Wed Jan 17 00:57:07 2018

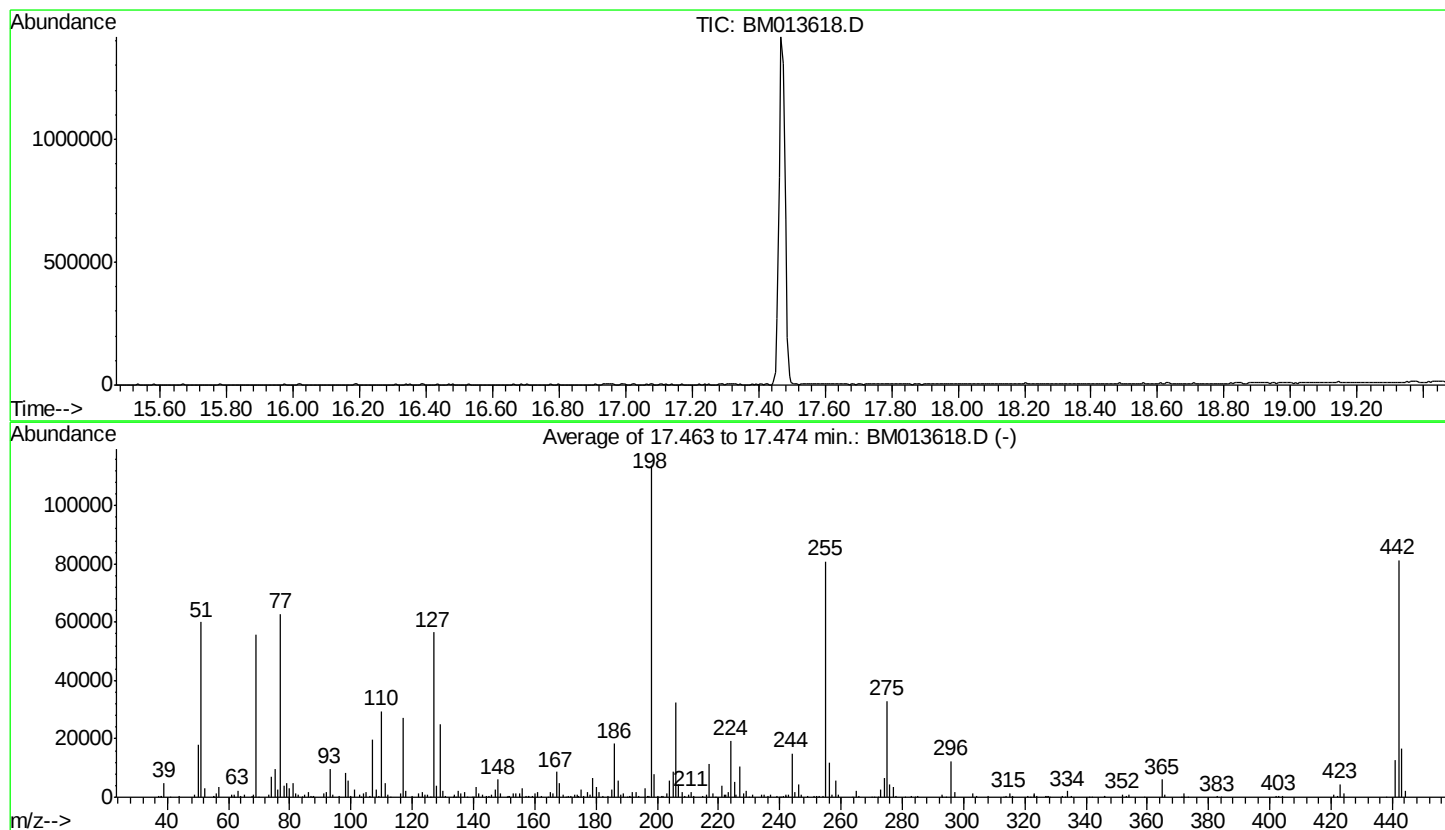

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.9	60106	PASS
68	69	0.00	2	1.3	743	PASS
69	198	0.00	100	48.9	55642	PASS
70	69	0.00	2	0.3	140	PASS
127	198	10	80	49.7	56450	PASS
197	198	0.00	2	0.5	535	PASS
198	198	100	100	100.0	113682	PASS
199	198	5	9	7.0	7903	PASS
275	198	10	60	29.0	32984	PASS
365	198	1	100	5.3	5978	PASS
441	443	0.01	100	78.5	12943	PASS
442	198	50	100	71.4	81213	PASS
443	442	15	24	20.3	16495	PASS

m/z	Abundance
37.00	359.0
37.90	1066.0
39.00	5510.0
39.90	489.0
44.00	1435.0
49.00	876.0
50.10	16536.0
51.00	48032.0
52.00	2476.0
55.00	339.0
56.00	1867.0
57.00	2650.0
61.20	613.0
61.80	689.0
63.10	2702.0
65.10	504.0
68.10	675.0
69.00	43032.0
69.90	420.0
73.10	677.0
74.10	4955.0
75.00	7680.0
76.10	2666.0
77.10	51688.0
78.10	3860.0
79.00	4495.0
79.80	2315.0
81.00	4487.0
81.90	880.0
82.80	928.0
83.80	449.0
85.00	1195.0
86.10	1388.0
87.00	413.0
87.90	597.0
91.10	1141.0
92.00	1174.0
93.00	8278.0
94.00	729.0
96.20	369.0
98.00	5855.0
99.00	4072.0
101.00	1952.0
103.20	545.0
103.90	887.0
105.00	1575.0
106.10	532.0
107.00	17224.0
108.10	1492.0
109.00	519.0
110.00	21296.0
111.10	2847.0
112.00	935.0
115.90	1167.0
117.00	19112.0
117.90	1980.0
120.00	302.0
121.90	1111.0
123.20	1280.0
124.00	550.0
125.00	347.0
127.00	46664.0
128.00	3184.0
129.00	17464.0
129.90	1837.0
130.90	309.0
133.90	621.0
134.90	1896.0
135.90	1131.0
137.00	1482.0
138.00	339.0
140.00	464.0
141.00	2960.0
141.90	565.0
143.00	948.0
146.00	676.0
147.00	1687.0
148.00	3363.0
149.00	950.0
153.00	630.0
153.90	1540.0
154.90	1906.0
155.90	3227.0
156.90	488.0
157.90	667.0
160.10	794.0
160.90	994.0
164.90	1584.0
165.90	652.0
167.00	6092.0
167.90	4173.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

169.10	306.0
170.90	324.0
173.10	765.0
173.90	1385.0
175.10	2914.0
175.90	795.0
177.00	1216.0
177.90	500.0
178.90	4646.0
180.00	2774.0
181.00	1277.0
182.20	322.0
185.00	1290.0
186.00	13982.0
187.10	3959.0
188.00	364.0
189.10	1016.0
191.00	399.0
191.80	629.0
193.10	1240.0
194.20	475.0
196.00	2447.0
196.90	537.0
197.90	78344.0
198.90	6078.0
199.90	374.0
201.40	587.0
203.00	696.0
204.00	3790.0
205.00	5496.0
206.00	21384.0
207.10	4427.0
208.10	1361.0
210.20	311.0
211.10	784.0
214.80	368.0
217.00	7487.0
218.00	1347.0
221.00	2672.0
221.70	1095.0
223.00	1051.0
224.10	15168.0
225.10	4319.0
225.80	462.0
227.10	8225.0
228.00	907.0
229.00	1494.0
230.90	781.0
234.00	536.0
235.10	388.0
235.90	396.0
237.10	987.0
241.90	850.0
242.90	815.0
244.00	9809.0
245.00	1335.0
246.10	2788.0
247.00	781.0
249.00	447.0
255.00	52840.0
255.90	6987.0
257.10	909.0
258.10	4193.0
259.10	797.0
265.00	1620.0
265.90	546.0
273.00	1509.0
273.90	4581.0
275.00	19976.0
275.90	2843.0
277.10	2419.0
277.90	733.0
285.00	345.0
292.90	613.0
296.00	7031.0
296.90	822.0
303.00	1281.0
304.00	362.0
314.00	349.0
315.00	779.0
323.00	1262.0
326.80	376.0
327.80	449.0
334.00	1385.0
335.00	514.0
340.90	391.0
341.90	429.0
346.10	495.0
351.90	905.0
354.10	694.0
365.00	2835.0
365.80	486.0
371.90	450.0
421.00	446.0
422.20	303.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

423.00	2275.0
423.90	395.0
441.00	6861.0
442.10	42112.0
443.10	10007.0
444.00	400.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

m/z	Abundance
37.00	485.0
38.10	941.0
39.10	5236.0
40.00	449.0
41.00	310.0
44.10	1636.0
48.90	569.0
50.10	22144.0
51.00	73832.0
52.00	3560.0
54.90	518.0
56.00	1523.0
57.00	4840.0
60.80	1002.0
61.20	1006.0
62.00	1361.0
63.00	1985.0
63.90	370.0
65.00	1169.0
68.10	1555.0
69.00	71416.0
73.00	636.0
74.10	9357.0
75.00	11259.0
76.10	2575.0
77.10	74944.0
78.10	4502.0
79.00	6492.0
79.90	4243.0
81.00	5724.0
82.00	1809.0
82.90	1413.0
84.00	328.0
85.00	948.0
86.00	1576.0
87.00	583.0
87.90	402.0
91.00	1243.0
92.00	2752.0
93.00	11355.0
94.10	775.0
98.00	10506.0
99.00	7362.0
99.90	1029.0
100.90	2697.0
102.90	1312.0
104.00	2185.0
105.00	1912.0
105.90	561.0
107.00	22528.0
108.00	3475.0
109.00	415.0
110.00	38696.0
111.10	7099.0
112.00	533.0
112.80	572.0
116.00	1672.0
117.00	34288.0
117.90	2340.0
119.90	614.0
121.90	2155.0
123.10	2630.0
124.00	1666.0
124.80	747.0
125.90	304.0
127.00	68664.0
128.00	4481.0
129.00	31360.0
129.90	2602.0
131.00	753.0
133.80	821.0
134.20	701.0
135.00	2702.0
135.90	1435.0
137.10	1974.0
140.90	4120.0
141.80	1466.0
143.10	1202.0
144.20	451.0
145.10	670.0
146.00	915.0
147.00	3190.0
148.00	8729.0
148.90	1499.0
151.10	529.0
151.90	514.0
153.00	1280.0
153.90	983.0
155.10	2172.0
155.90	2927.0
157.00	731.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

157.90	907.0
159.00	634.0
159.90	892.0
160.90	2275.0
162.00	776.0
164.20	362.0
165.00	1769.0
166.00	1343.0
167.00	10961.0
168.00	5070.0
169.10	1323.0
169.90	456.0
170.90	516.0
171.90	770.0
173.00	1210.0
173.90	1195.0
175.00	3365.0
176.00	684.0
176.90	1967.0
178.00	1238.0
179.00	8103.0
180.00	4929.0
181.00	2035.0
182.10	395.0
184.10	559.0
184.90	3545.0
186.00	18728.0
187.00	6196.0
188.00	1182.0
189.00	1996.0
191.10	543.0
192.00	2601.0
193.00	2187.0
194.00	438.0
196.00	3990.0
197.10	794.0
197.90	136384.0
198.90	10462.0
200.00	430.0
201.40	863.0
201.90	340.0
203.00	2168.0
204.10	6979.0
205.00	11897.0
206.00	41432.0
207.00	5567.0
207.90	1315.0
209.00	891.0
210.00	1374.0
210.90	1870.0
212.00	464.0
214.90	506.0
215.90	1149.0
217.00	13543.0
217.90	1232.0
221.00	4175.0
221.70	1149.0
222.10	1003.0
223.10	2429.0
224.00	21776.0
225.00	6663.0
225.90	893.0
227.00	12371.0
227.90	1327.0
229.10	1870.0
229.80	318.0
230.90	923.0
234.10	1605.0
234.90	822.0
235.90	812.0
237.00	818.0
238.90	586.0
239.80	389.0
241.00	434.0
241.90	1462.0
243.00	1221.0
244.00	17928.0
244.90	2476.0
246.00	4547.0
246.90	1064.0
248.90	633.0
251.00	422.0
251.80	395.0
253.00	1130.0
255.00	92184.0
256.00	13996.0
257.00	1395.0
258.00	6279.0
259.00	982.0
265.00	1710.0
266.00	605.0
269.90	410.0
272.00	353.0
273.00	3604.0
274.00	7719.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

275.00	38584.0
276.00	5853.0
277.00	4148.0
283.00	742.0
285.10	480.0
293.10	805.0
296.00	14685.0
297.00	2523.0
303.00	1329.0
304.10	671.0
307.90	338.0
313.90	497.0
315.00	1949.0
315.80	506.0
316.20	555.0
320.90	593.0
321.80	312.0
323.00	2840.0
324.10	570.0
326.80	610.0
328.20	496.0
332.00	672.0
333.00	340.0
333.90	1627.0
334.90	365.0
346.00	731.0
352.00	923.0
353.10	520.0
354.20	830.0
359.00	335.0
365.00	6750.0
365.90	801.0
372.10	1618.0
373.10	320.0
402.00	780.0
403.00	1327.0
404.10	637.0
420.90	985.0
422.10	851.0
423.10	5998.0
423.90	1583.0
437.80	310.0
441.10	15314.0
442.10	85744.0
443.10	16832.0
444.10	2357.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

m/z	Abundance
37.00	349.0
37.90	629.0
39.10	4162.0
44.00	1320.0
49.10	655.0
50.00	15410.0
51.00	58456.0
52.10	2840.0
55.20	345.0
55.90	1097.0
57.00	2951.0
61.00	933.0
62.00	1406.0
63.00	2549.0
63.90	802.0
65.00	1487.0
67.80	876.0
69.00	52480.0
73.10	768.0
74.00	6776.0
75.00	9795.0
76.00	3299.0
77.00	61736.0
78.00	3750.0
79.00	4044.0
79.90	3167.0
81.00	4068.0
81.90	1337.0
83.00	517.0
85.00	876.0
86.10	2027.0
87.20	496.0
91.00	1227.0
92.10	1876.0
93.00	9516.0
93.90	542.0
96.00	366.0
98.00	8979.0
99.10	5557.0
99.90	430.0
101.10	3100.0
103.00	766.0
104.00	1365.0
104.90	1945.0
106.00	919.0
107.00	19168.0
108.00	2838.0
108.90	672.0
110.00	28624.0
111.10	5079.0
111.80	675.0
116.10	1328.0
117.00	28008.0
117.90	2159.0
122.00	1129.0
123.10	1866.0
123.90	628.0
125.00	1124.0
126.20	486.0
127.00	54024.0
128.00	4725.0
129.00	26392.0
130.00	2722.0
133.10	419.0
133.80	718.0
134.90	1450.0
136.00	899.0
137.00	1359.0
139.70	405.0
141.00	3640.0
141.90	1322.0
142.90	551.0
144.10	561.0
145.10	300.0
146.00	941.0
147.00	2804.0
148.00	6158.0
149.00	1516.0
150.80	366.0
151.10	352.0
151.80	356.0
153.00	1792.0
154.00	1600.0
155.00	1979.0
156.00	2522.0
157.00	702.0
158.10	773.0
159.00	434.0
160.00	1984.0
160.90	2675.0
164.90	1708.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

166.00	1386.0
167.00	8878.0
168.00	5684.0
169.20	1067.0
172.00	909.0
173.10	1271.0
174.10	1368.0
175.00	2232.0
175.90	401.0
177.10	1996.0
177.80	509.0
178.90	7440.0
179.90	3395.0
181.10	1688.0
182.10	398.0
183.90	468.0
184.90	2772.0
186.00	22408.0
186.90	7449.0
187.90	729.0
189.00	1334.0
190.10	340.0
190.80	470.0
191.10	496.0
192.00	2564.0
193.00	2077.0
193.90	575.0
195.90	3292.0
196.90	1068.0
197.90	126320.0
199.00	7170.0
200.00	1023.0
201.70	637.0
203.00	1065.0
204.00	6753.0
205.10	9039.0
206.00	34088.0
207.00	5578.0
208.10	2010.0
209.00	676.0
210.20	737.0
211.10	2710.0
211.90	393.0
215.00	548.0
216.00	904.0
217.00	12802.0
218.00	1822.0
219.00	403.0
221.00	4901.0
222.10	1148.0
222.90	2192.0
224.00	21656.0
225.00	5490.0
225.90	669.0
227.00	11115.0
228.00	1338.0
229.00	2958.0
231.00	510.0
234.00	561.0
235.00	954.0
235.90	636.0
237.00	1021.0
239.00	480.0
240.10	622.0
240.90	565.0
242.10	1237.0
243.00	1255.0
244.10	17600.0
245.10	2124.0
246.00	5416.0
247.00	901.0
249.10	450.0
251.10	325.0
251.80	446.0
253.10	344.0
254.00	889.0
255.00	97648.0
256.00	14352.0
257.10	629.0
258.00	6205.0
258.90	1122.0
263.80	303.0
265.00	3206.0
266.00	450.0
270.80	307.0
272.90	2364.0
274.00	7763.0
275.00	40392.0
276.10	4784.0
277.00	3649.0
277.90	586.0
280.80	388.0
283.10	709.0
284.10	327.0
284.90	443.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

285.20	417.0
293.00	1441.0
294.00	391.0
296.00	15387.0
297.00	1828.0
303.00	1565.0
304.10	686.0
307.90	567.0
312.80	422.0
314.10	421.0
314.80	903.0
315.10	869.0
316.00	643.0
320.90	1018.0
323.20	3038.0
323.90	1026.0
327.00	1101.0
327.80	334.0
332.10	526.0
334.10	3171.0
335.10	763.0
345.80	1422.0
351.90	1027.0
353.00	1402.0
354.00	1631.0
365.00	8351.0
365.90	961.0
370.90	579.0
372.10	1779.0
382.90	907.0
384.20	330.0
401.90	613.0
402.80	655.0
403.90	668.0
421.00	988.0
422.00	722.0
423.00	5540.0
424.00	1436.0
441.10	16656.0
442.10	115784.0
443.10	22648.0
444.00	3431.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75

Scan 2456 (17.433 min): BM013618.D
DFTPP75

m/z	Abundance
39.90	315.0
44.10	1053.0
207.10	826.0

Instrument :
BNA_M
ClientSampleId :
DFTPP75