
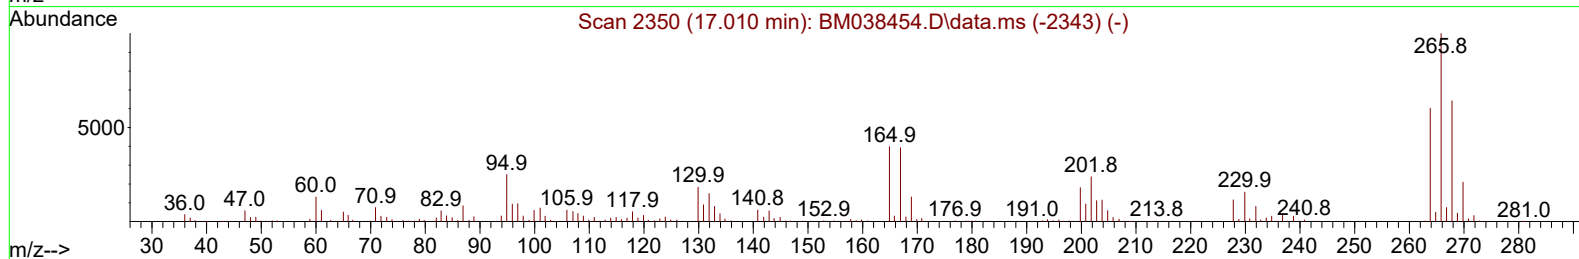
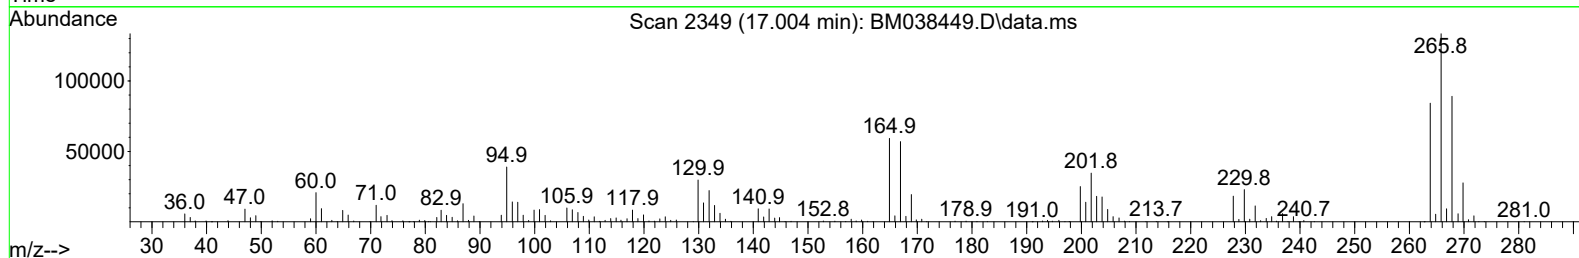


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011623\
Data File : BM038449.D
Acq On : 16 Jan 2023 12:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:30:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 03:06:05 2023
Response via : Initial Calibration

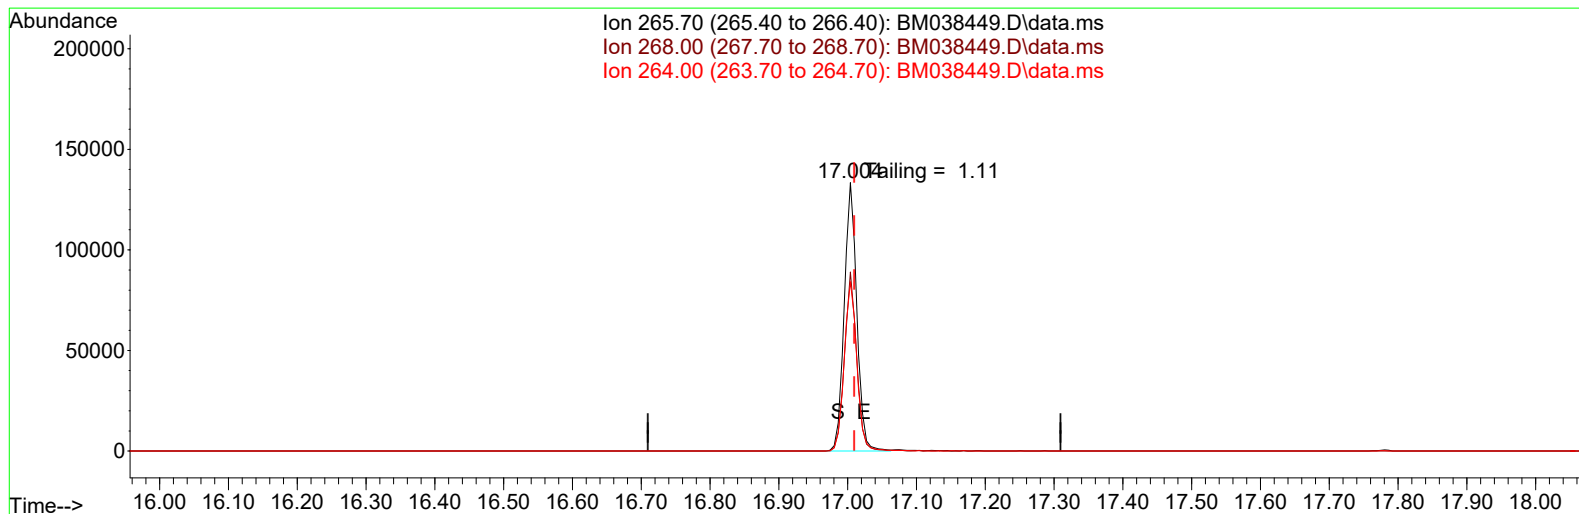

TIC: BM038449.D\data.ms

(70) Pentachlorophenol (C)




17.004min (-0.006) 0.00 ng

response 168979

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	66.73
264.00	60.20	63.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011623\
Data File : BM038449.D
Acq On : 16 Jan 2023 12:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:30:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 03:06:05 2023
Response via : Initial Calibration

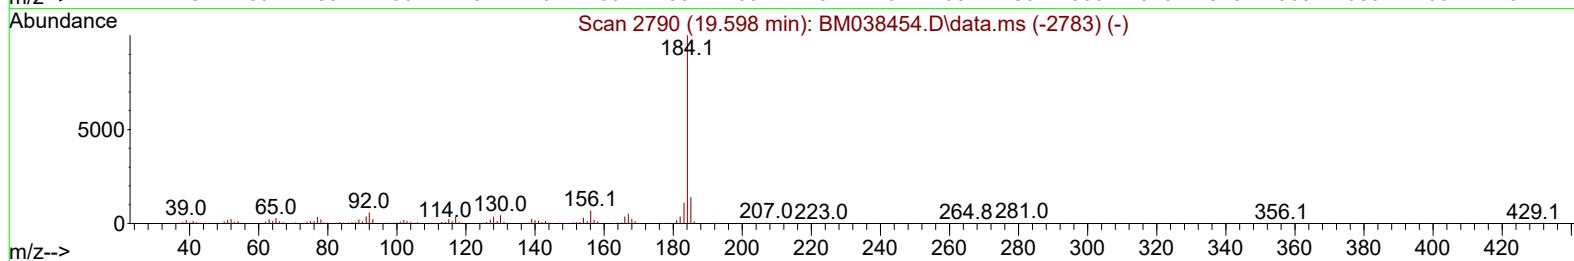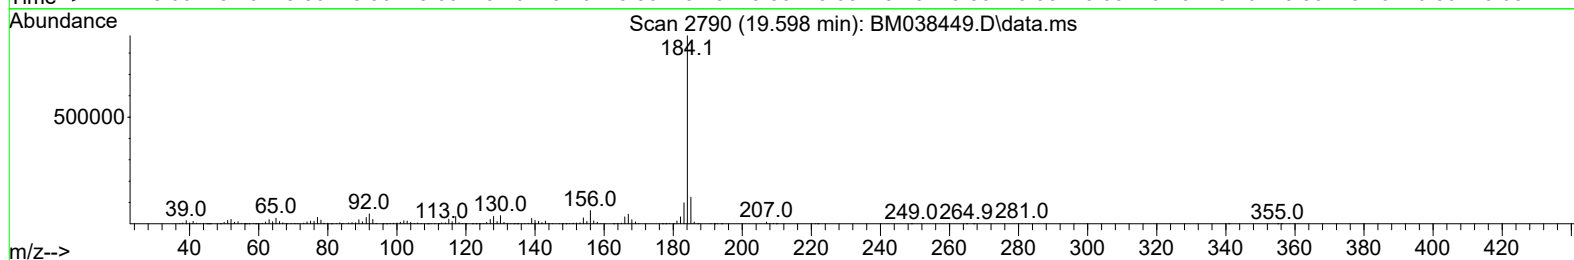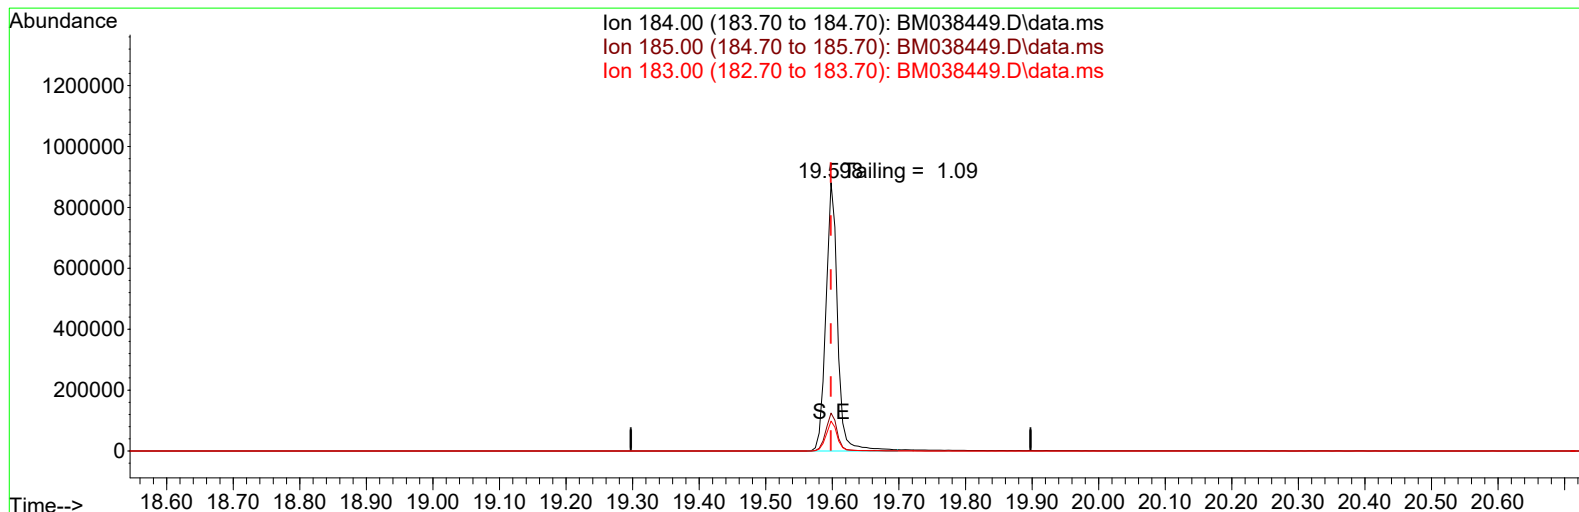

TIC: BM038449.D\data.ms

(77) Benzidine

19.598min (+ 0.000) 0.00 ng

response 1081435

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.13
183.00	10.80	11.17
0.00	0.00	0.00