

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011623\
 Data File : BM038460.D
 Acq On : 16 Jan 2023 19:58
 Operator : CG/JU
 Sample : PB150096BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB150096BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM038460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.069	314	320	329	rBV	672033	917247	34.84%	6.229%
2	5.534	392	399	408	rBV	1531784	2051181	77.90%	13.930%
3	7.145	666	673	689	rBV	1258667	1934924	73.49%	13.141%
4	7.981	809	815	824	rVB	210478	318594	12.10%	2.164%
5	9.157	1006	1015	1025	rBV	700593	1094979	41.59%	7.436%
6	10.792	1286	1293	1303	rBV	208931	341470	12.97%	2.319%
7	13.239	1703	1709	1719	rBV	1473210	2059514	78.22%	13.987%
8	14.615	1936	1943	1950	rBV	265506	367001	13.94%	2.492%
9	16.098	2189	2195	2209	rBV	1212028	1616153	61.38%	10.976%
10	17.356	2403	2409	2418	rBV	290386	392461	14.91%	2.665%
11	19.968	2848	2853	2863	rBV	2464550	2633023	100.00%	17.882%
12	20.715	2977	2980	2986	rVB2	29227	33602	1.28%	0.228%
13	21.527	3114	3118	3126	rBV	333467	428082	16.26%	2.907%
14	23.950	3523	3530	3538	rBV2	255920	536453	20.37%	3.643%




Sum of corrected areas: 14724684

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011623\
Data File : BM038460.D
Acq On : 16 Jan 2023 19:58
Operator : CG/JU
Sample : PB150096BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150096BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

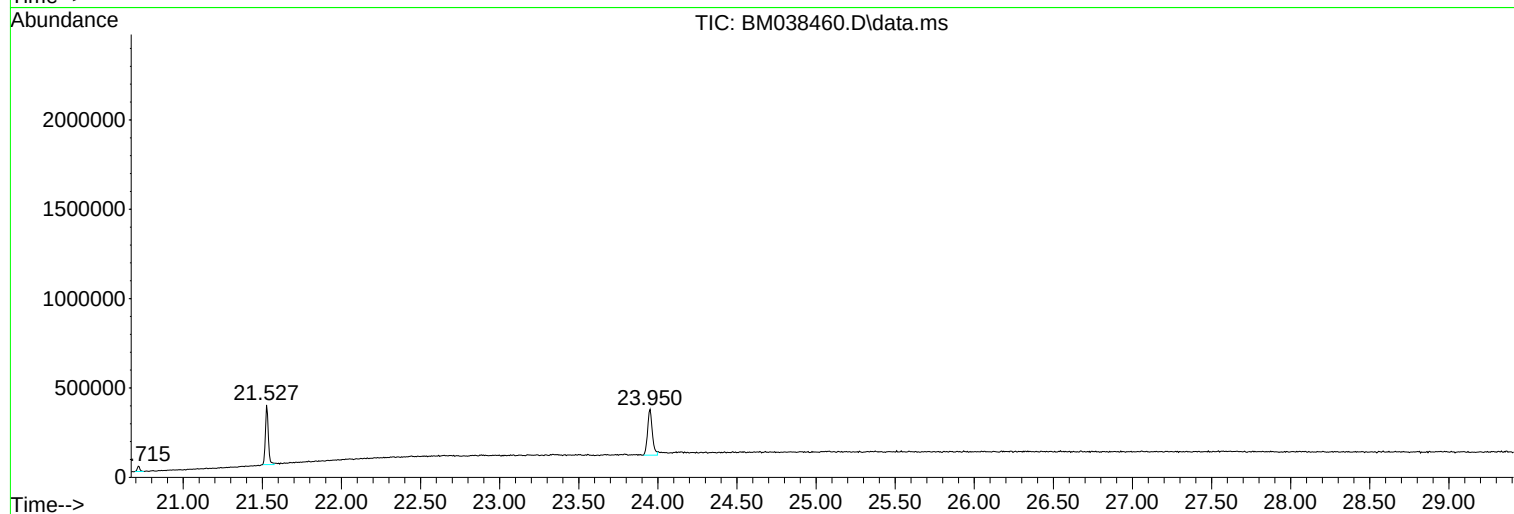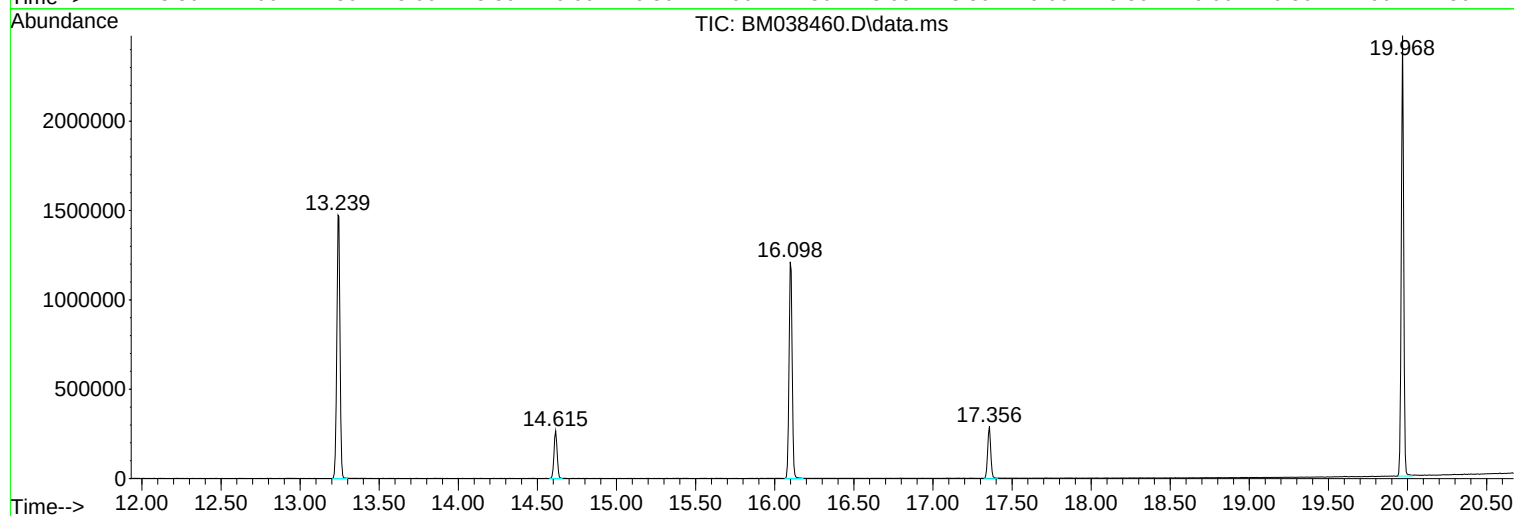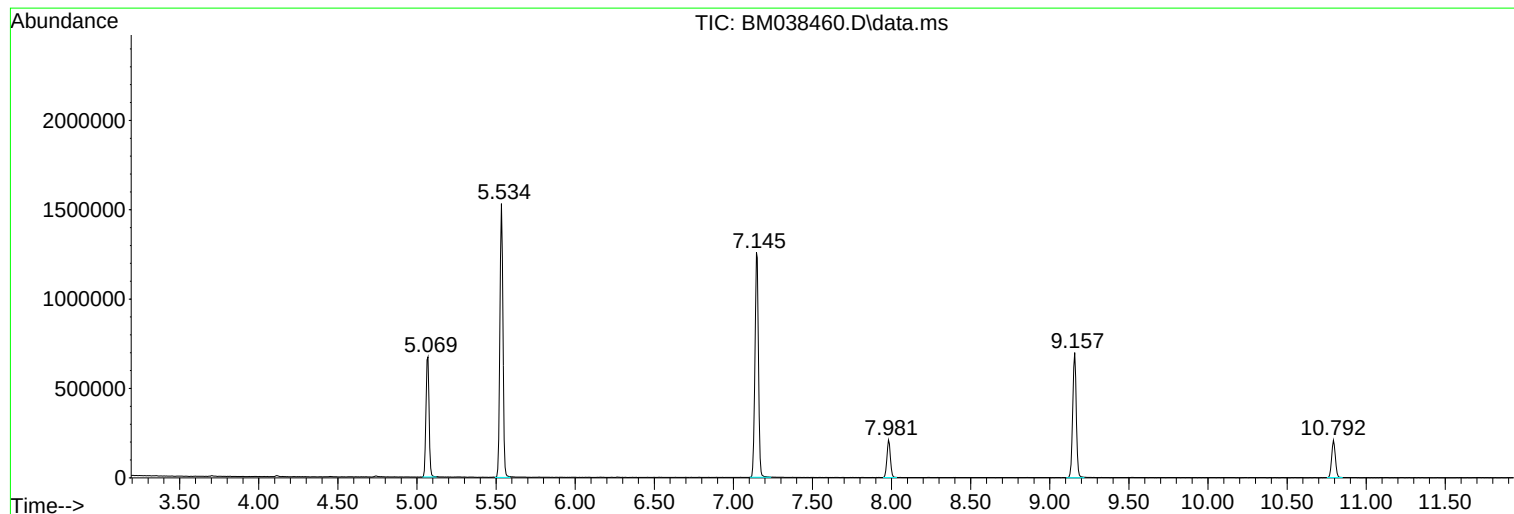

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011623\
Data File : BM038460.D
Acq On : 16 Jan 2023 19:58
Operator : CG/JU
Sample : PB150096BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150096BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.069	57.58 ng	917247	1,4-Dichlorobenzene-d4	7.981

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
3	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	23		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		

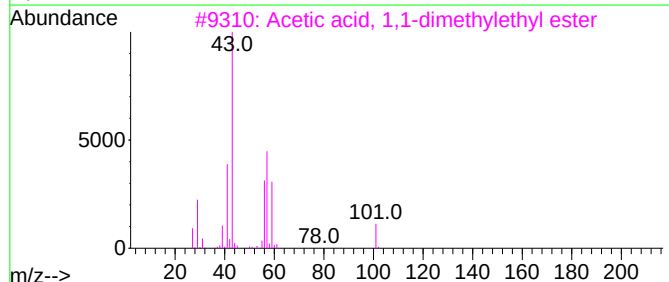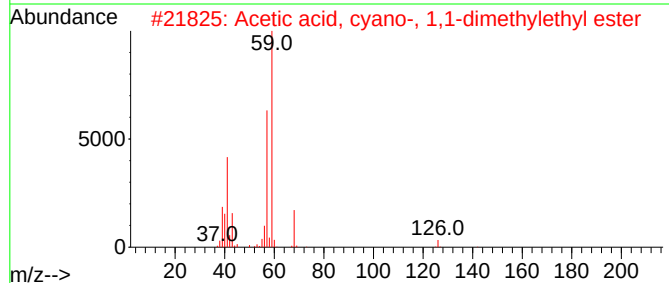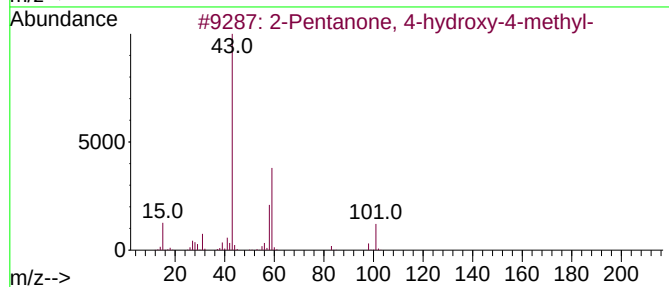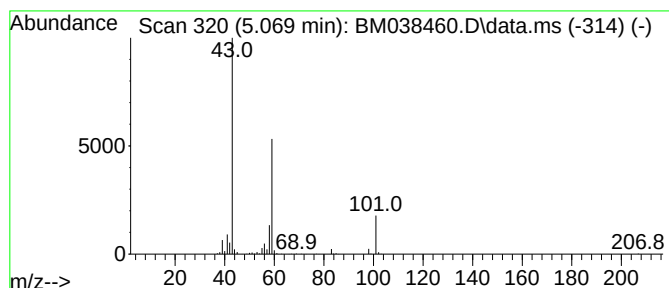

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011623\
Data File : BM038460.D
Acq On : 16 Jan 2023 19:58
Operator : CG/JU
Sample : PB150096BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150096BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.069	57.6	ng	917247	1	7.981	318594	20.0